


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022721\
 Data File : BM028912.D
 Acq On : 26 Feb 2021 10:06
 Operator : CG/JU
 Sample : DFTPP37
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP37

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION
 Last Update : Fri Feb 26 15:22:35 2021

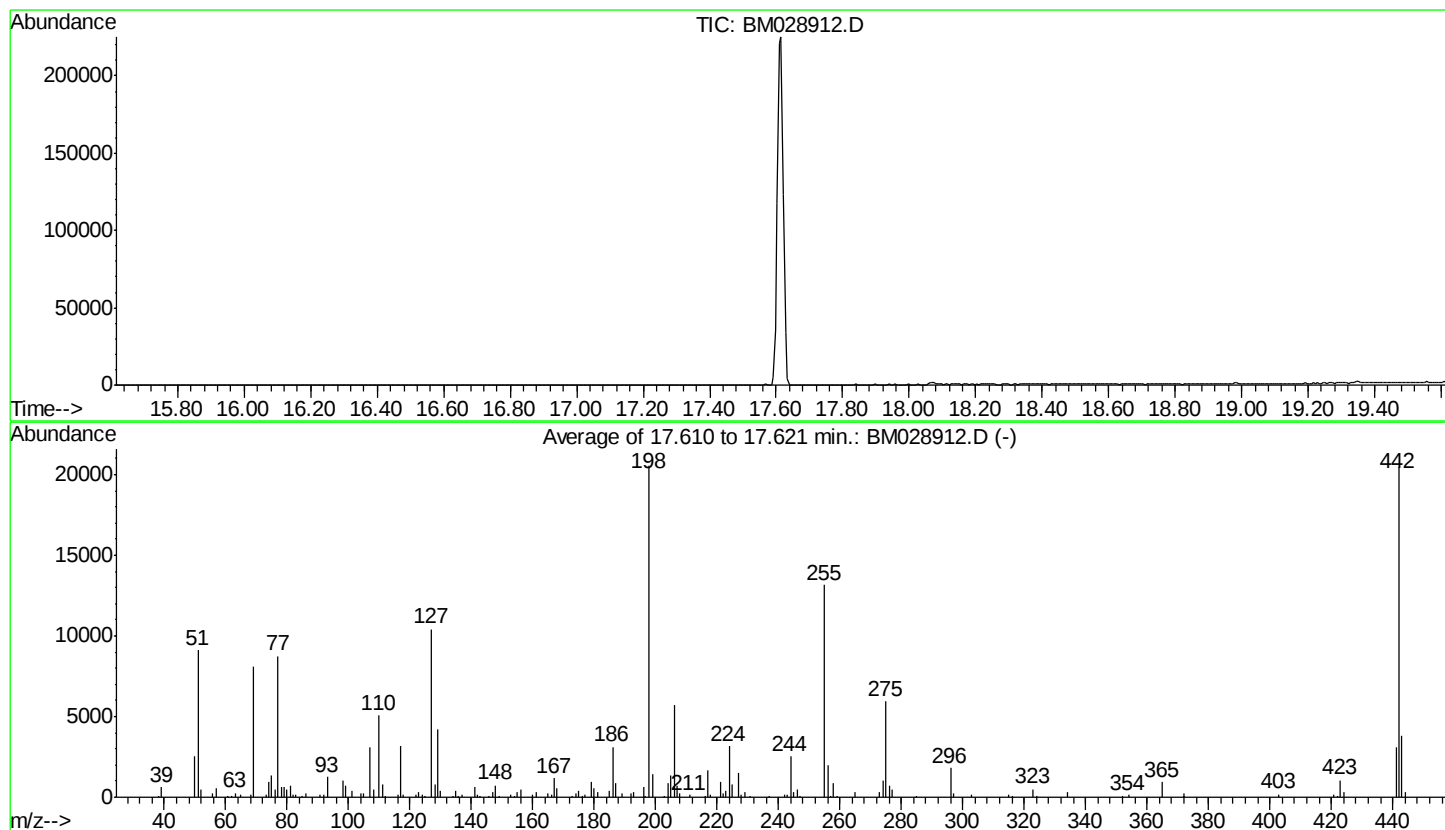

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	9110	PASS
68	69	0.00	2	1.9	150	PASS
69	198	0.00	100	39.3	8079	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.6	10409	PASS
197	198	0.00	2	0.3	61	PASS
198	198	100	100	100.0	20554	PASS
199	198	5	9	7.0	1435	PASS
275	198	10	60	28.9	5949	PASS
365	198	1	100	4.5	923	PASS
441	198	0.01	100	15.2	3129	PASS
442	198	50	100	99.4	20437	PASS
443	442	15	24	18.8	3835	PASS

Scan 2481 (17.580 min): BM028912.D
DFTPP37

m/z	Abundance
43.90	180.0
207.00	206.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

m/z	Abundance
38.00	155.0
39.00	856.0
50.00	3339.0
51.10	11920.0
52.00	611.0
55.90	378.0
57.00	665.0
60.90	153.0
61.90	160.0
63.00	454.0
65.00	216.0
68.00	203.0
69.00	10574.0
72.90	179.0
74.00	1230.0
75.00	1783.0
76.10	615.0
77.00	11331.0
78.00	782.0
79.00	827.0
79.90	674.0
81.00	934.0
81.90	250.0
82.90	210.0
86.00	319.0
90.90	228.0
92.00	236.0
93.00	1572.0
98.00	1271.0
99.00	892.0
101.00	523.0
104.00	354.0
105.00	347.0
107.00	3917.0
108.00	561.0
110.00	6358.0
111.00	1064.0
112.00	153.0
116.00	202.0
117.00	3954.0
117.90	260.0
121.90	269.0
123.00	413.0
124.00	181.0
124.90	162.0
127.00	12642.0
128.00	1005.0
129.00	5443.0
130.00	417.0
134.00	180.0
135.00	441.0
137.00	212.0
141.00	738.0
141.90	252.0
142.90	158.0
145.90	181.0
146.90	362.0
148.00	869.0
153.00	221.0
154.00	164.0
155.00	376.0
156.00	691.0
160.00	179.0
161.00	373.0
164.90	320.0
166.00	175.0
167.00	1477.0
168.00	734.0
172.90	209.0
173.90	260.0
175.00	525.0
176.00	167.0
177.00	298.0
179.00	1167.0
179.90	693.0
181.00	372.0
185.00	445.0
186.00	3633.0
187.00	941.0
188.90	288.0
192.00	340.0
193.00	385.0
196.00	762.0
196.70	184.0
198.00	23440.0
198.90	1730.0
202.90	158.0
204.00	1017.0
205.00	1572.0
206.00	6448.0
207.00	1084.0
208.00	256.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

210.90	207.0
217.00	2007.0
217.90	197.0
221.00	1171.0
221.90	223.0
223.00	478.0
224.00	3606.0
225.00	940.0
227.00	1693.0
227.90	234.0
228.90	338.0
237.00	153.0
242.00	200.0
243.00	216.0
244.00	2761.0
245.10	349.0
246.00	653.0
246.90	178.0
255.00	14480.0
256.00	2071.0
257.00	178.0
258.00	906.0
264.90	365.0
272.90	383.0
273.90	1094.0
275.00	6348.0
276.00	832.0
276.90	533.0
296.00	1909.0
296.90	274.0
302.90	244.0
314.90	218.0
323.00	537.0
333.90	380.0
353.90	201.0
364.90	894.0
371.90	297.0
402.90	197.0
421.00	150.0
423.00	1040.0
424.00	308.0
441.00	2858.0
442.00	18536.0
443.00	3762.0
444.00	319.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

m/z	Abundance
39.10	729.0
50.00	2965.0
51.10	10349.0
52.00	586.0
55.90	292.0
56.90	628.0
63.00	383.0
65.00	159.0
68.00	248.0
69.00	9157.0
73.00	169.0
74.00	1020.0
75.00	1591.0
76.00	453.0
77.00	9919.0
78.00	732.0
79.00	732.0
79.90	563.0
81.00	755.0
82.00	204.0
82.90	163.0
84.90	157.0
86.00	289.0
90.90	229.0
91.90	186.0
93.00	1445.0
98.00	1306.0
99.00	924.0
100.90	410.0
103.90	330.0
104.90	276.0
107.00	3557.0
108.00	532.0
110.00	5904.0
111.00	881.0
115.90	208.0
117.00	3740.0
117.90	229.0
121.90	286.0
122.90	400.0
123.90	218.0
124.90	173.0
127.00	12178.0
128.00	1025.0
129.00	4702.0
129.90	494.0
134.90	453.0
135.90	198.0
137.00	221.0
141.00	744.0
142.00	194.0
147.00	368.0
147.90	924.0
149.00	181.0
152.90	234.0
155.00	403.0
156.00	564.0
159.90	208.0
161.00	373.0
165.00	300.0
166.00	192.0
167.00	1350.0
168.00	620.0
174.00	308.0
175.00	520.0
176.90	225.0
178.90	1086.0
180.00	658.0
180.90	300.0
184.90	446.0
186.00	3736.0
187.00	1117.0
189.00	209.0
192.00	269.0
192.90	403.0
195.90	784.0
197.90	24544.0
199.00	1758.0
203.00	169.0
204.00	958.0
205.00	1558.0
206.00	6800.0
207.00	1126.0
207.90	371.0
211.00	252.0
216.00	154.0
216.90	1866.0
218.00	199.0
221.00	1076.0
221.90	236.0
223.00	450.0
224.00	3826.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

225.00	948.0
227.00	1760.0
227.90	231.0
229.00	306.0
230.90	175.0
236.90	158.0
242.00	198.0
243.00	243.0
244.00	3010.0
245.00	417.0
246.00	629.0
255.00	15622.0
256.00	2405.0
257.00	182.0
258.00	1080.0
259.00	185.0
265.00	440.0
272.90	409.0
274.00	1268.0
275.00	7295.0
276.00	896.0
276.90	581.0
285.00	152.0
296.00	2187.0
296.90	300.0
303.00	222.0
314.90	199.0
316.00	154.0
323.00	596.0
323.90	171.0
334.00	374.0
351.90	187.0
354.00	212.0
365.00	1155.0
372.10	377.0
402.90	210.0
420.90	246.0
422.00	190.0
423.00	1247.0
423.90	298.0
441.00	3807.0
442.00	24624.0
443.00	4538.0
443.90	426.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

m/z	Abundance
39.00	310.0
50.00	1419.0
51.00	5062.0
52.00	250.0
56.90	310.0
69.00	4507.0
73.10	152.0
74.00	536.0
74.90	755.0
76.00	255.0
77.10	5032.0
78.00	319.0
78.90	388.0
80.00	277.0
81.00	403.0
85.90	151.0
92.90	709.0
97.90	644.0
99.00	420.0
101.00	193.0
104.00	158.0
104.90	172.0
107.00	1735.0
108.00	247.0
110.00	2940.0
110.90	429.0
117.00	1753.0
122.90	189.0
127.00	6407.0
128.00	345.0
129.00	2411.0
129.90	284.0
135.00	229.0
140.90	343.0
146.90	193.0
147.90	456.0
154.90	170.0
156.00	297.0
159.90	154.0
161.00	176.0
164.90	155.0
167.00	722.0
168.00	324.0
173.90	167.0
175.00	266.0
179.00	549.0
179.90	413.0
181.00	216.0
185.00	296.0
186.00	1921.0
187.00	560.0
188.90	173.0
192.00	152.0
192.90	209.0
196.00	381.0
197.90	13679.0
199.00	817.0
204.00	574.0
205.00	1003.0
206.00	3824.0
207.00	612.0
208.00	157.0
217.00	1109.0
221.00	580.0
221.90	169.0
223.00	334.0
224.00	2039.0
225.00	530.0
227.00	1013.0
228.90	212.0
244.00	1752.0
244.90	192.0
246.00	254.0
255.00	9323.0
256.00	1390.0
258.00	589.0
264.90	216.0
273.00	277.0
273.90	754.0
275.00	4206.0
276.00	533.0
277.00	393.0
296.00	1370.0
297.00	169.0
323.00	387.0
333.90	278.0
352.00	175.0
364.90	720.0
372.00	269.0
403.00	174.0
423.00	928.0
423.90	273.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37

441.00	2724.0
442.00	18152.0
443.00	3205.0
443.90	252.0

Instrument :
BNA_M
ClientSampleId :
DFTPP37