
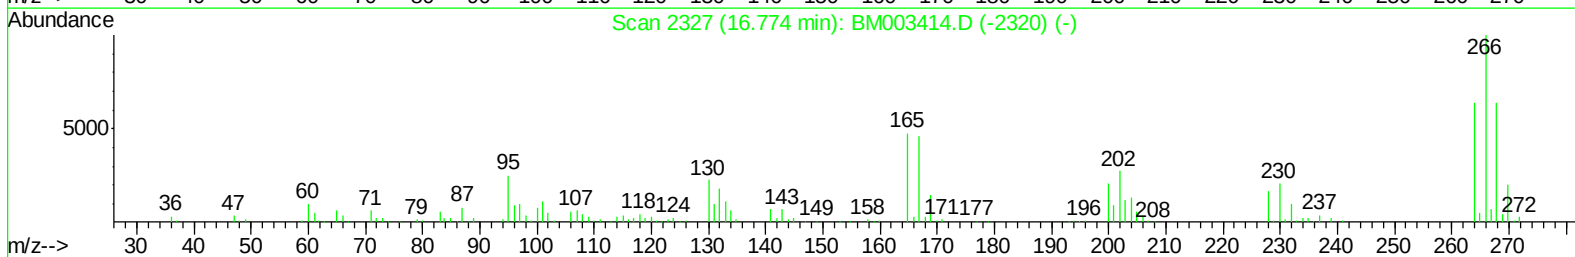
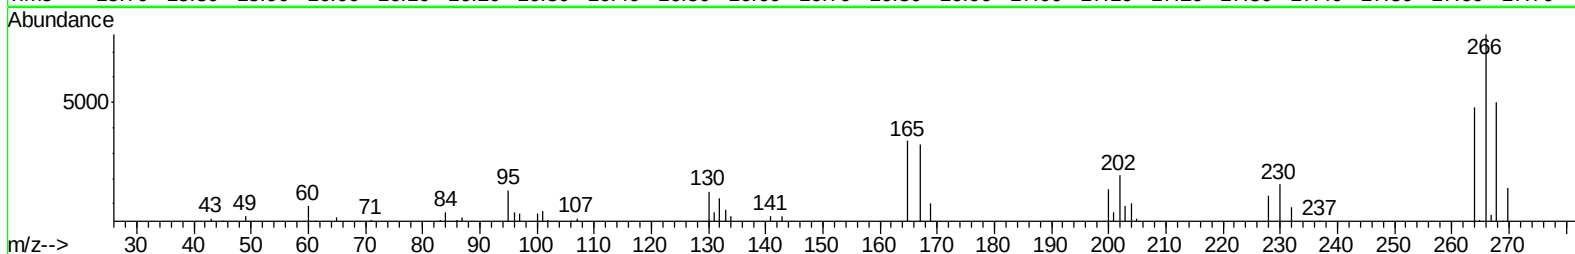


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022816\
Data File : BM004451.D
Acq On : 28 Feb 2016 15:29
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 07:45:12 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

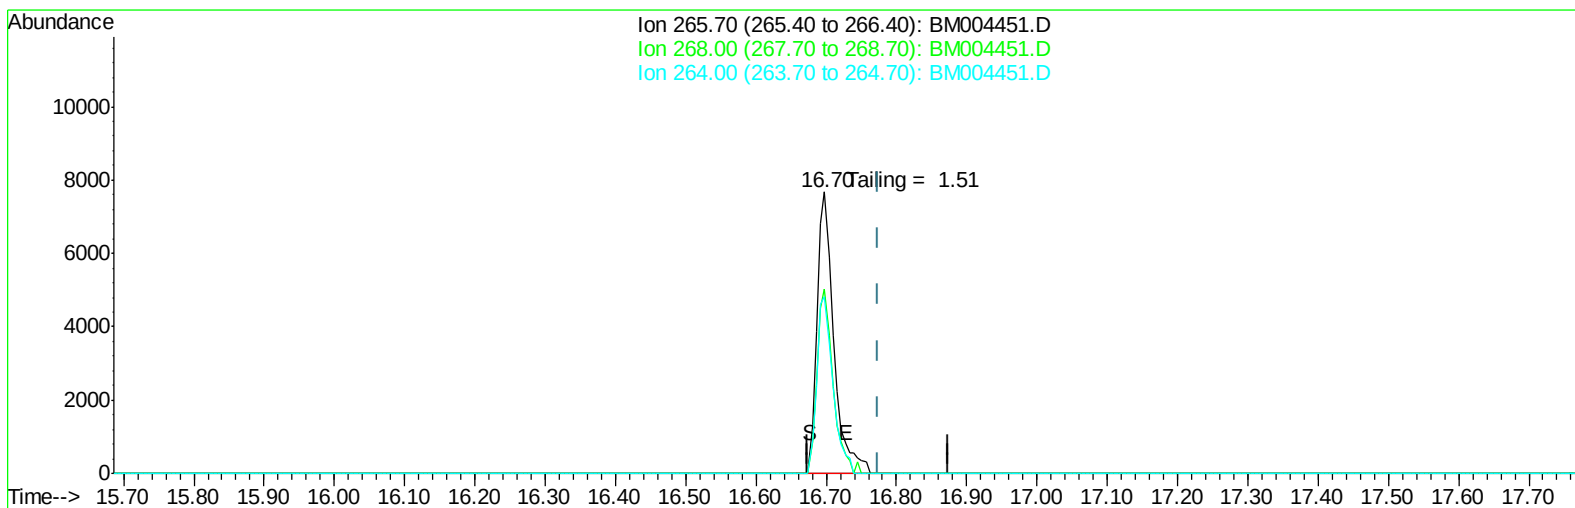

TIC: BM004451.D

(69) Pentachlorophenol (C)




16.698min (-0.076) 0.00ng

response 10789

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	65.44
264.00	61.20	62.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022816\
Data File : BM004451.D
Acq On : 28 Feb 2016 15:29
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 07:45:12 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

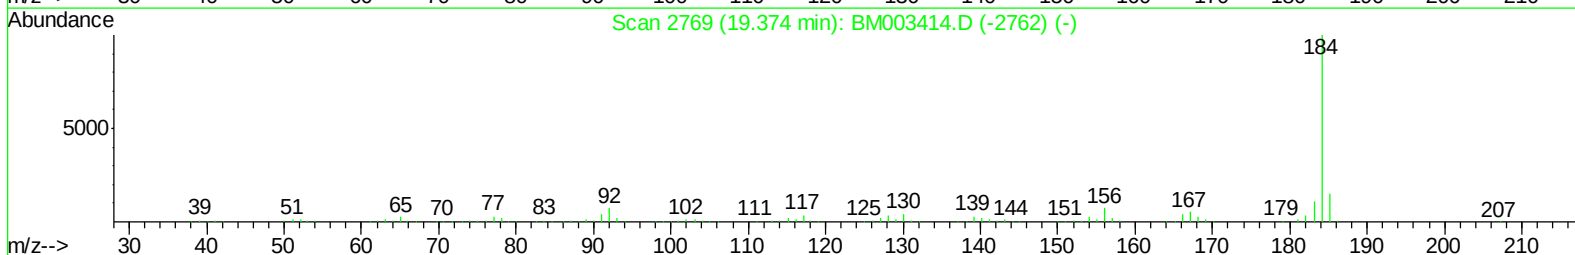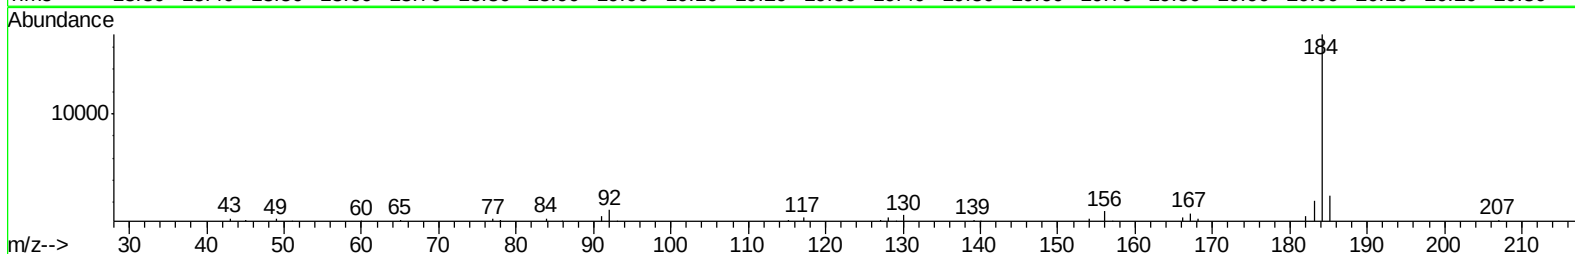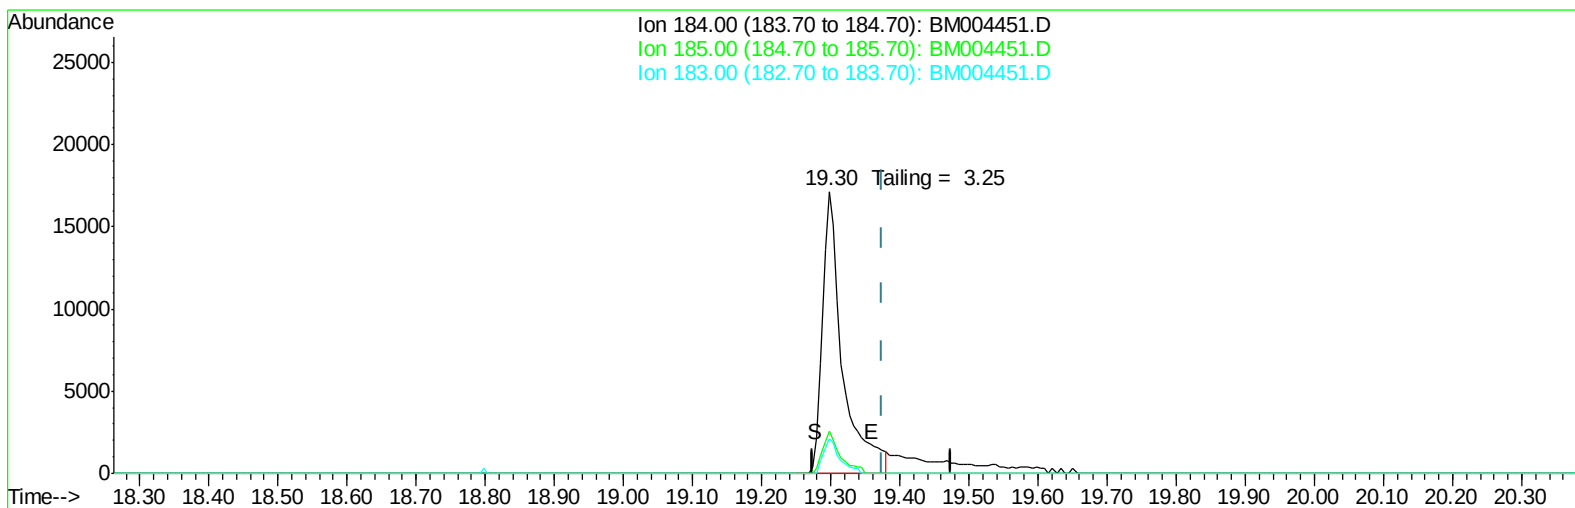

TIC: BM004451.D

(76) Benzidine

19.298min (-0.076) 365.55ng m

response 34500

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	15.02
183.00	11.10	12.49
0.00	0.00	0.00