
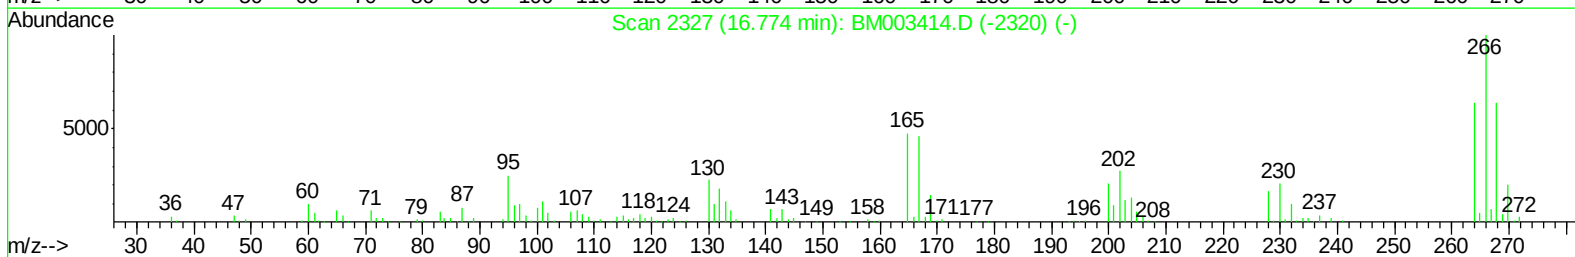
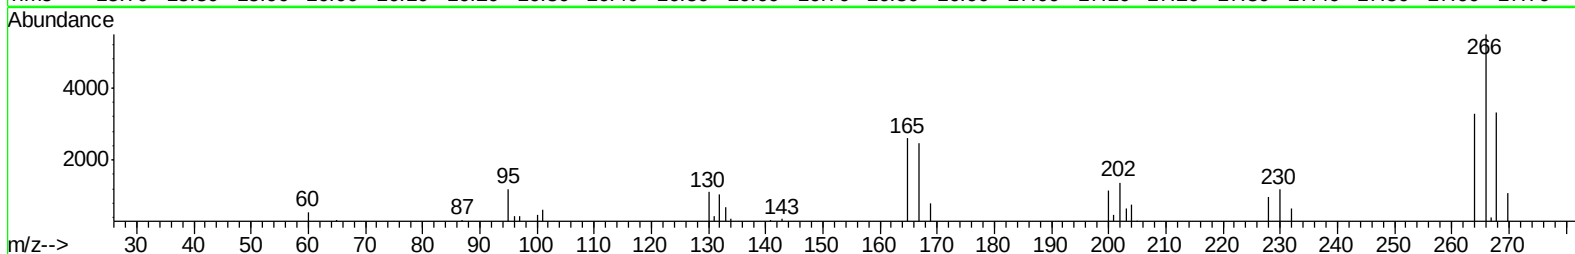


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022816\
Data File : BM004461.D
Acq On : 28 Feb 2016 22:45
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 07:46:02 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

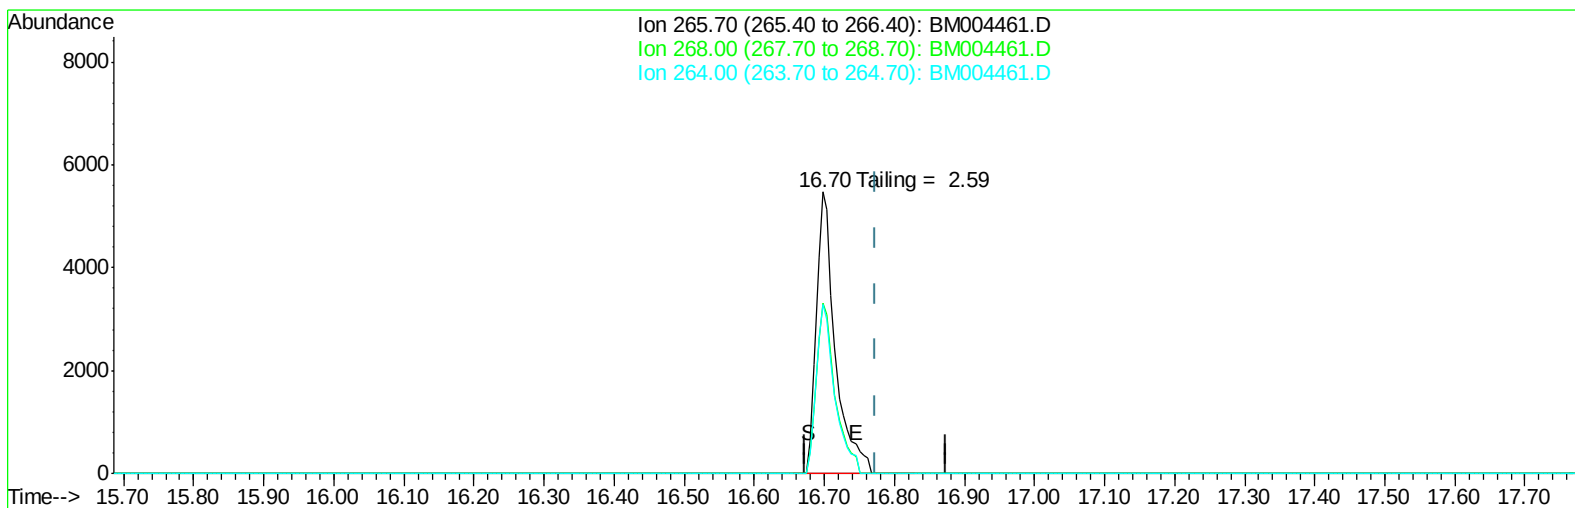

TIC: BM004461.D

(69) Pentachlorophenol (C)




16.698min (-0.076) 0.00ng

response 9313

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	60.58
264.00	61.20	60.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022816\
Data File : BM004461.D
Acq On : 28 Feb 2016 22:45
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 29 07:46:02 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

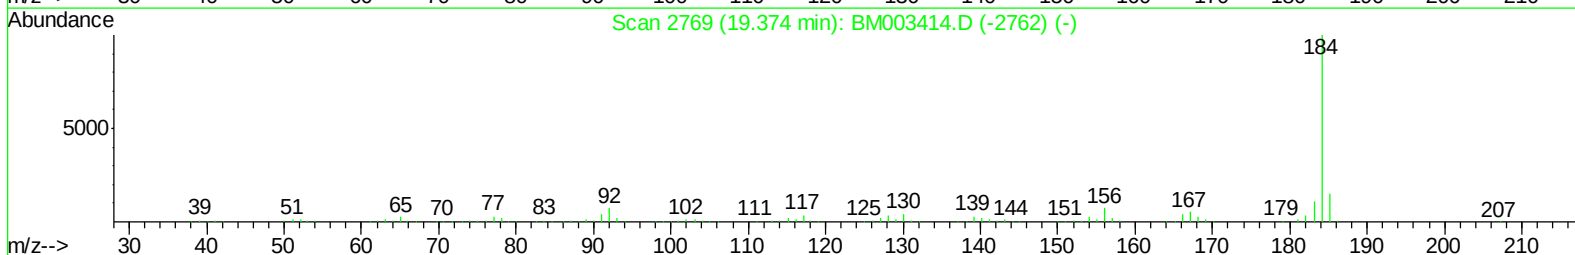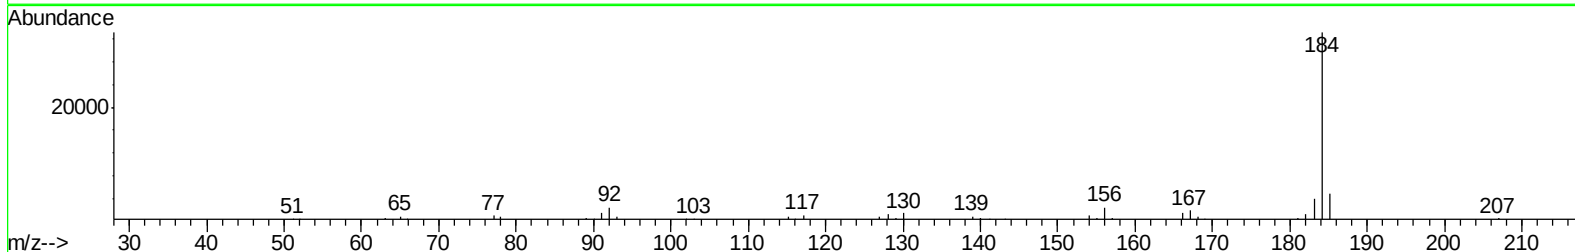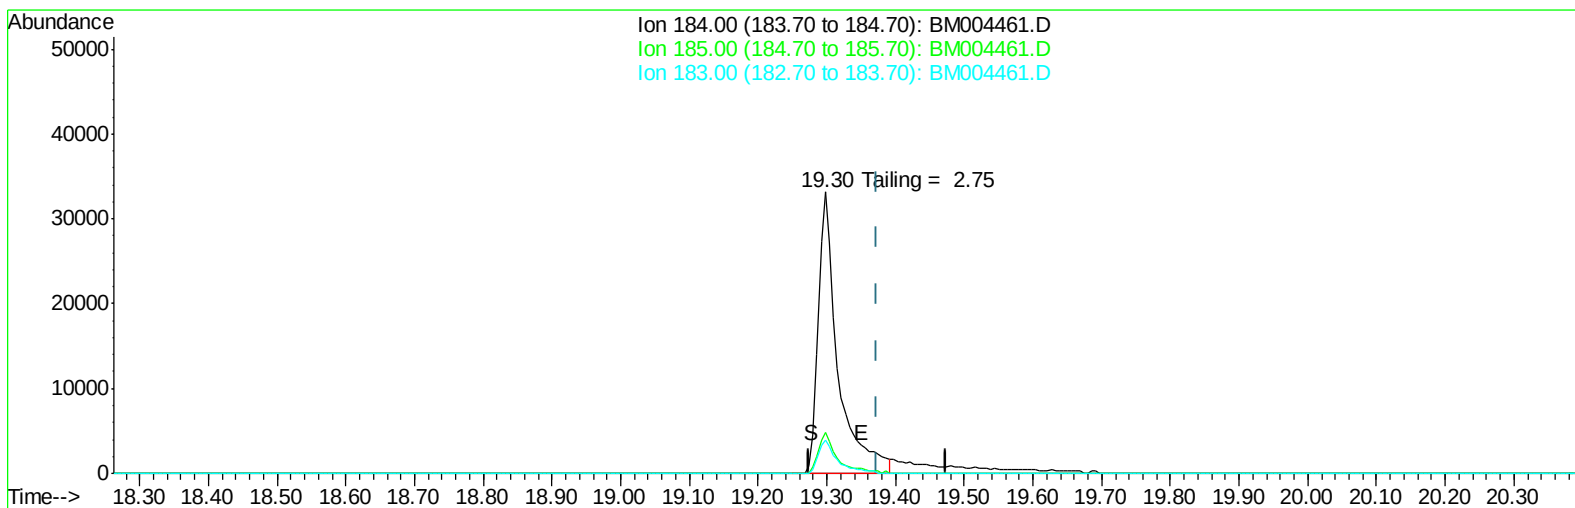

TIC: BM004461.D

(76) Benzidine

19.298min (-0.076) 5674.73ng

response 65992

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.54
183.00	11.10	11.86
0.00	0.00	0.00