


Data Path : Z:\HPCHEM1\BNA M\Data\BM022816\
 Data File : BM004451.D
 Acq On : 28 Feb 2016 15:29
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM022816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 29 05:57:18 2016

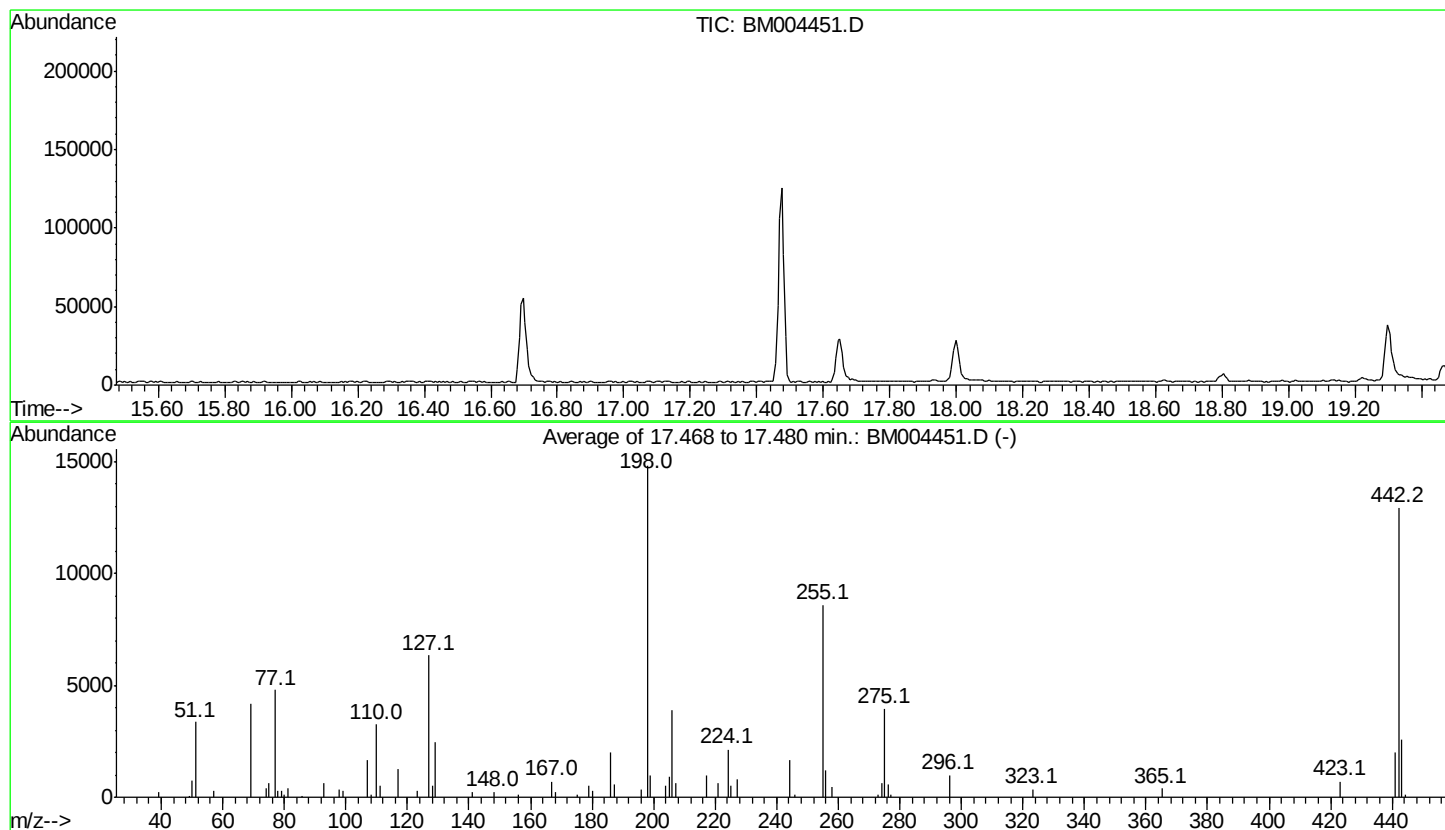

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.6	3350	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.1	4167	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.8	6333	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14808	PASS
199	198	5	9	6.8	1000	PASS
275	198	10	60	26.7	3959	PASS
365	198	1	100	2.6	389	PASS
441	442	0.01	24	15.4	1986	PASS
442	198	50	100	87.3	12927	PASS
443	442	15	24	20.0	2590	PASS