

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022818\
 Data File : BM014409.D
 Acq On : 28 Feb 2018 19:31
 Operator : SJ/JU
 Sample : J1679-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE602

Quant Time: Mar 01 00:47:28 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 01 00:47:00 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	62189	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	312011	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.17	164	207308	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.94	188	509699	20.00	ng/ul	0.00
75) Chrysene-d12	21.15	240	585882	20.00	ng/ul	0.00
83) Perylene-d12	23.33	264	628217	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.09	96	6263	4.31	ng/uL	0.00
5) Phenol-d5	6.72	99	158822	30.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	100051	31.45	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	132626	32.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	148654	32.32	ng/ul	0.00
19) Nitrobenzene-d5	8.67	128	74713	32.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.39	143	83546	35.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.93	165	135644	27.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.45	131	192468	39.52	ng/ul	0.00
43) Dimethylphthalate-d6	13.60	166	608309	35.53	ng/ul	0.00
46) Acenaphthylene-d8	13.86	160	721575	34.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	63232	26.75	ng/ul	0.00
57) Fluorene-d10	15.18	176	511286	33.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.34	200	66698	21.81	ng/ul	0.00
70) Anthracene-d10	17.04	188	842441	34.26	ng/ul	0.00
76) Pyrene-d10	19.34	212	975877	32.29	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.19	264	1033812	33.81	ng/ul	0.00
Target Compounds						
15) N-Nitroso-di-n-propylamine	8.25	70	5636	1.417	ng/ul#	1
44) Dimethylphthalate	13.65	163	93978	5.567	ng/ul#	93




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022818\
Data File : BM014409.D
Acq On : 28 Feb 2018 19:31
Operator : SJ/JU
Sample : J1679-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE602

Quant Time: Mar 01 00:47:28 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 01 00:47:00 2018
Response via : Initial Calibration

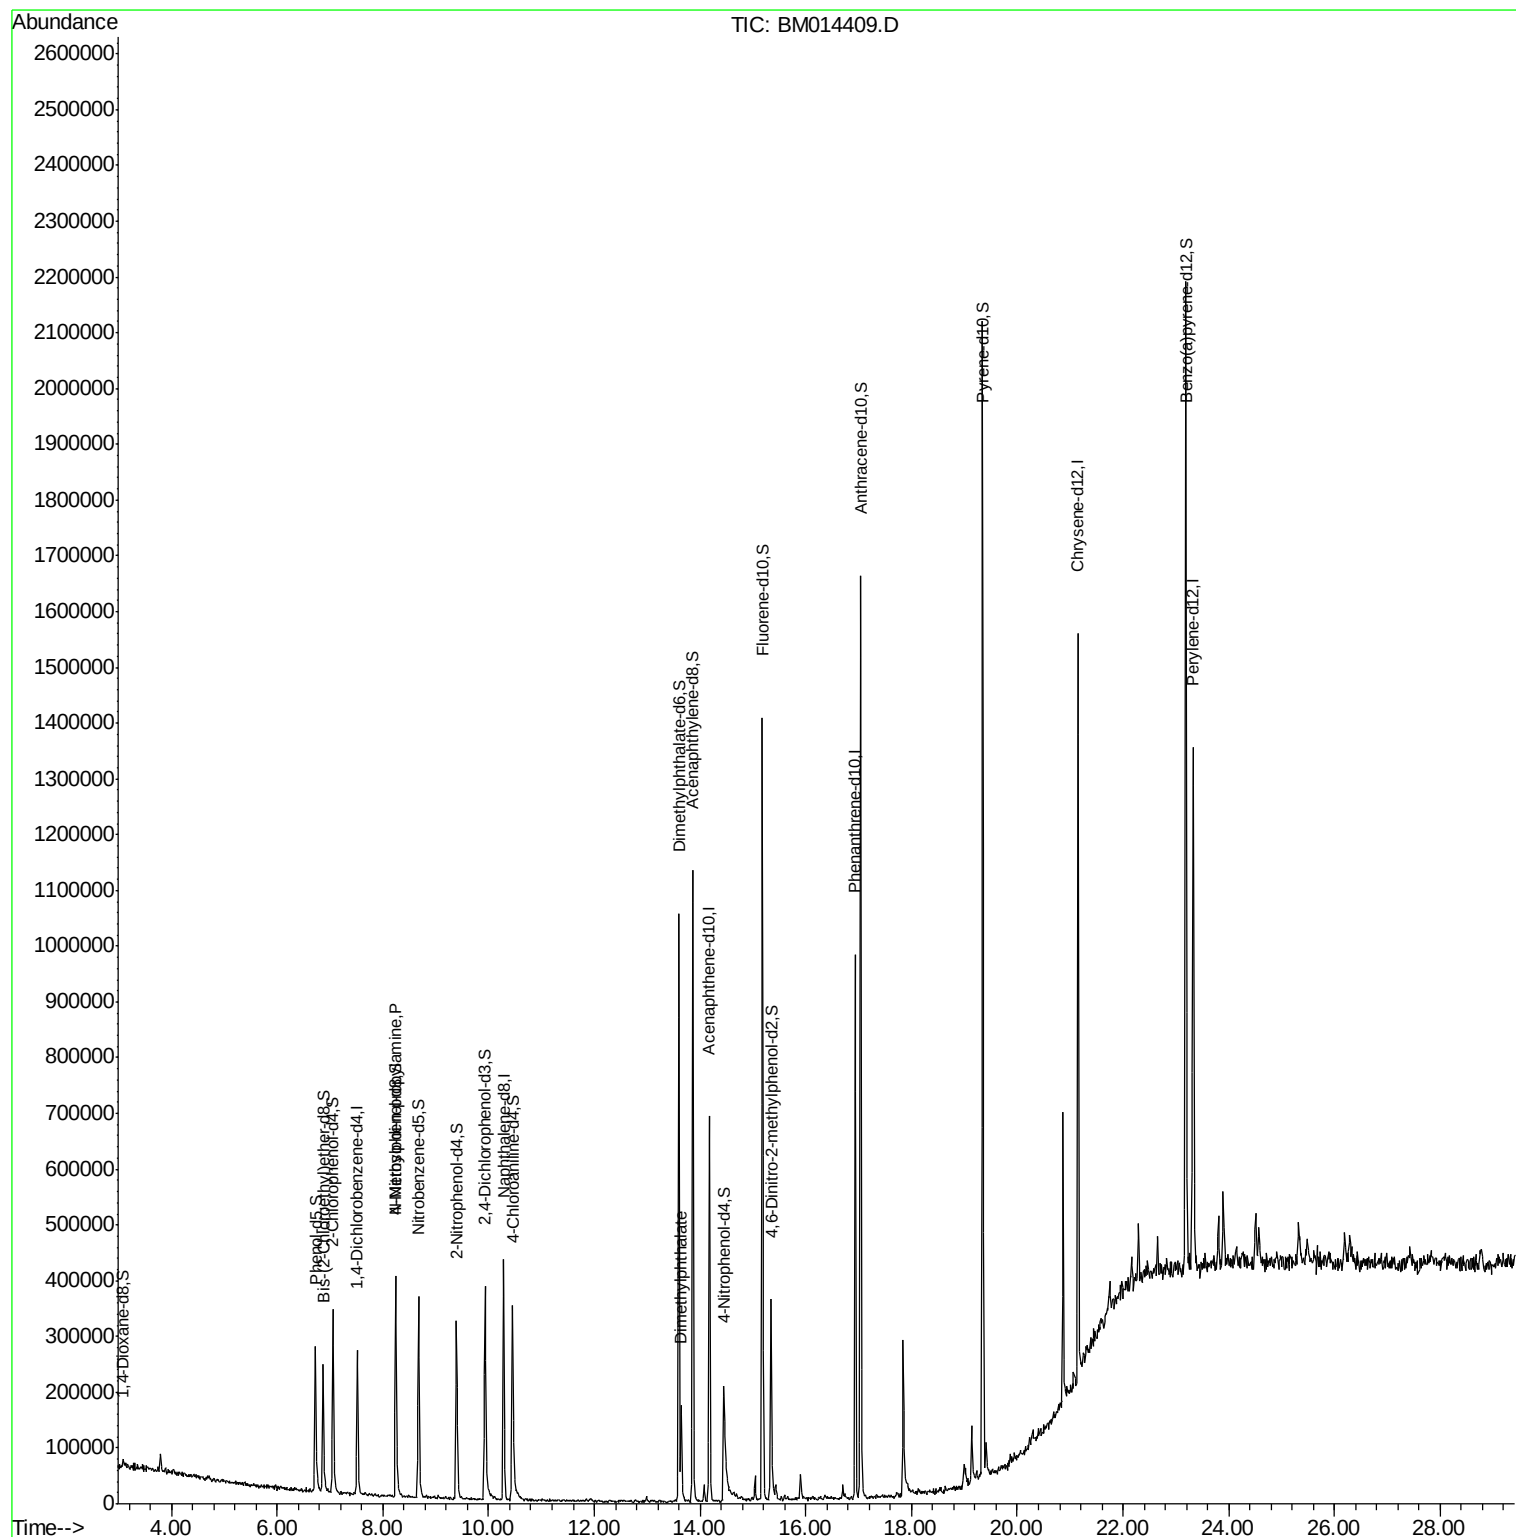

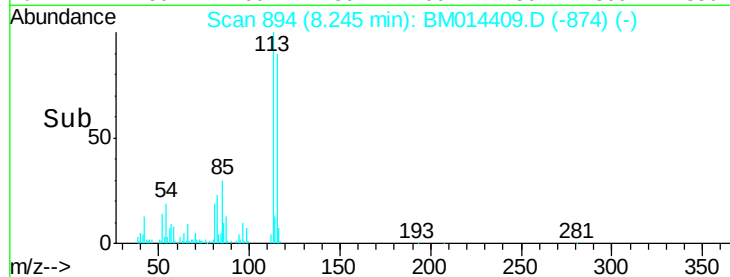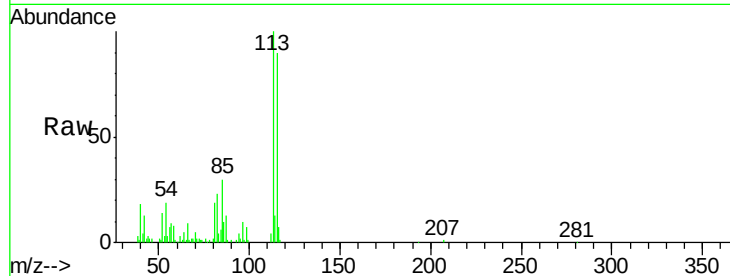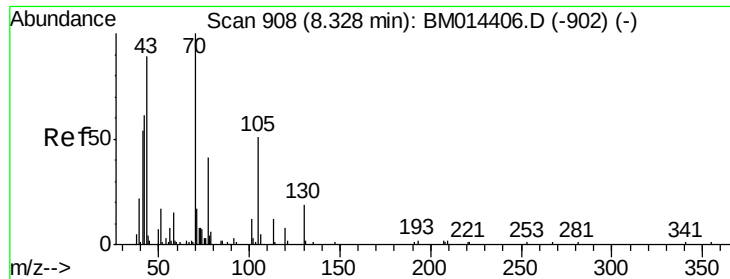

#15

N-Nitroso-di-n-propylamine

Concen: 1.417 ng/ul

RT: 8.25 min Scan# 894

Delta R.T. -0.08 min

Lab File: BM014409.D

Acq: 28 Feb 2018 19:31

Instrument :

BNA_M

ClientSampleId :

BE602

Tot Ion: 70 Resp: 5636





Ion Ratio Lower Upper

70 100

42 267.5 76.0 114.0#

101 0.0 6.7 10.1#

130 0.0 14.6 22.0#

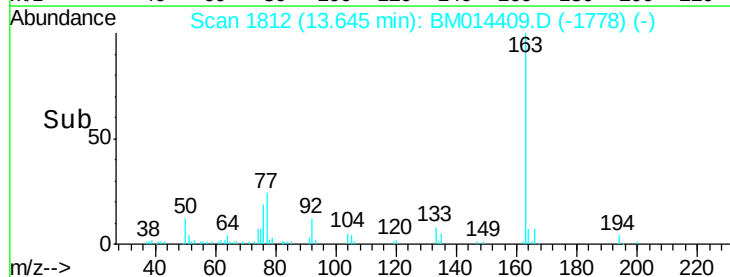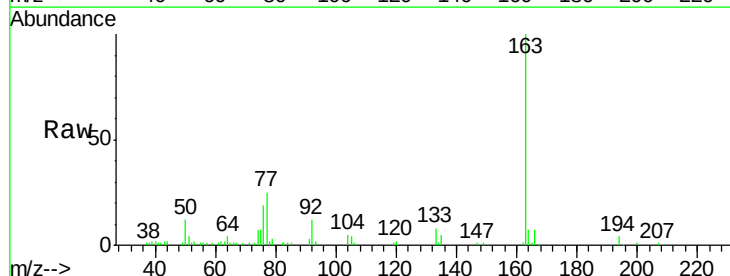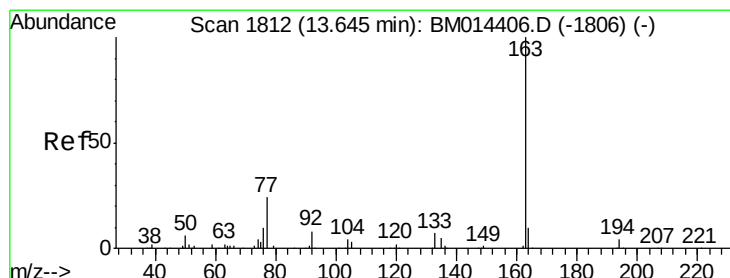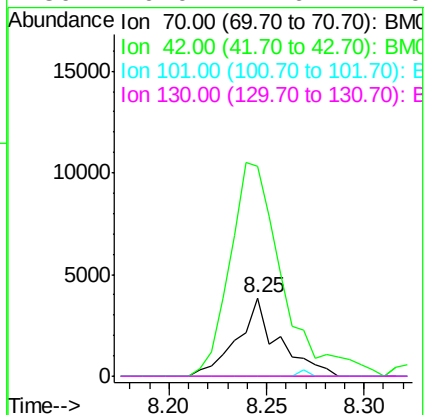

#44

Dimethylphthalate

Concen: 5.567 ng/ul

RT: 13.65 min Scan# 1812

Delta R.T. -0.00 min

Lab File: BM014409.D

Acq: 28 Feb 2018 19:31

Tgt Ion: 163 Resp: 93978

Ion Ratio Lower Upper

163 100

194 3.6 3.5 5.3

164 7.1 8.2 12.4#

