

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022819\
 Data File : BM018975.D
 Acq On : 28 Feb 2019 18:38
 Operator : JU/SJ
 Sample : K1638-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PE-5(BELOW-EXPOSED-PIPE)

Quant Time: Mar 01 01:14:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	242028	20.00	ng	-0.03
21) Naphthalene-d8	10.47	136	1059584	20.00	ng	-0.03
39) Acenaphthene-d10	14.34	164	612820	20.00	ng	-0.02
64) Phenanthrene-d10	17.09	188	1390514	20.00	ng	-0.02
76) Chrysene-d12	21.29	240	1338326	20.00	ng	-0.02
87) Perylene-d12	23.53	264	1190364	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	1327322	89.86	ng	-0.02
7) Phenol-d6	6.86	99	1956442	94.02	ng	-0.02
23) Nitrobenzene-d5	8.86	82	1254112	54.73	ng	-0.03
42) 2,4,6-Tribromophenol	15.84	330	763069	86.38	ng	-0.02
45) 2-Fluorobiphenyl	12.95	172	2383037	51.62	ng	-0.03
79) Terphenyl-d14	19.73	244	3695268	56.96	ng	-0.02
Target Compounds						
9) Benzaldehyde	6.86	77	5551	Below Cal	Qvalue #	7
50) Dimethylphthalate	13.80	163	129466	2.535 ng		99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022819\
Data File : BM018975.D
Acq On : 28 Feb 2019 18:38
Operator : JU/SJ
Sample : K1638-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PE-5(BELOW-EXPOSED-PIPE)

Quant Time: Mar 01 01:14:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

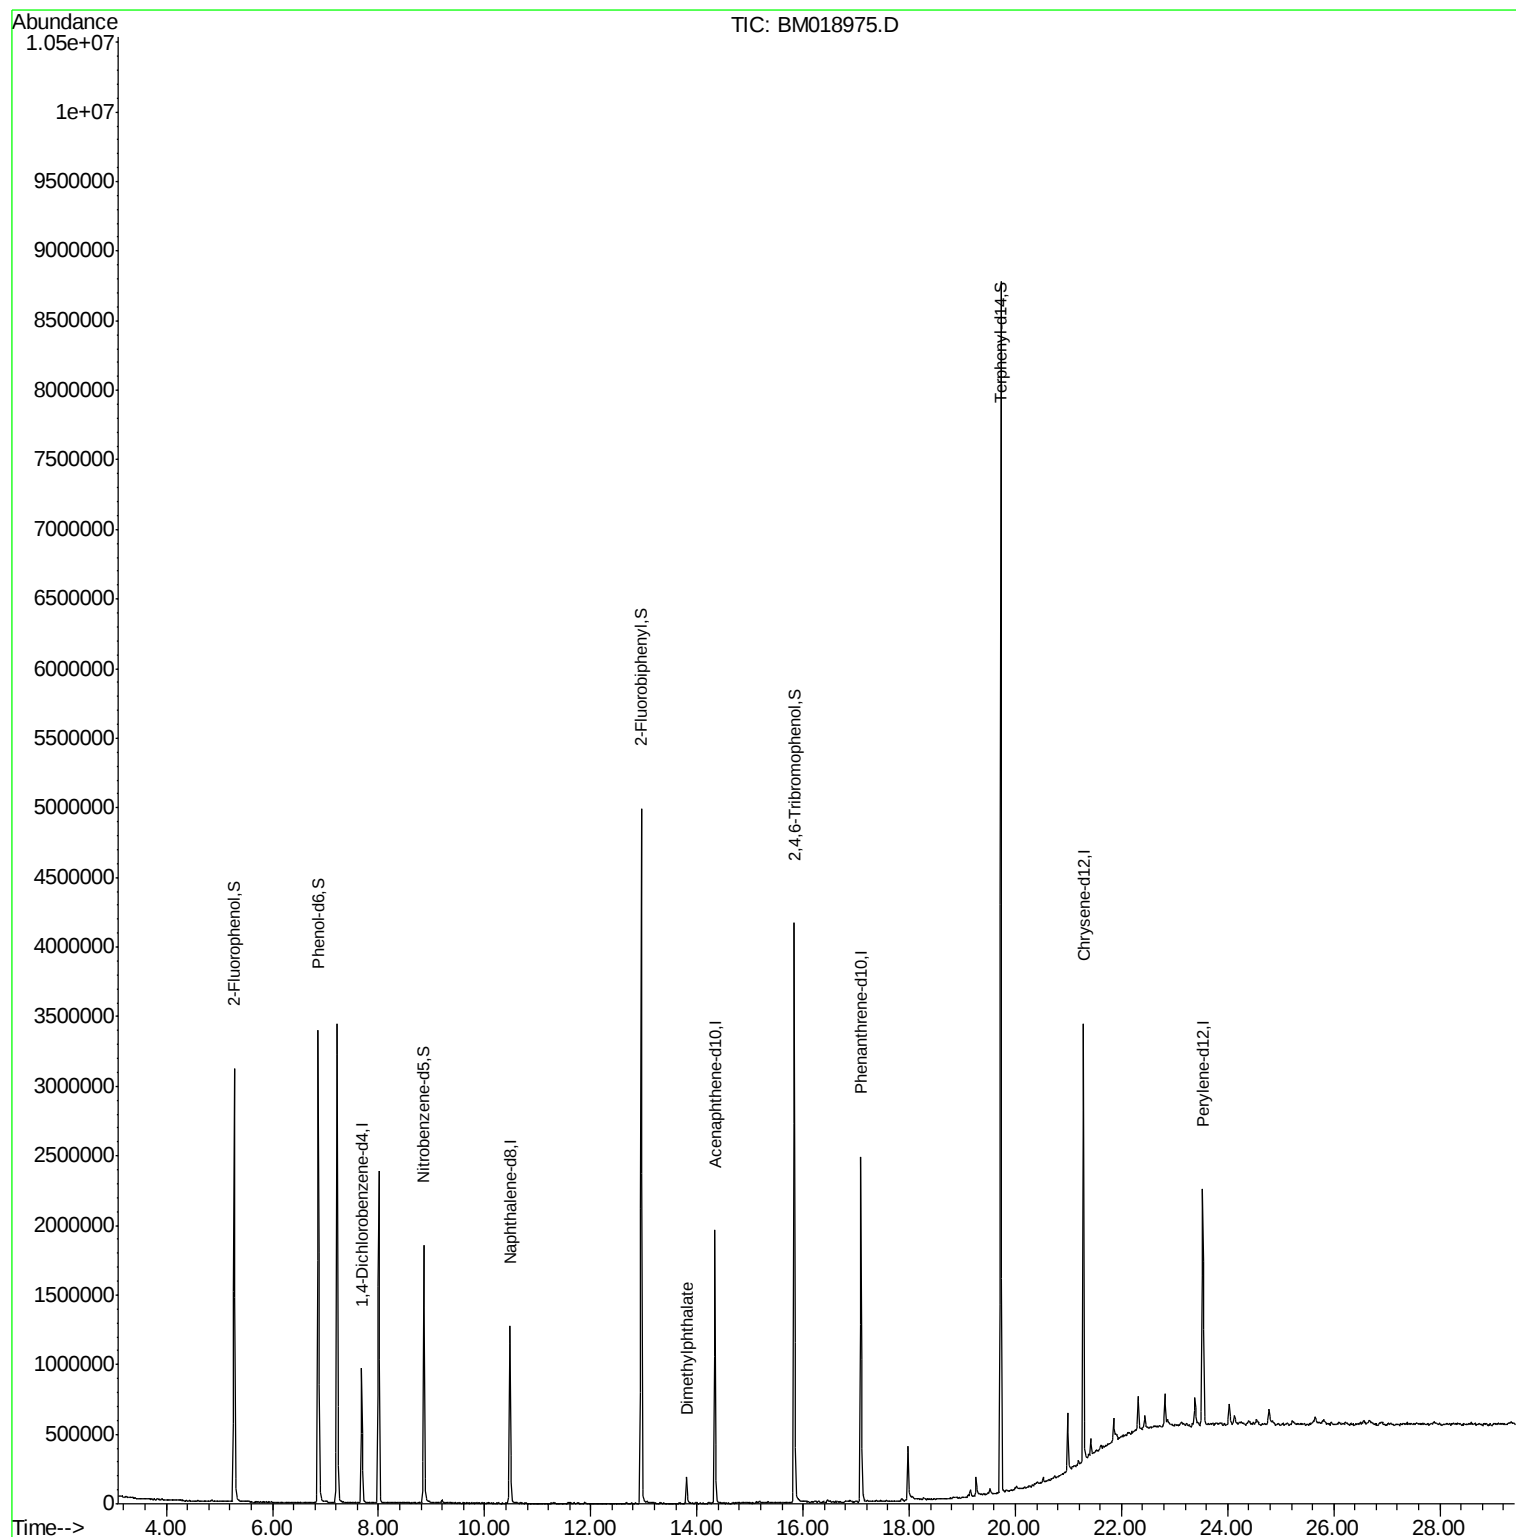




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.69 min Scan# 782
Delta R.T. -0.03 min
Lab File: BM018975.D
Acq: 28 Feb 2019 18:38

Instrument :
BNA_M
ClientSampleId :
PE-5(BELOW-EXPOSED-PIPE)

Tgt Ion:152 Resp: 242028
Ion Ratio Lower Upper
152 100
150 157.5 127.3 190.9
115 65.2 50.8 76.2

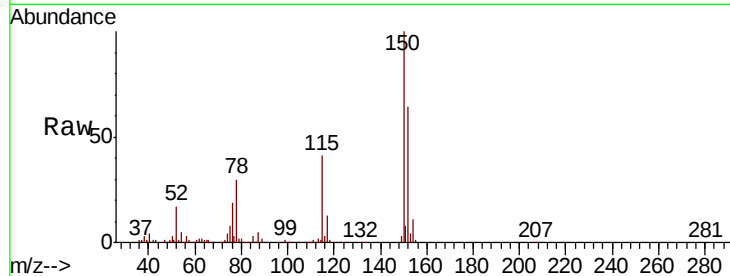


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

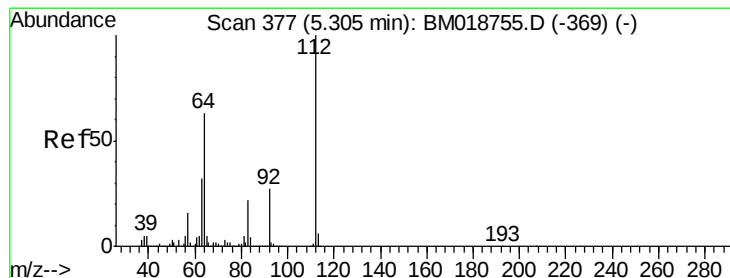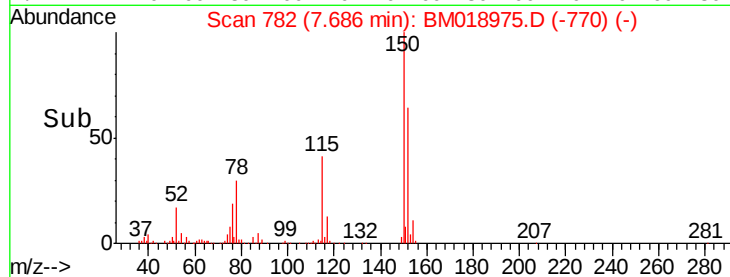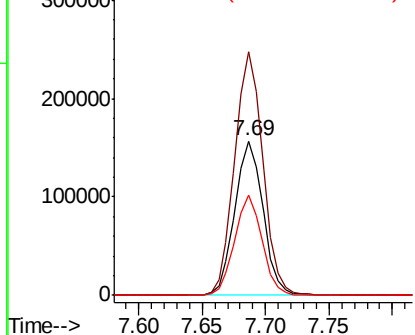



#5

2-Fluorophenol
Concen: 89.857 ng
RT: 5.28 min Scan# 373
Delta R.T. -0.02 min
Lab File: BM018975.D
Acq: 28 Feb 2019 18:38

Tgt Ion:112 Resp: 1327322
Ion Ratio Lower Upper
112 100
64 64.5 50.6 75.8
63 32.8 25.7 38.5

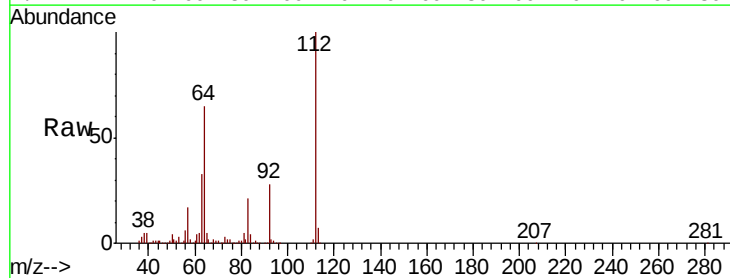

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

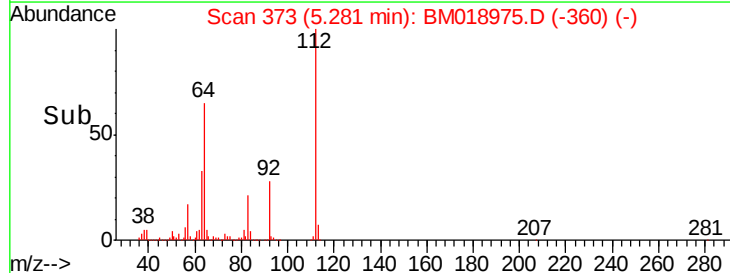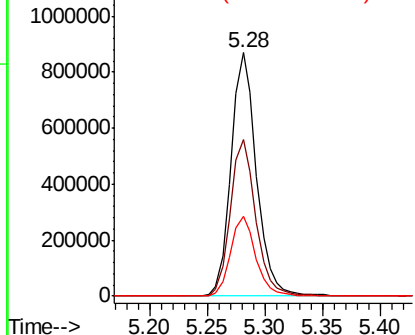



#7

Phenol-d6

Concen: 94.017 ng

RT: 6.86 min Scan# 642

Delta R.T. -0.02 min

Lab File: BM018975.D

Acq: 28 Feb 2019 18:38

Instrument :

BNA_M

ClientSampleId :

PE-5(BELOW-EXPOSED-PIPE)


Tgt Ion: 99 Resp: 1956442

Ion Ratio Lower Upper

99 100

42 13.9 11.0 16.6




71 38.0 31.3 46.9

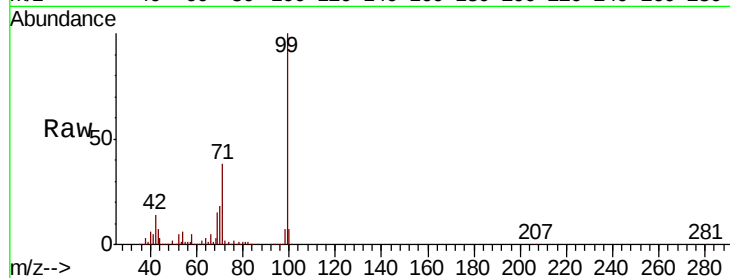

Abundance Ion 99.00 (98.70 to 99.70): BM018975.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018975.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018975.D (-637) (-)

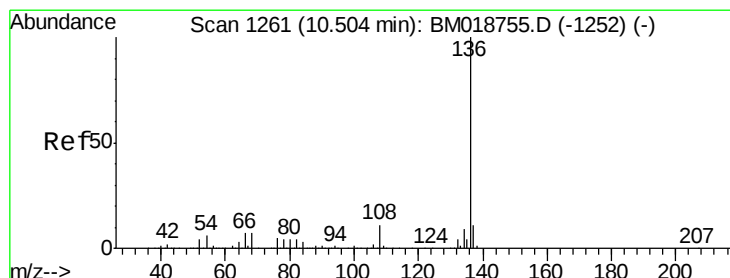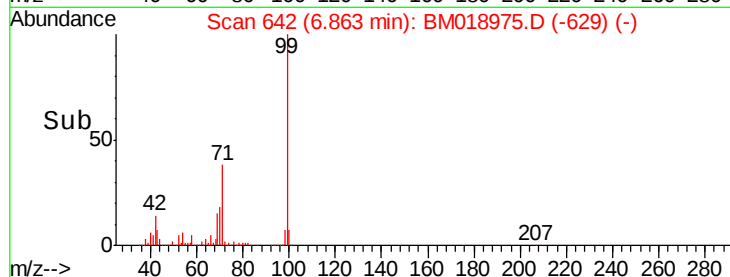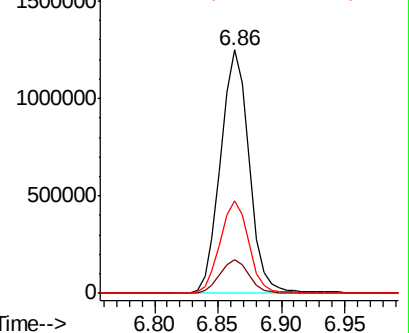

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.47 min Scan# 1256

Delta R.T. -0.03 min

Lab File: BM018975.D

Acq: 28 Feb 2019 18:38

Tgt Ion: 136 Resp: 1059584


Ion Ratio Lower Upper

136 100

137 10.8 8.8 13.2

54 6.7 5.0 7.6

68 7.3 5.5 8.3


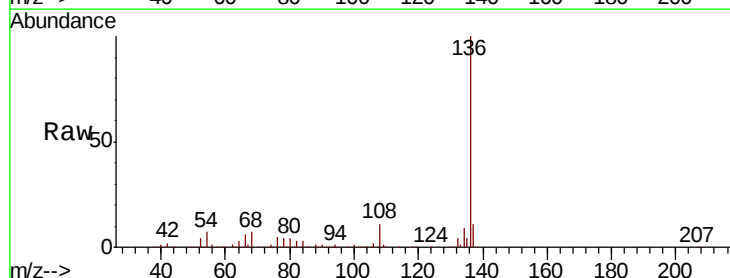



Abundance Ion 136.00 (135.70 to 136.70): BM018975.D (-1244) (-)

Ion 137.00 (136.70 to 137.70): BM018975.D (-1244) (-)

Ion 54.00 (53.70 to 54.70): BM018975.D (-1244) (-)

Ion 68.00 (67.70 to 68.70): BM018975.D (-1244) (-)



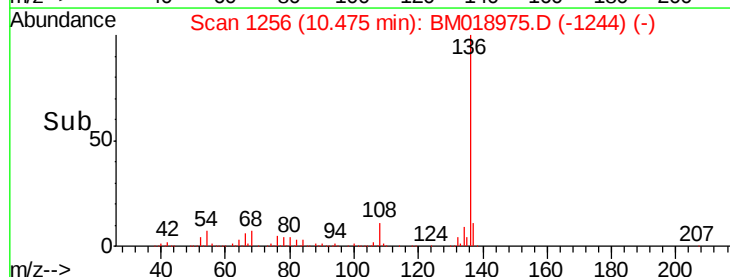
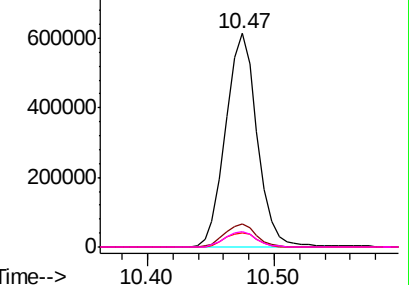


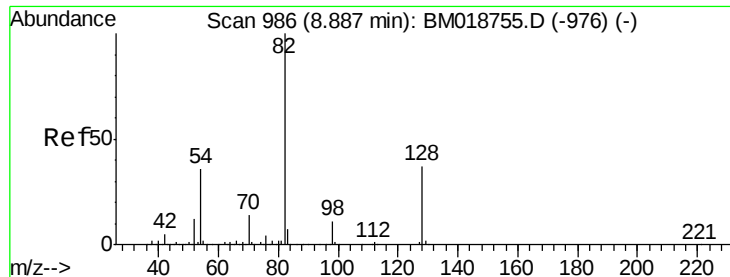

#23
 Nitrobenzene-d5
 Concen: 54.728 ng
 RT: 8.86 min Scan# 981
 Delta R.T. -0.03 min
 Lab File: BM018975.D
 Acq: 28 Feb 2019 18:38




Instrument :
 BNA_M
 ClientSampleId :
 PE-5(BELOW-EXPOSED-PIPE)


Tgt Ion: 82 Resp: 1254112
 Ion Ratio Lower Upper
 82 100
 128 37.6 29.9 44.9
 54 36.7 29.1 43.7

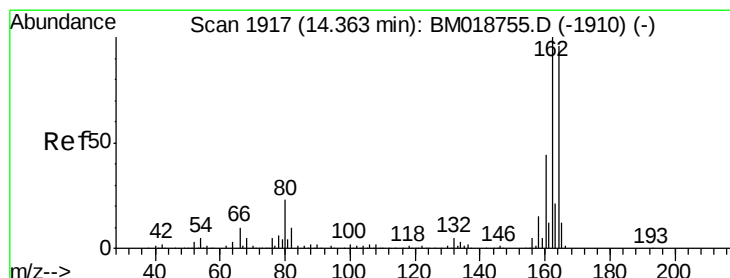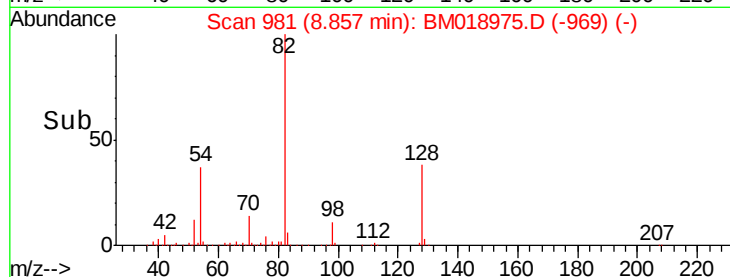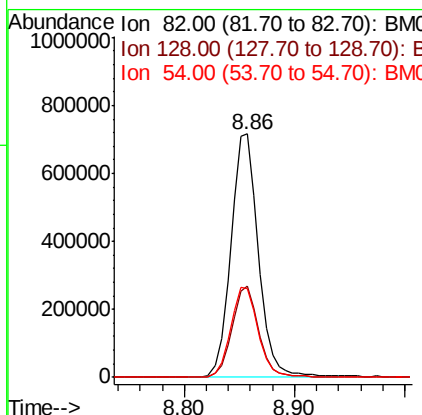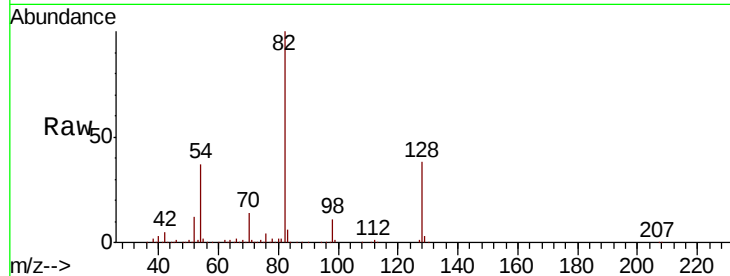

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.34 min Scan# 1913
 Delta R.T. -0.02 min
 Lab File: BM018975.D
 Acq: 28 Feb 2019 18:38

Tgt Ion: 164 Resp: 612820
 Ion Ratio Lower Upper
 164 100
 162 104.7 83.4 125.0
 160 46.4 36.6 55.0

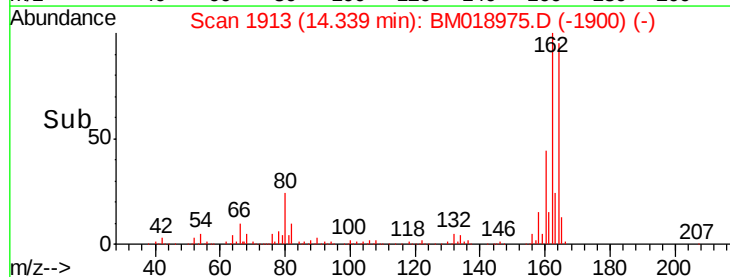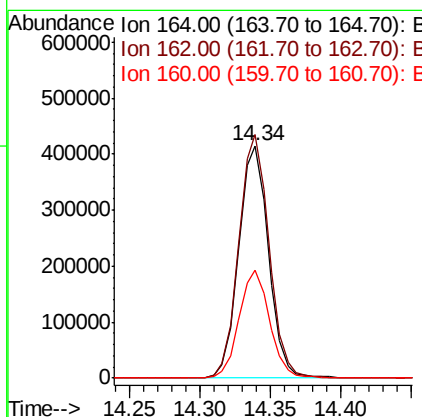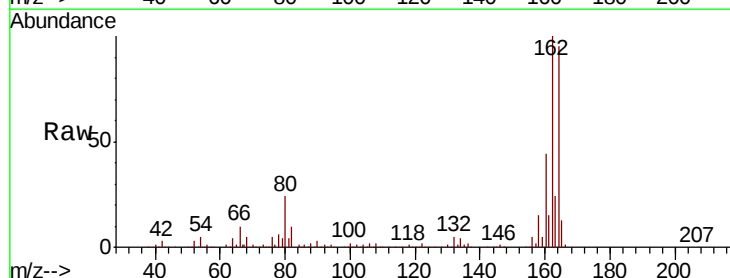

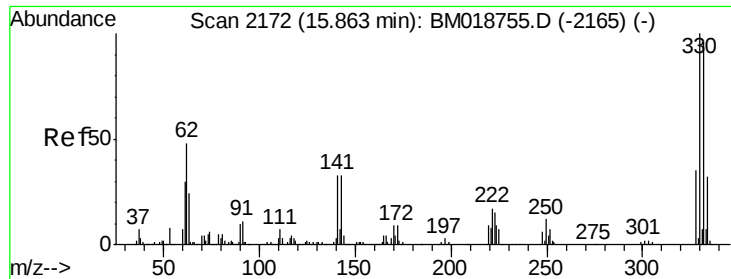

#42

2,4,6-Tribromophenol

Concen: 86.382 ng

RT: 15.84 min Scan# 2168

Delta R.T. -0.02 min

Lab File: BM018975.D

Acq: 28 Feb 2019 18:38

Instrument :

BNA_M

ClientSampleId :

PE-5(BELOW-EXPOSED-PIPE)


Tgt Ion:330 Resp: 763069

Ion Ratio Lower Upper

330 100

332 96.7 76.9 115.3




141 35.2 28.7 43.1

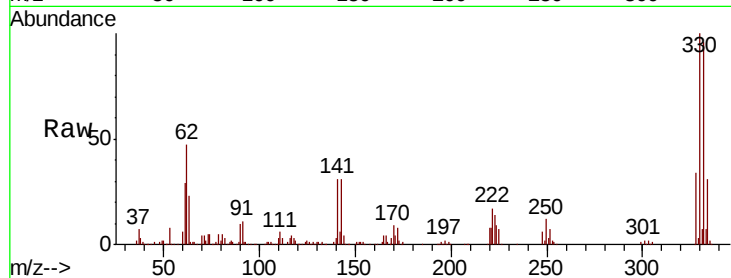

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

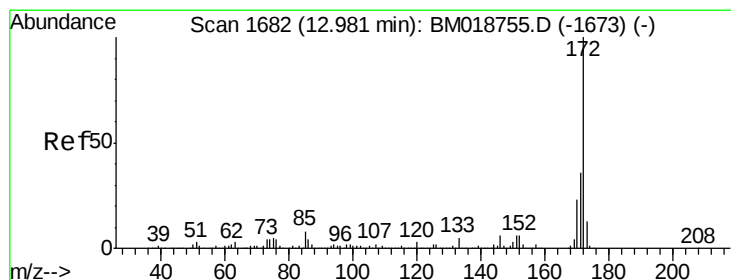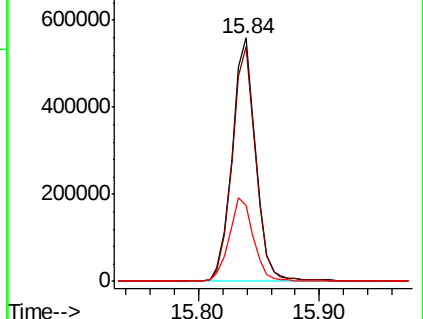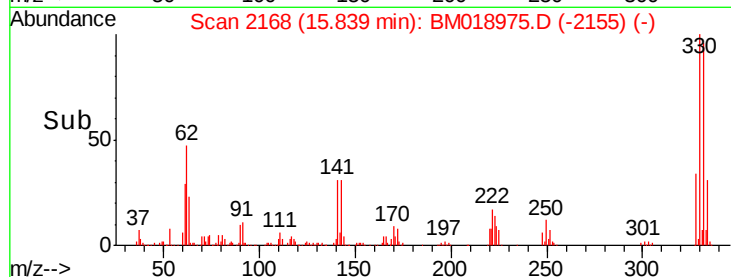

#45

2-Fluorobiphenyl

Concen: 51.621 ng

RT: 12.95 min Scan# 1677

Delta R.T. -0.03 min

Lab File: BM018975.D

Acq: 28 Feb 2019 18:38


Tgt Ion:172 Resp: 2383037

Ion Ratio Lower Upper

172 100

171 35.3 29.0 43.6



170 23.6 18.6 28.0

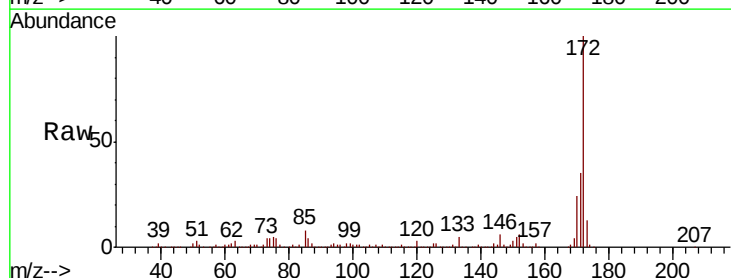


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

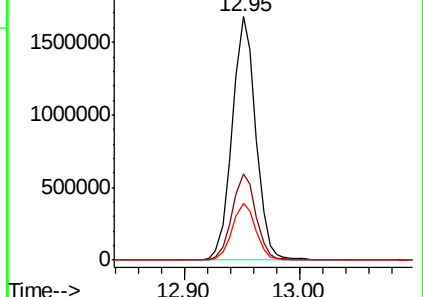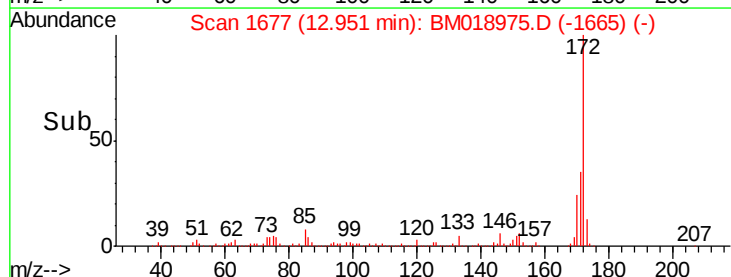


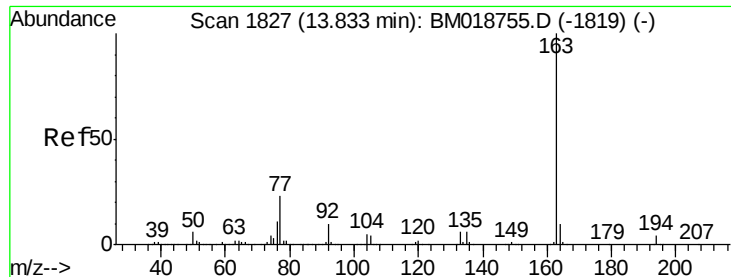




#50
Dimethylphthalate
Concen: 2.535 ng
RT: 13.80 min Scan# 1822
Delta R.T. -0.03 min
Lab File: BM018975.D
Acq: 28 Feb 2019 18:38

Instrument :
BNA_M
ClientSampleId :
PE-5(BELOW-EXPOSED-PIPE)

Tgt Ion:163 Resp: 129466
Ion Ratio Lower Upper
163 100
194 3.6 3.2 4.8
164 9.4 7.8 11.8

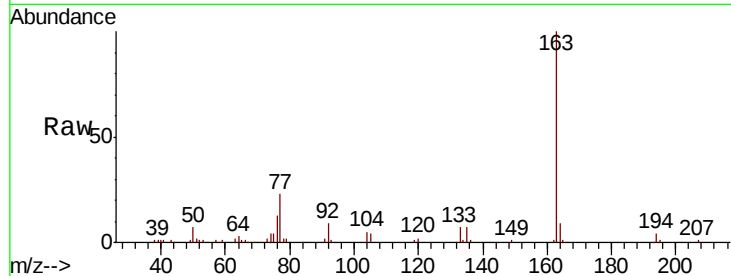


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

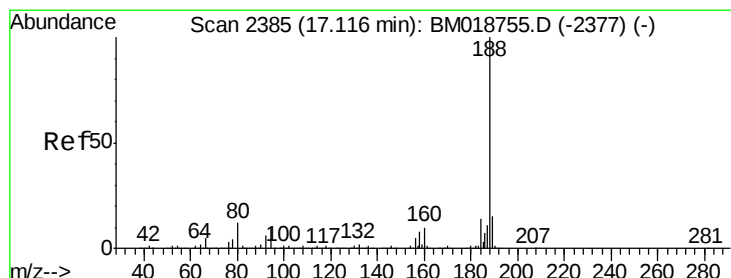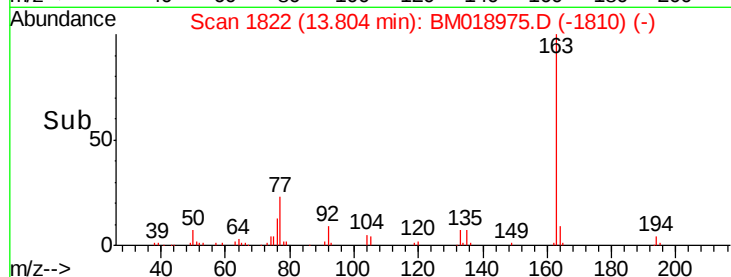
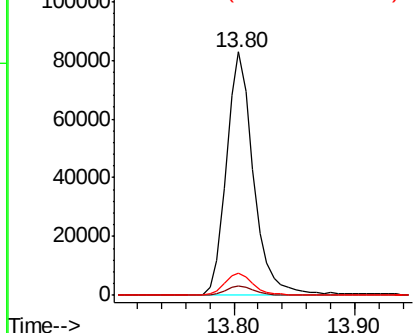



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.09 min Scan# 2381
Delta R.T. -0.02 min
Lab File: BM018975.D
Acq: 28 Feb 2019 18:38

Tgt Ion:188 Resp: 1390514
Ion Ratio Lower Upper
188 100
94 10.0 8.2 12.2
80 12.5 9.7 14.5

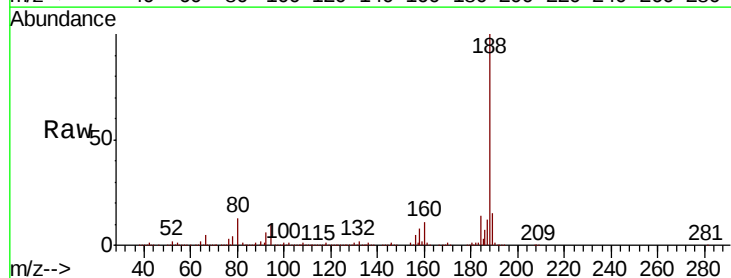

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BM0
Ion 80.00 (79.70 to 80.70): BM0

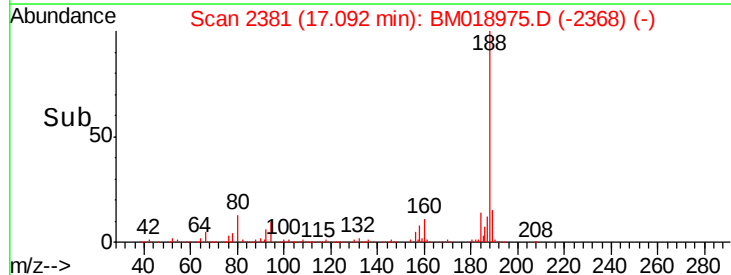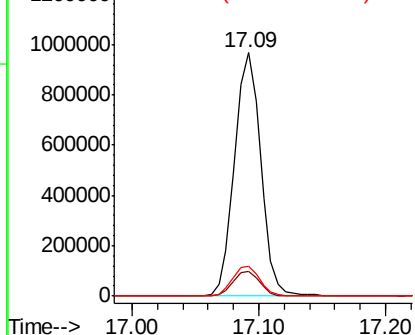


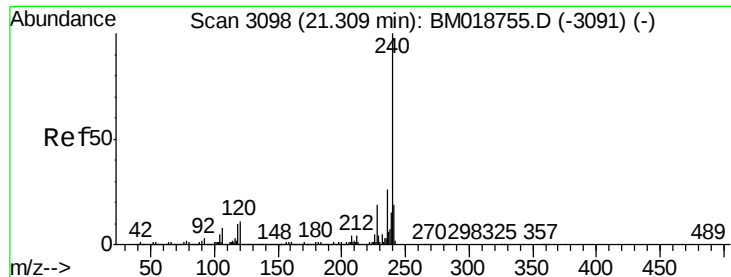




#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.29 min Scan# 3094
Delta R.T. -0.02 min
Lab File: BM018975.D
Acq: 28 Feb 2019 18:38

Instrument :
BNA_M
ClientSampleId :
PE-5(BELOW-EXPOSED-PIPE)

Tgt Ion:240 Resp: 1338326
Ion Ratio Lower Upper
240 100
120 11.4 8.9 13.3
236 25.8 20.9 31.3

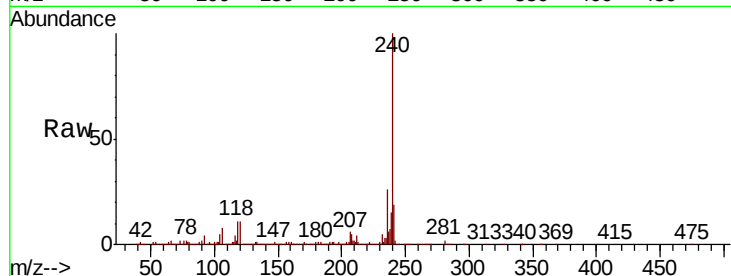


Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

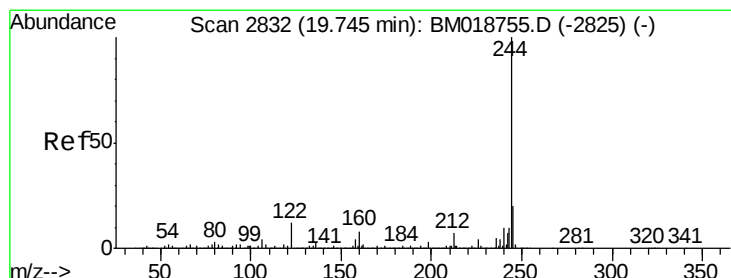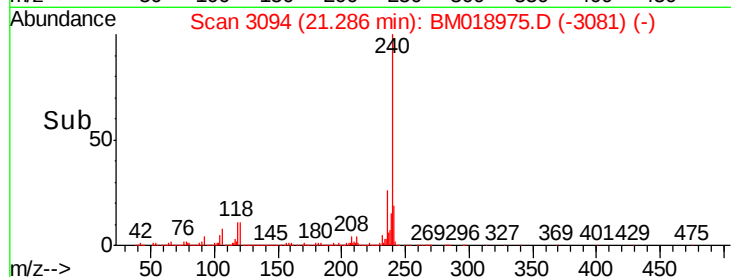
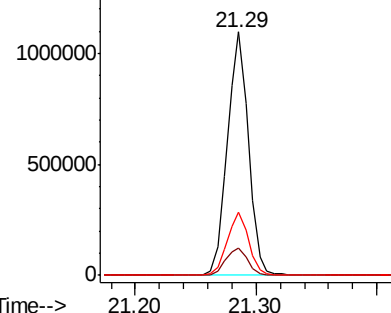



#79
Terphenyl-d14
Concen: 56.959 ng
RT: 19.73 min Scan# 2829
Delta R.T. -0.02 min
Lab File: BM018975.D
Acq: 28 Feb 2019 18:38

Tgt Ion:244 Resp: 3695268
Ion Ratio Lower Upper
244 100
212 6.8 5.6 8.4
122 10.9 9.3 13.9

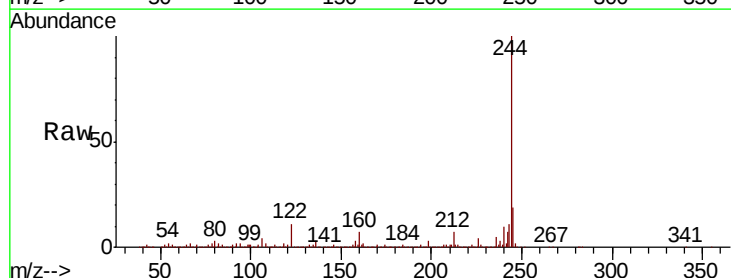

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

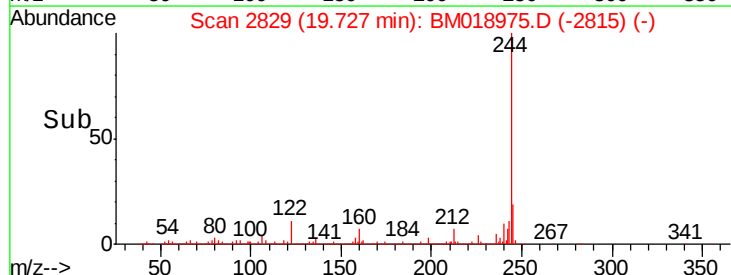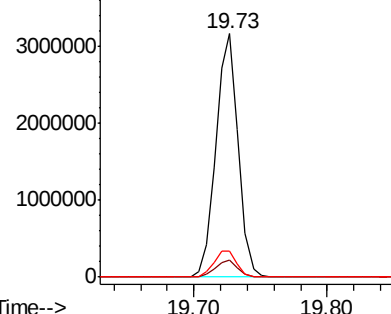

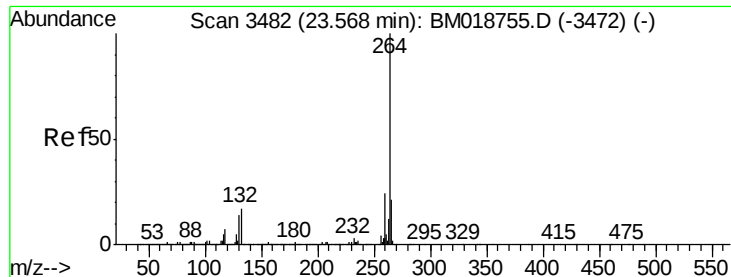

#87
Perylene-d12
Concen: 20.000 ng
RT: 23.53 min Scan# 3476
Delta R.T. -0.04 min
Lab File: BM018975.D
Acq: 28 Feb 2019 18:38

Instrument :
BNA_M
ClientSampleId :
PE-5(BELOW-EXPOSED-PIPE)

Tgt Ion:264 Resp: 1190364

Ion	Ratio	Lower	Upper
264	100		
260	24.0	18.9	28.3
265	22.4	17.3	25.9

