
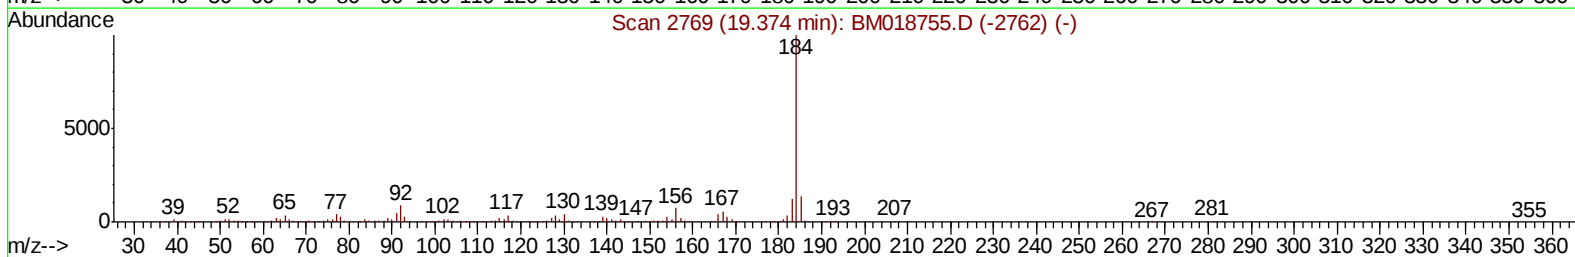
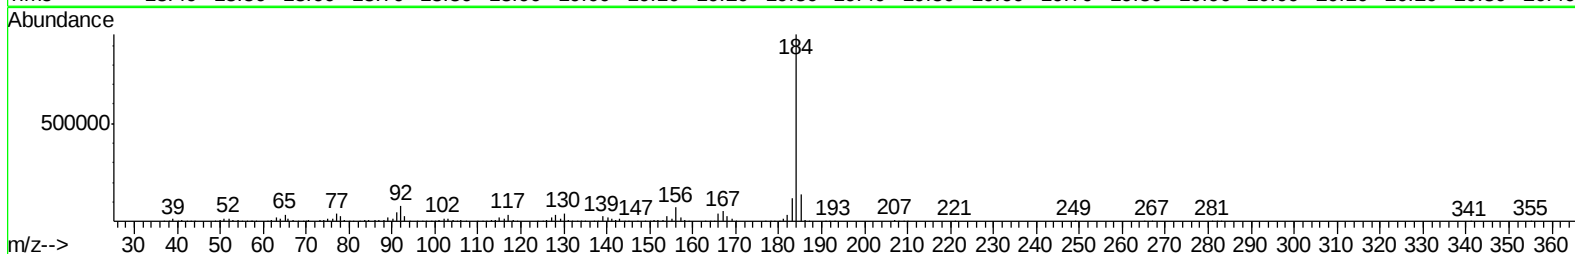


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022819\
 Data File : BM018964.D
 Acq On : 28 Feb 2019 12:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 02:02:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration

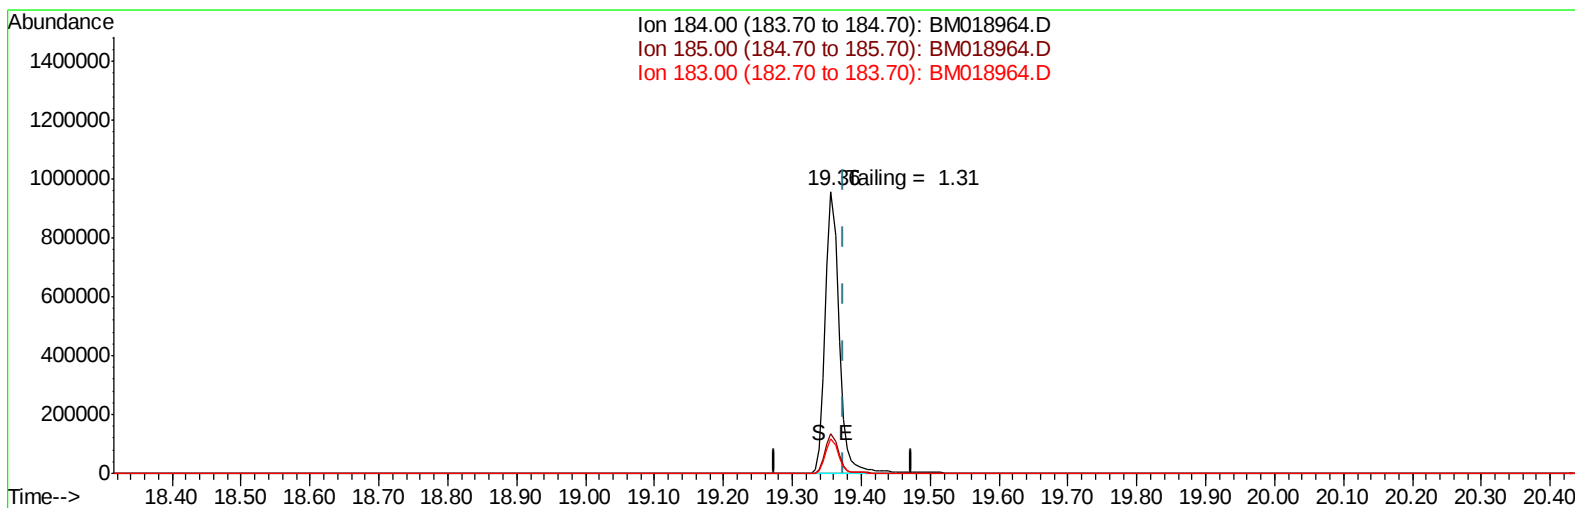

TIC: BM018964.D

(77) Benzidine




19.356min (-0.018) 15420.31ng

response 1337403

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	14.24
183.00	12.10	12.11
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022819\
Data File : BM018964.D
Acq On : 28 Feb 2019 12:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 02:02:46 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

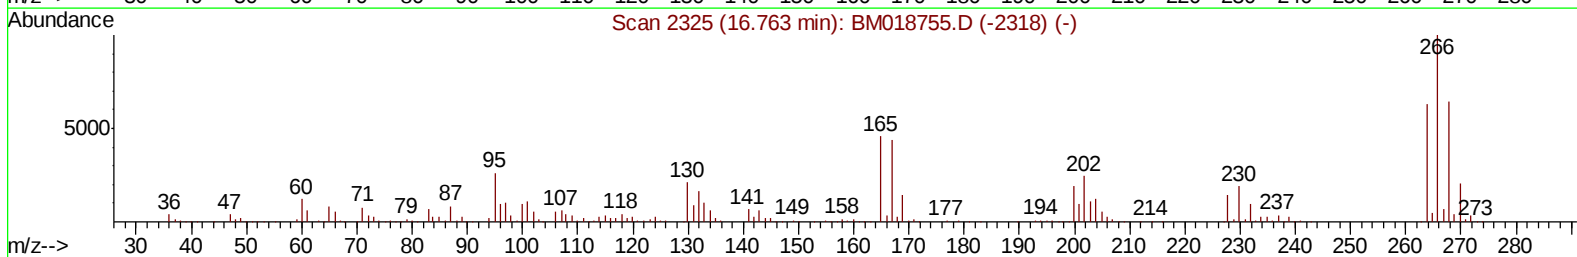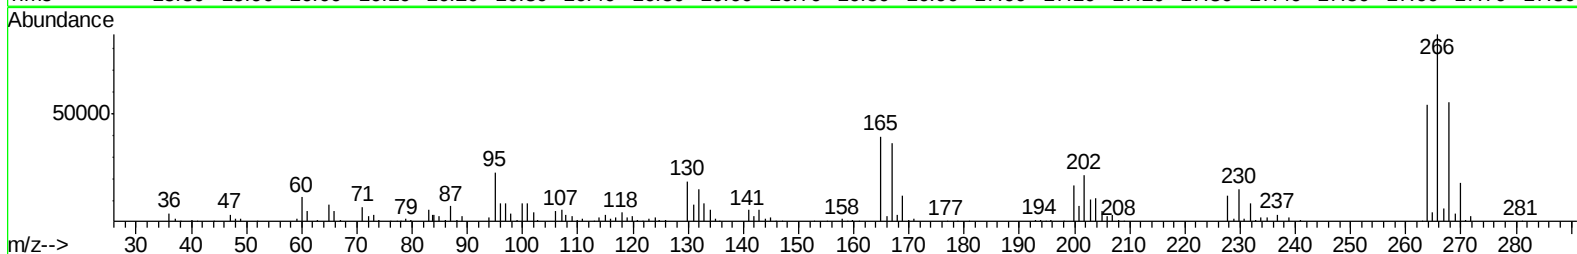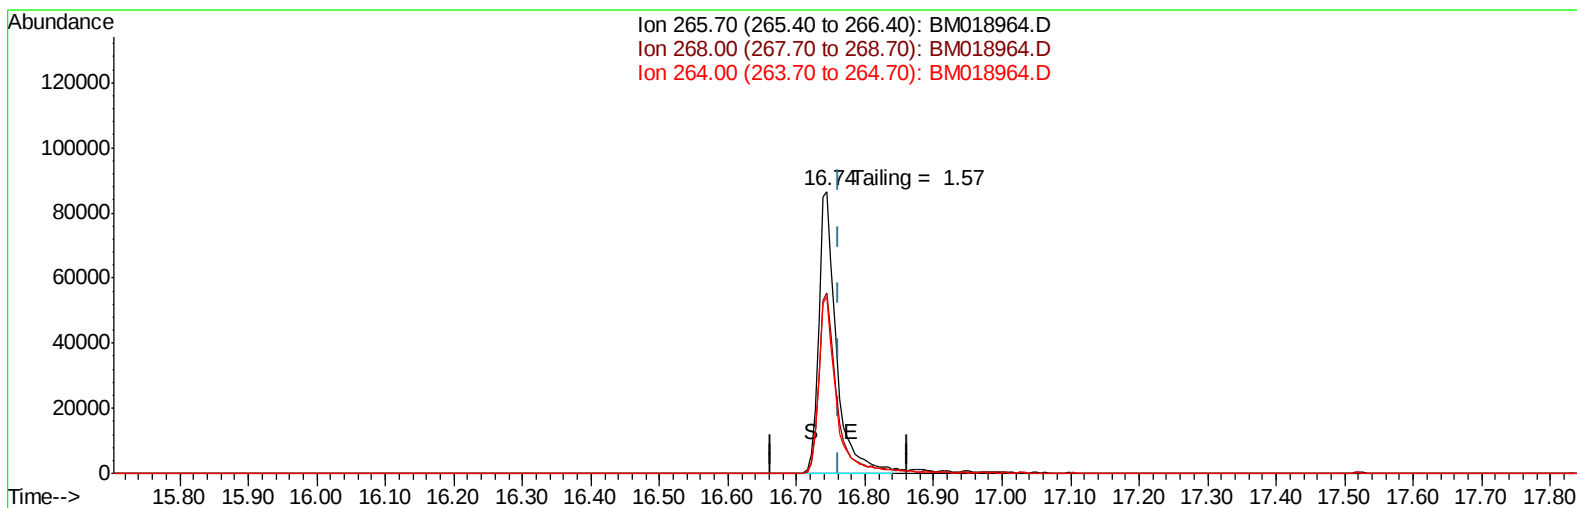

TIC: BM018964.D

(70) Pentachlorophenol (C)

16.745min (-0.018) 0.00ng

response 154688

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	64.10
264.00	63.20	62.58
0.00	0.00	0.00