

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022819\
 Data File : BM018968.D
 Acq On : 28 Feb 2019 14:26
 Operator : JU/SJ
 Sample : K1616-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TI-658

Quant Time: Mar 01 01:23:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	222467	20.00	ng	-0.03
21) Naphthalene-d8	10.47	136	987887	20.00	ng	-0.03
39) Acenaphthene-d10	14.34	164	593242	20.00	ng	-0.02
64) Phenanthrene-d10	17.09	188	1344318	20.00	ng	-0.02
76) Chrysene-d12	21.29	240	1428888	20.00	ng	-0.02
87) Perylene-d12	23.54	264	1259321	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.28	112	471185	34.70	ng	-0.02
7) Phenol-d6	6.86	99	426400	22.29	ng	-0.02
23) Nitrobenzene-d5	8.86	82	1630441	76.31	ng	-0.03
42) 2,4,6-Tribromophenol	15.84	330	671452	78.52	ng	-0.02
45) 2-Fluorobiphenyl	12.95	172	3399948	76.08	ng	-0.03
79) Terphenyl-d14	19.73	244	4928333	71.15	ng	-0.02
Target Compounds						
50) Dimethylphthalate	13.80	163	166685	3.371	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022819\
Data File : BM018968.D
Acq On : 28 Feb 2019 14:26
Operator : JU/SJ
Sample : K1616-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TI-658

Quant Time: Mar 01 01:23:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

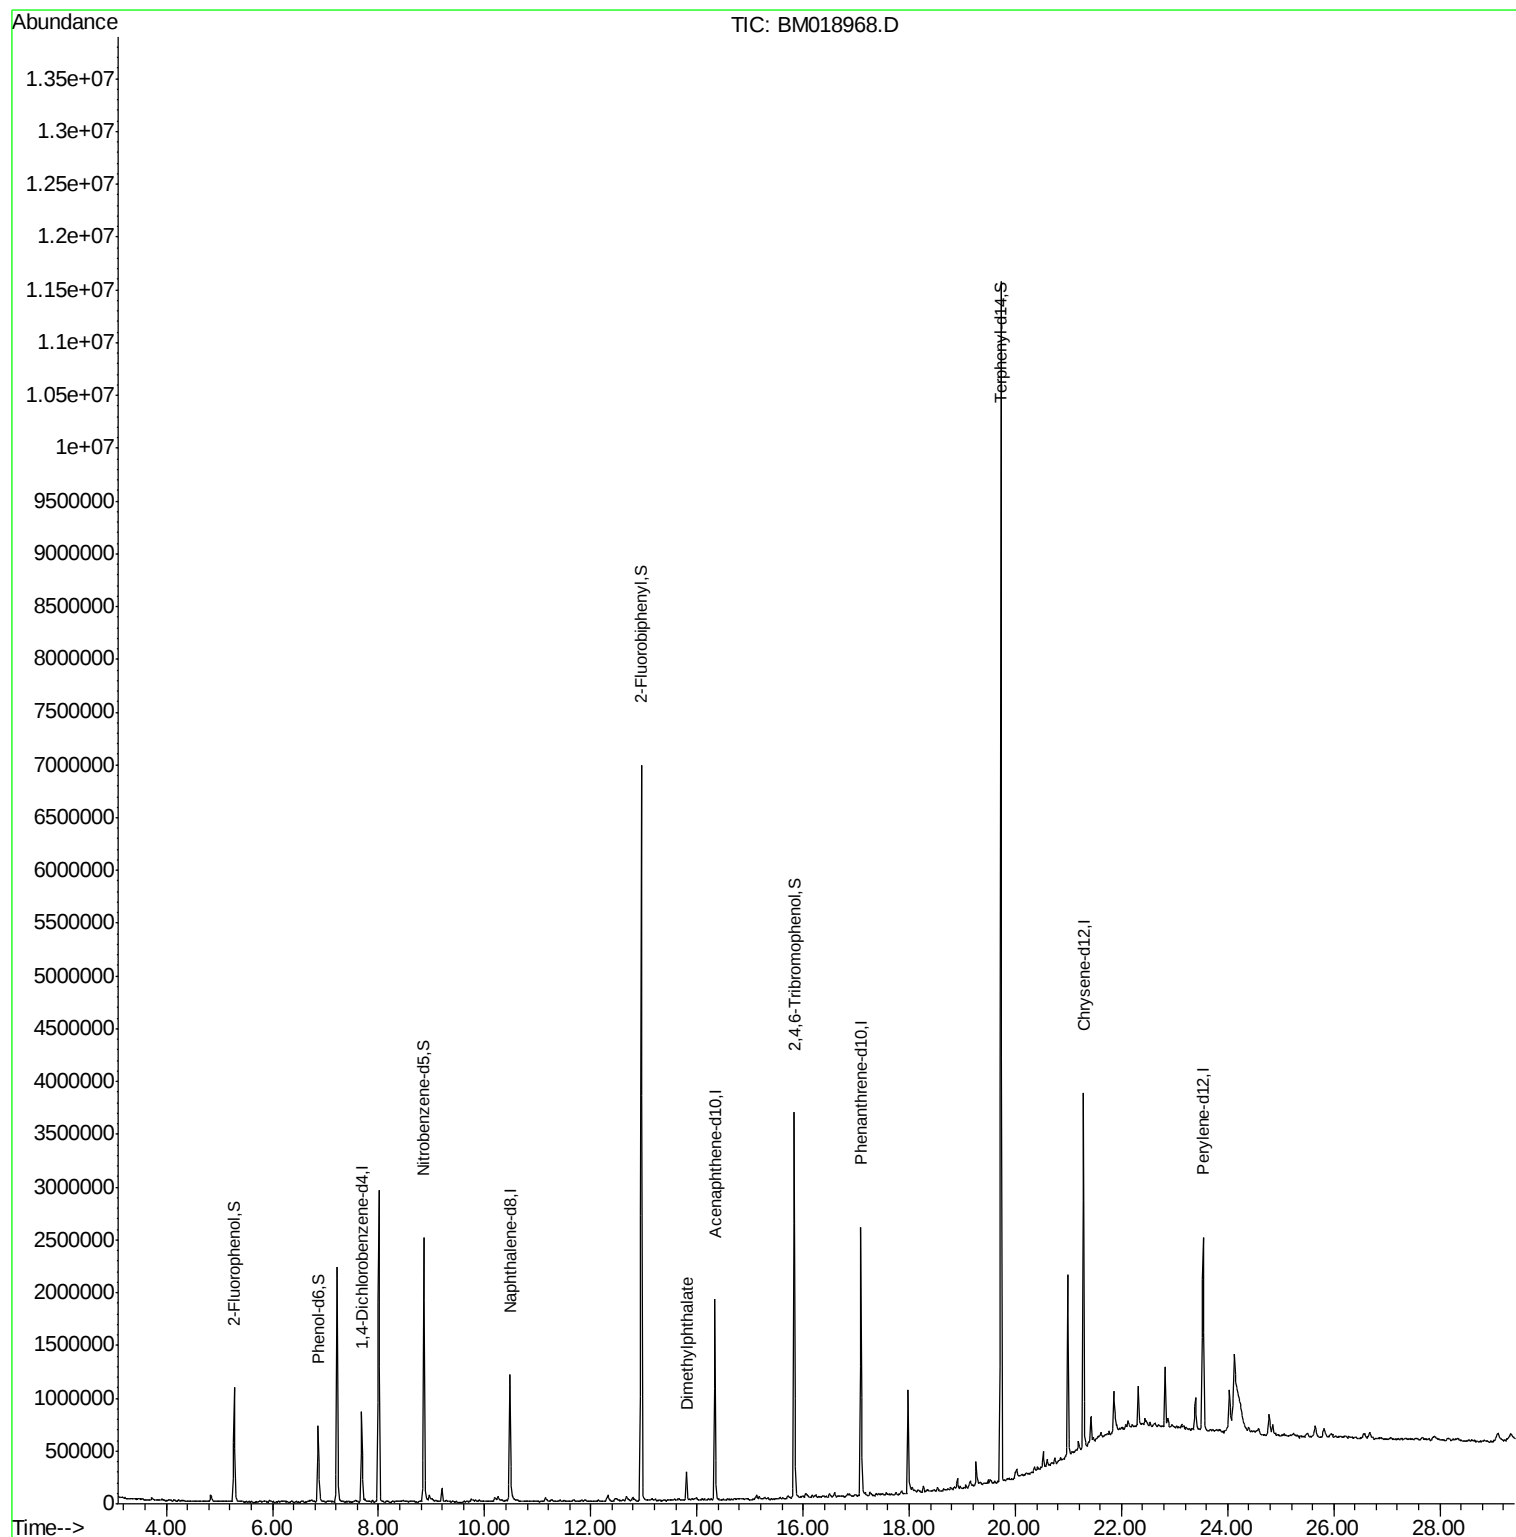

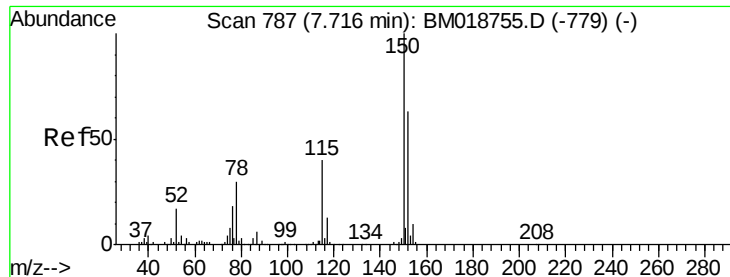


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.69 min Scan# 782
Delta R.T. -0.03 min
Lab File: BM018968.D
Acq: 28 Feb 2019 14:26

Instrument :
BNA_M
ClientSampleId :
TI-658

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.1	127.3	190.9
115	62.3	50.8	76.2



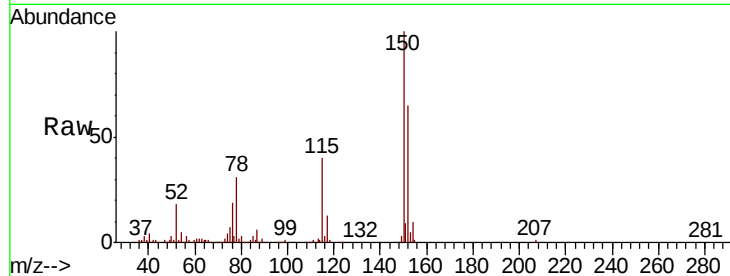


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

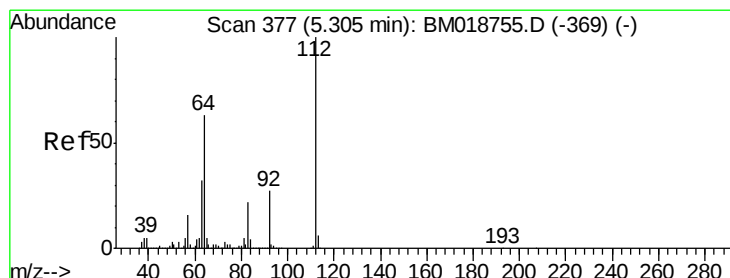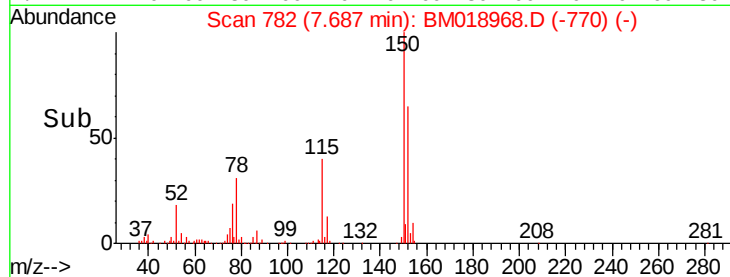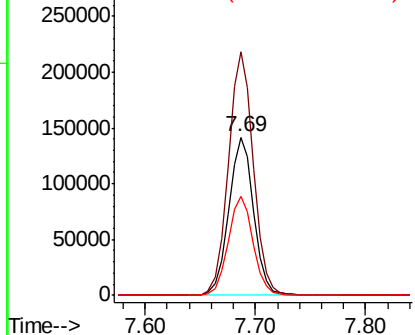

#5

2-Fluorophenol
Concen: 34.703 ng
RT: 5.28 min Scan# 373
Delta R.T. -0.02 min
Lab File: BM018968.D
Acq: 28 Feb 2019 14:26

Tgt Ion	Ratio	Lower	Upper
112	100		
64	62.6	50.6	75.8
63	32.1	25.7	38.5


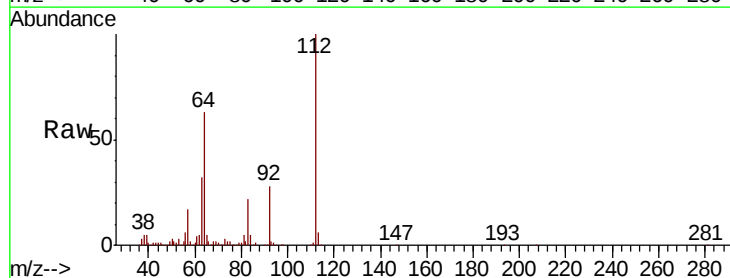


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BM0

Ion 63.00 (62.70 to 63.70): BM0

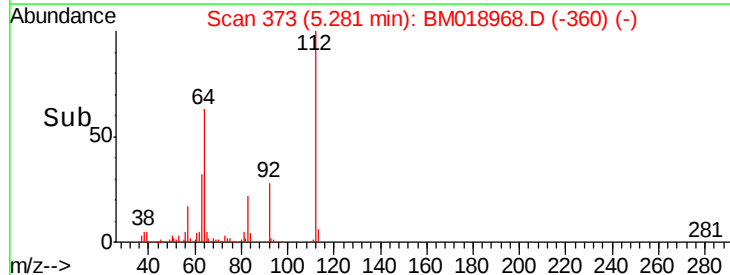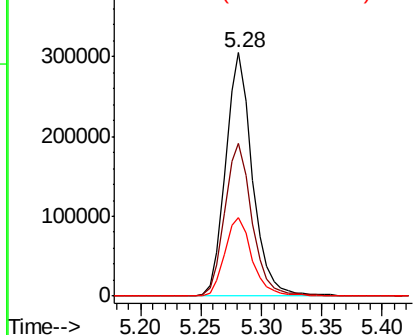



#7

Phenol-d6

Concen: 22.292 ng

RT: 6.86 min Scan# 642

Delta R.T. -0.02 min

Lab File: BM018968.D

Acq: 28 Feb 2019 14:26

Instrument :

BNA_M

ClientSampleId :

TI-658


Tot Ion: 99 Resp: 426400

Ion Ratio Lower Upper

99 100

42 13.6 11.0 16.6




71 37.9 31.3 46.9

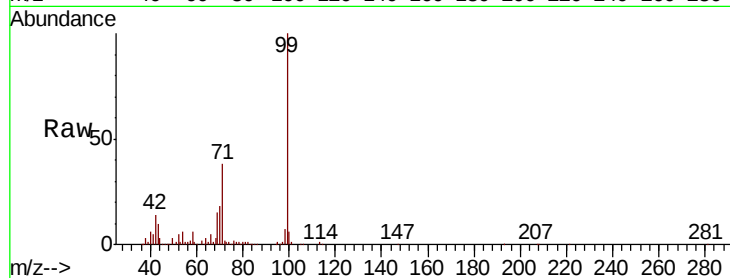

Abundance Ion 99.00 (98.70 to 99.70): BM018755.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018755.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018755.D (-637) (-)

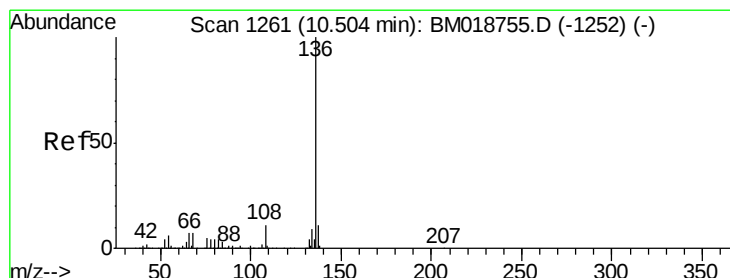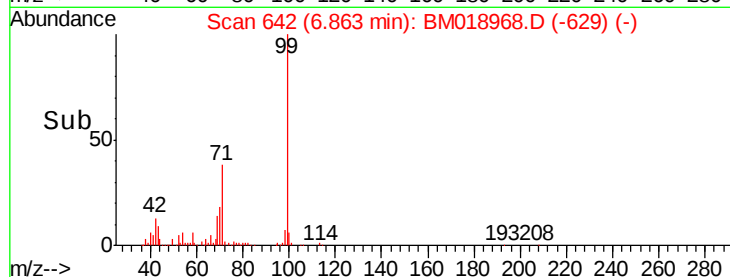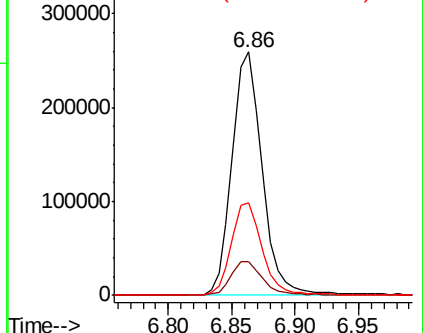

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.47 min Scan# 1256

Delta R.T. -0.03 min

Lab File: BM018968.D

Acq: 28 Feb 2019 14:26

Tgt Ion: 136 Resp: 987887


Ion Ratio Lower Upper

136 100

137 10.4 8.8 13.2

54 6.8 5.0 7.6

68 7.3 5.5 8.3


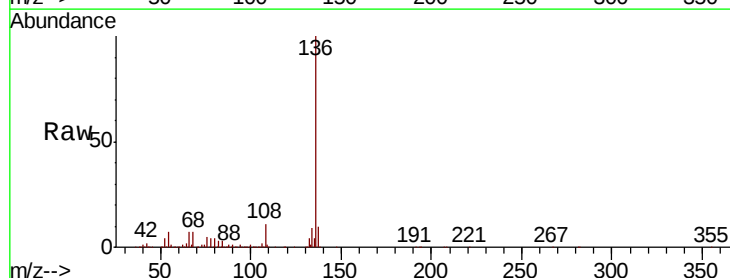



Abundance Ion 136.00 (135.70 to 136.70): BM018755.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM018755.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM018755.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM018755.D (-1252) (-)



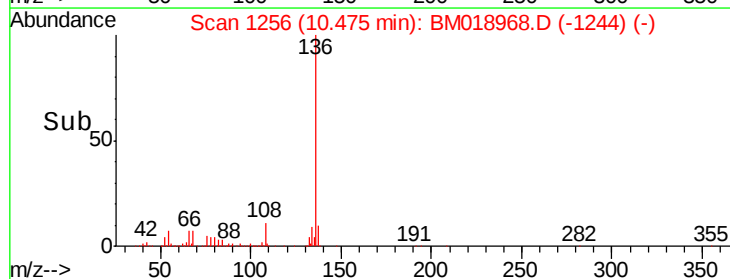
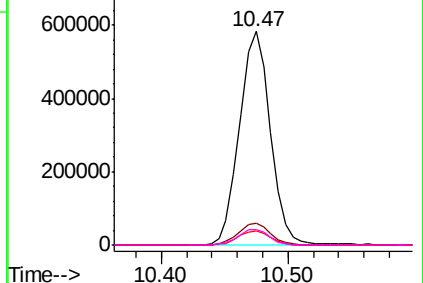


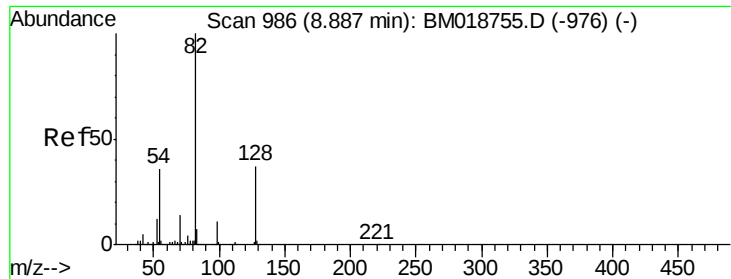

#23
 Nitrobenzene-d5
 Concen: 76.314 ng
 RT: 8.86 min Scan# 981
 Delta R.T. -0.03 min
 Lab File: BM018968.D
 Acq: 28 Feb 2019 14:26




Instrument :
 BNA_M
 ClientSampleId :
 TI-658

Tot Ion: 82 Resp: 1630441
 Ion Ratio Lower Upper
 82 100
 128 37.5 29.9 44.9
 54 36.9 29.1 43.7

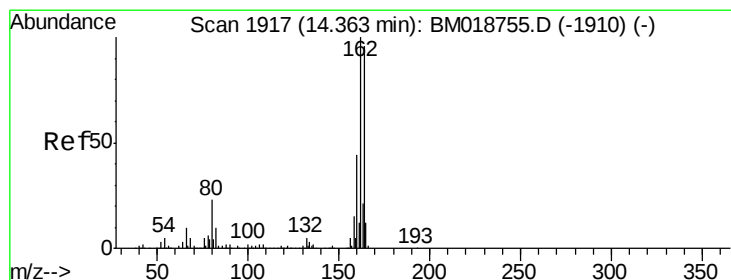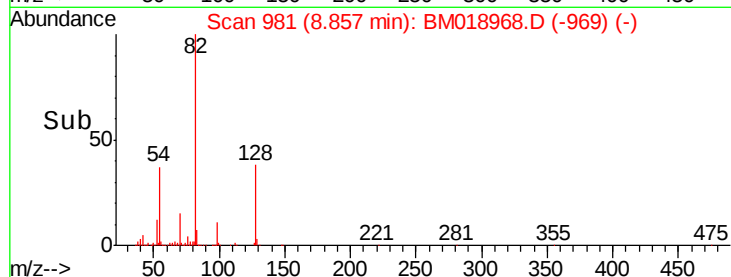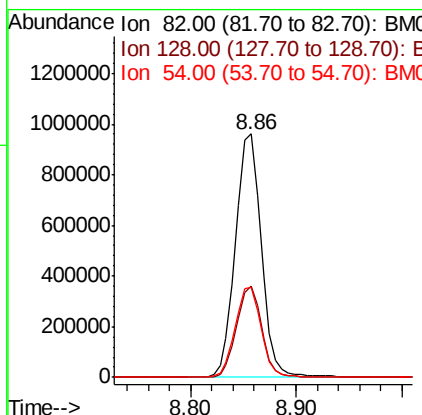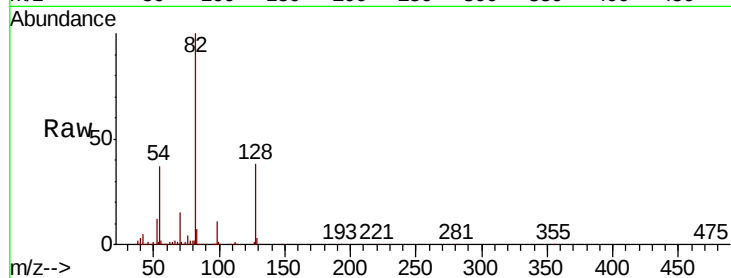

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.34 min Scan# 1913
 Delta R.T. -0.02 min
 Lab File: BM018968.D
 Acq: 28 Feb 2019 14:26

Tgt Ion: 164 Resp: 593242
 Ion Ratio Lower Upper
 164 100
 162 103.8 83.4 125.0
 160 46.7 36.6 55.0

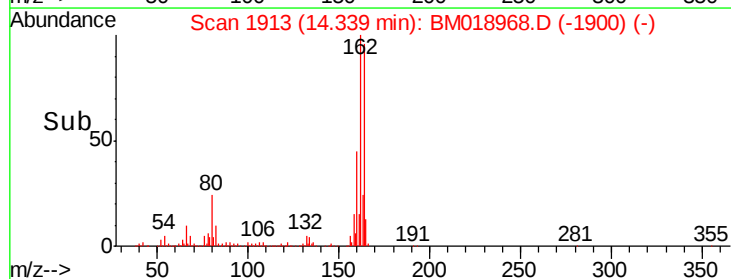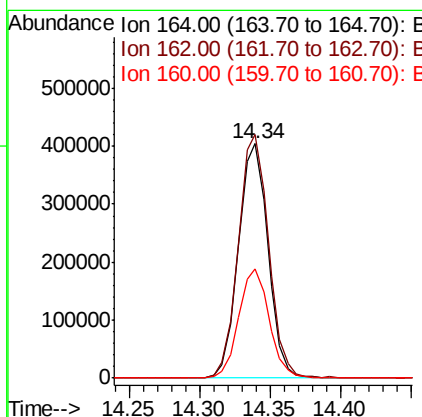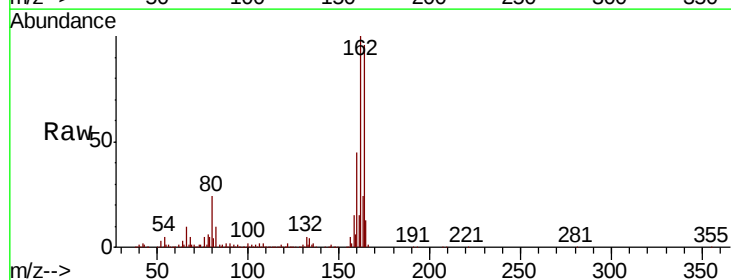







#42
 2,4,6-Tribromophenol
 Concen: 78.519 ng
 RT: 15.84 min Scan# 2168
 Delta R.T. -0.02 min
 Lab File: BM018968.D
 Acq: 28 Feb 2019 14:26

Instrument :
 BNA_M
 ClientSampleId :
 TI-658

Tot Ion:330 Resp: 671452
 Ion Ratio Lower Upper
 330 100
 332 98.0 76.9 115.3
 141 35.8 28.7 43.1

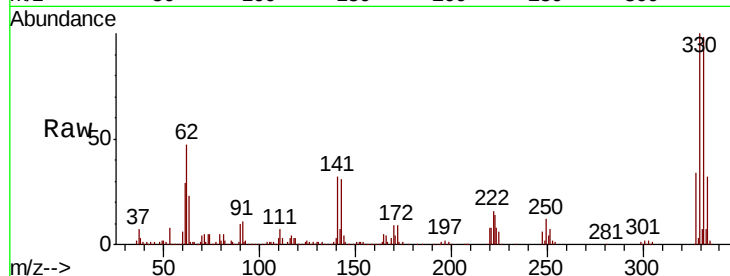


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

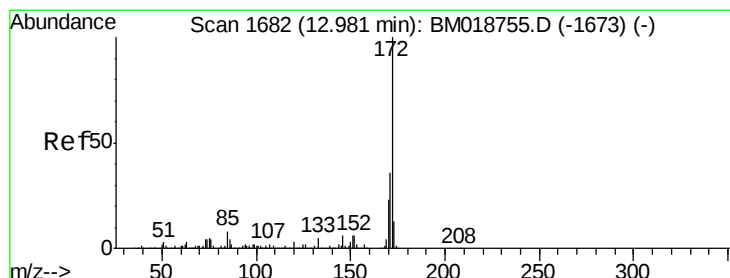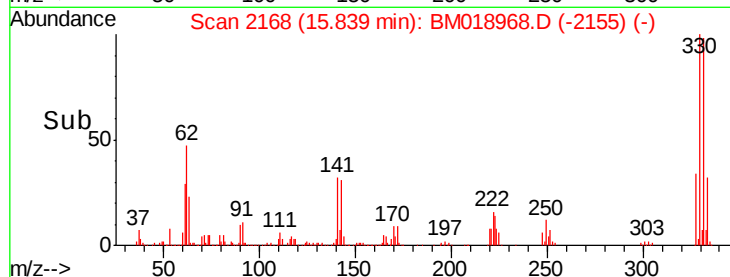
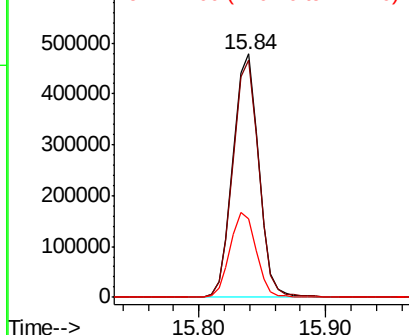



#45
 2-Fluorobiphenyl
 Concen: 76.079 ng
 RT: 12.95 min Scan# 1677
 Delta R.T. -0.03 min
 Lab File: BM018968.D
 Acq: 28 Feb 2019 14:26

Tgt Ion:172 Resp: 3399948
 Ion Ratio Lower Upper
 172 100
 171 35.8 29.0 43.6
 170 23.3 18.6 28.0

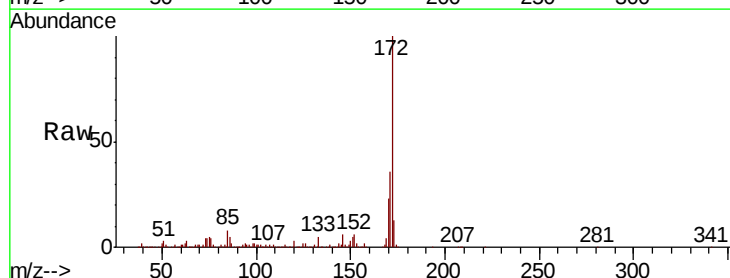

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

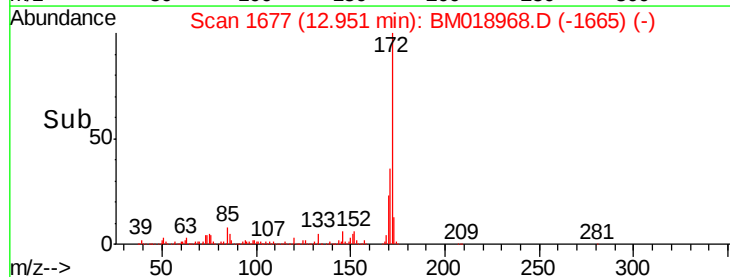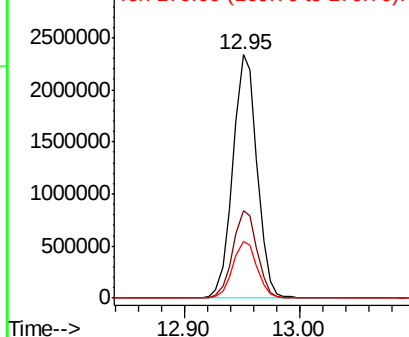


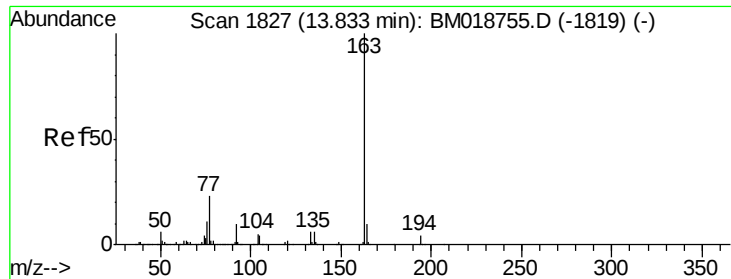

#50
Dimethylphthalate
Concen: 3.371 ng
RT: 13.80 min Scan# 1822
Delta R.T. -0.03 min
Lab File: BM018968.D
Acq: 28 Feb 2019 14:26

Instrument :
BNA_M
ClientSampleId :
TI-658

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.2	4.8
164	10.5	7.8	11.8



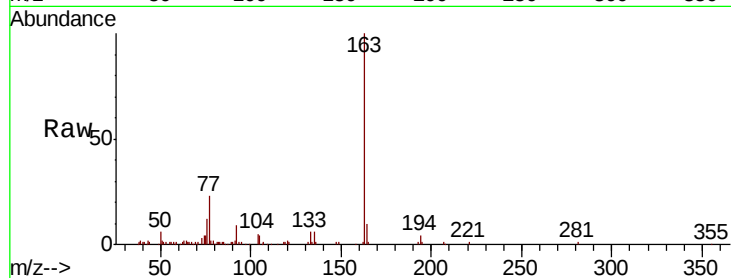


Abundance

Ion 163.00 (162.70 to 163.70): E


Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

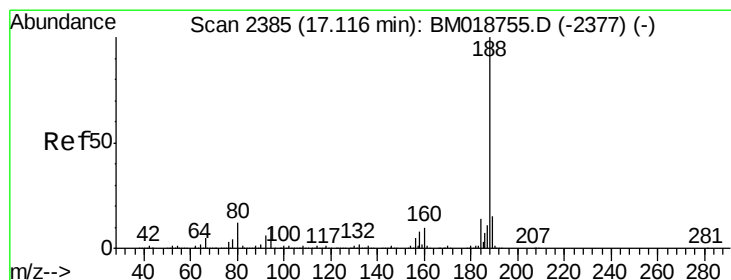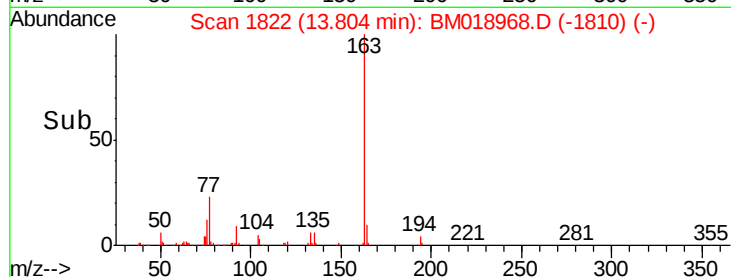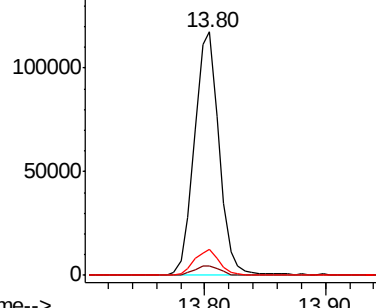

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.09 min Scan# 2381
Delta R.T. -0.02 min
Lab File: BM018968.D
Acq: 28 Feb 2019 14:26

Tgt Ion	Ratio	Lower	Upper
188	100		
94	10.1	8.2	12.2
80	12.4	9.7	14.5


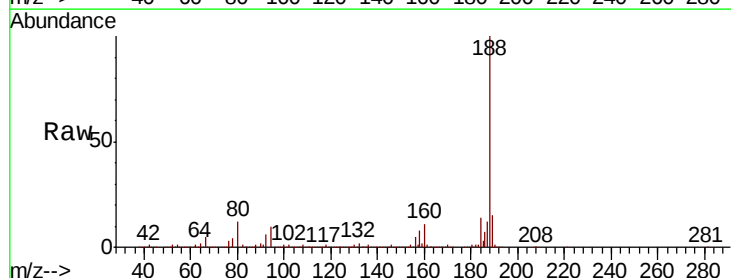



Abundance

Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

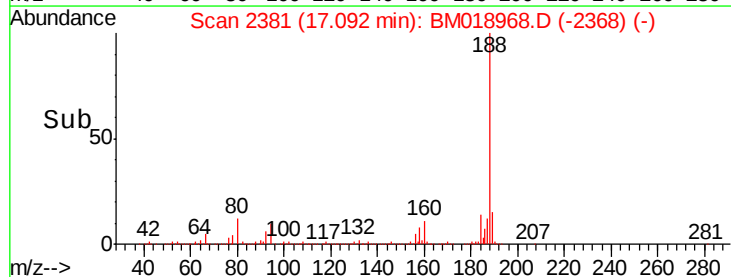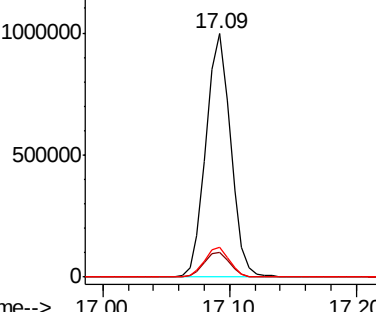


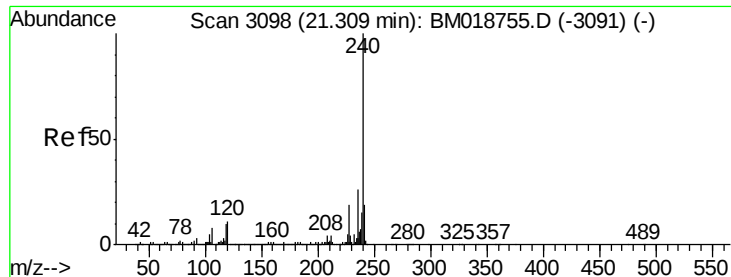




#76
 Chrvsene-d12
 Concen: 20.000 ng
 RT: 21.29 min Scan# 3094
 Delta R.T. -0.02 min
 Lab File: BM018968.D
 Acq: 28 Feb 2019 14:26

Instrument :
 BNA_M
 ClientSampleId :
 TI-658

Tot Ion:240 Resp: 1428888
 Ion Ratio Lower Upper
 240 100
 120 11.8 8.9 13.3
 236 25.6 20.9 31.3

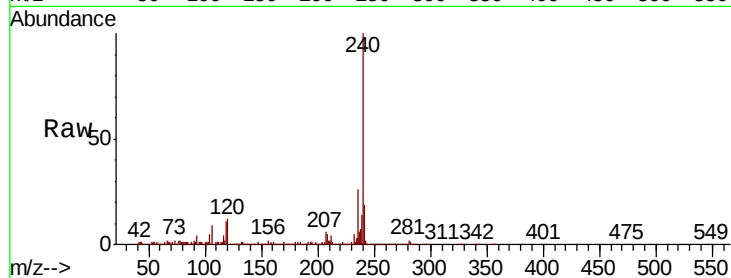


Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

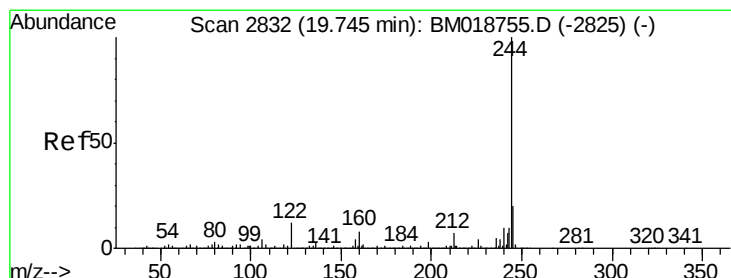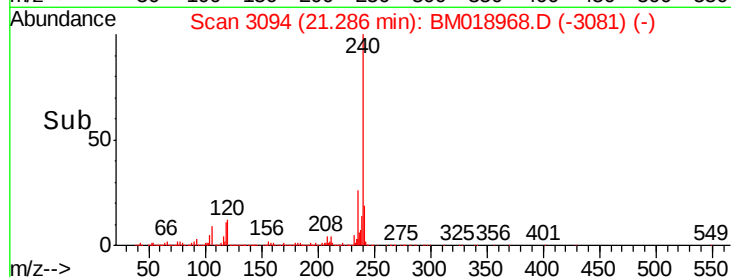
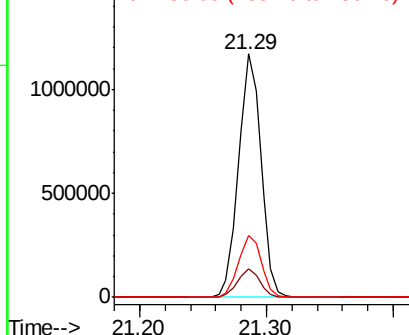



#79
 Terphenyl-d14
 Concen: 71.151 ng
 RT: 19.73 min Scan# 2829
 Delta R.T. -0.02 min
 Lab File: BM018968.D
 Acq: 28 Feb 2019 14:26

Tgt Ion:244 Resp: 4928333
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.6 8.4
 122 11.8 9.3 13.9

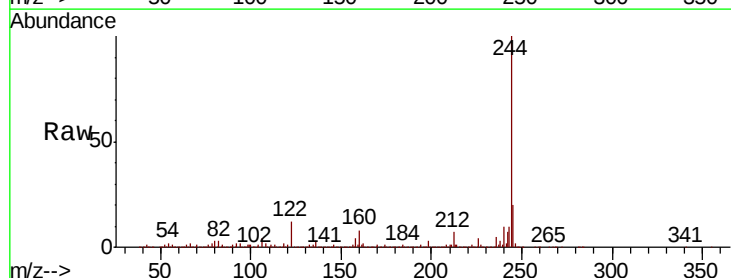

Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

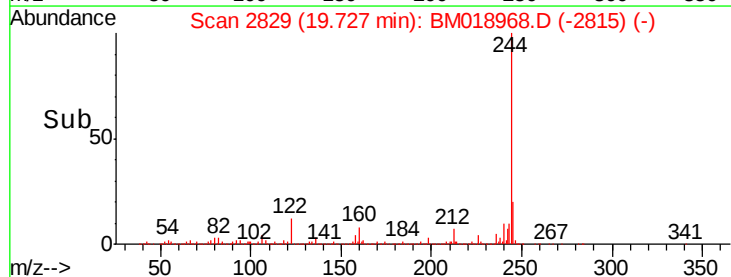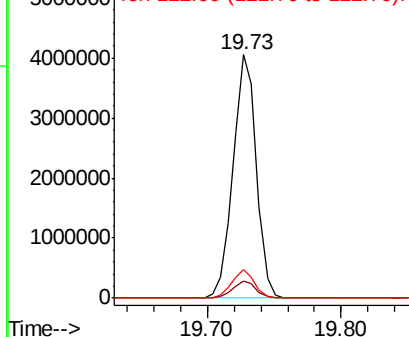

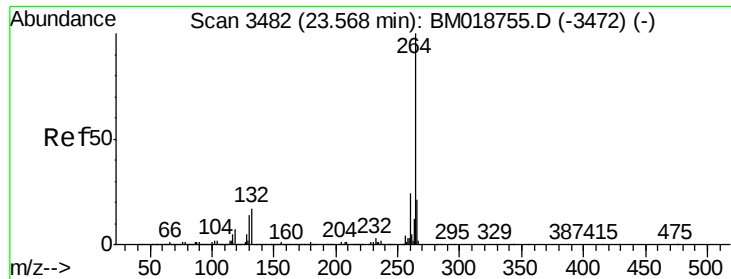

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.54 min Scan# 3477
 Delta R.T. -0.03 min
 Lab File: BM018968.D
 Acq: 28 Feb 2019 14:26

Instrument :
 BNA_M
 ClientSampleId :
 TI-658

Tot Ion: 264 Resp: 1259321
 Ion Ratio Lower Upper
 264 100
 260 23.5 18.9 28.3
 265 21.6 17.3 25.9

