


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022819\
Data File : BM018964.D
Acq On : 28 Feb 2019 12:03
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 11 16:02:12 2019

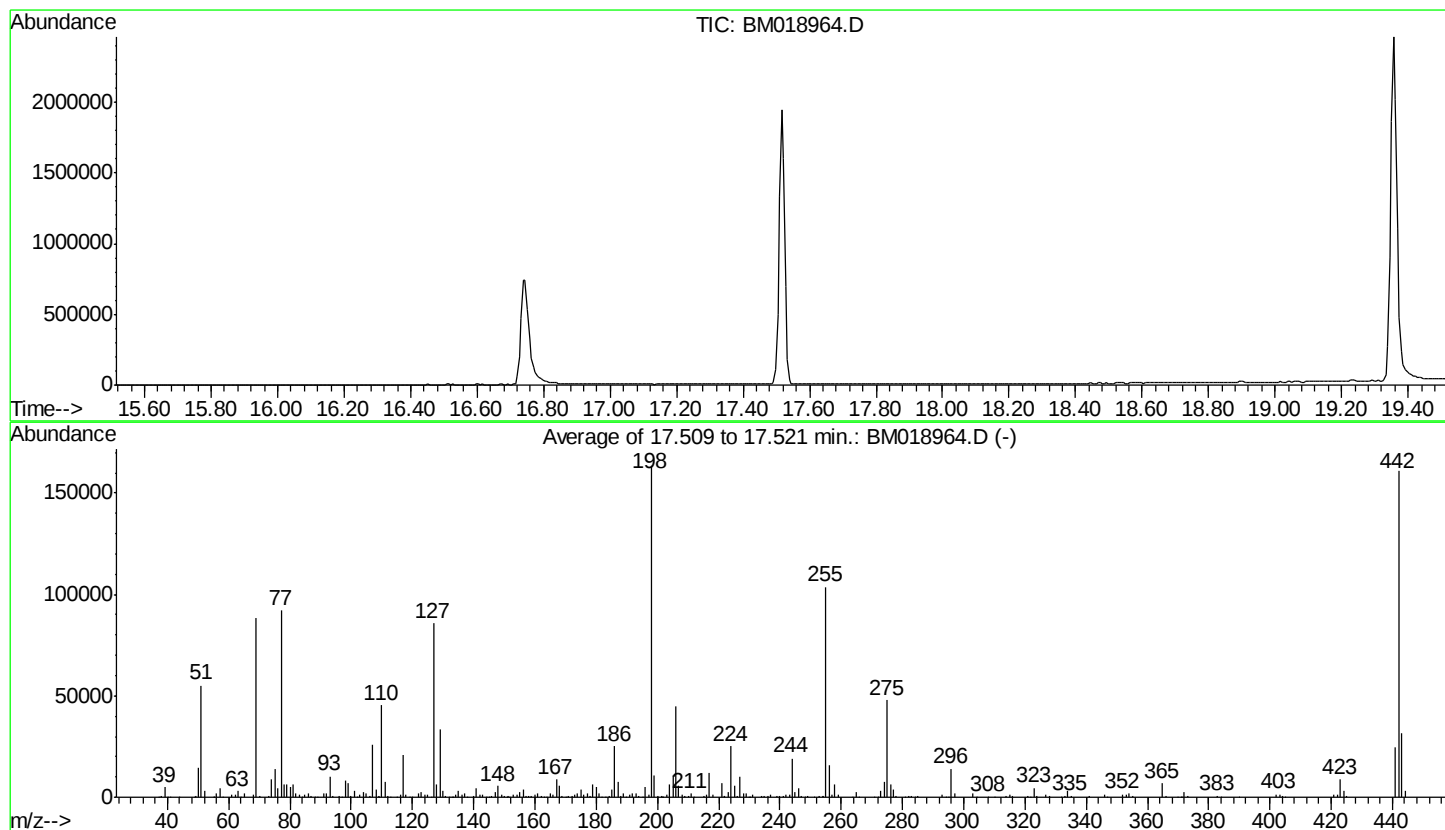

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2446

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	54936	PASS
68	69	0.00	2	1.7	1495	PASS
69	198	0.00	100	54.2	88664	PASS
70	69	0.00	2	0.6	523	PASS
127	198	10	80	52.4	85616	PASS
197	198	0.00	2	0.7	1188	PASS
198	198	100	100	100.0	163541	PASS
199	198	5	9	6.7	10892	PASS
275	198	10	60	29.3	47866	PASS
365	198	1	100	4.2	6935	PASS
441	198	0.01	100	15.1	24753	PASS
442	198	50	100	98.6	161285	PASS
443	442	15	24	19.4	31288	PASS