

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044444.D
 Acq On : 29 Feb 2024 17:53
 Operator : MA/JU
 Sample : P1512-07
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0SA5

Quant Time: Feb 29 22:33:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 29 03:37:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.963	152	165000	20.000	ng/ul	0.01
20) Naphthalene-d8	10.769	136	730332	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.598	164	424294	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.351	188	873912	20.000	ng/ul	0.01
79) Chrysene-d12	21.539	240	727811	20.000	ng/ul	0.00
88) Perylene-d12	23.968	264	795785	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	30698	5.870	ng/uL	0.00
4) Pyridine-d5	3.793	84	461158	32.289	ng/ul	0.00
7) Phenol-d5	7.128	99	534235	33.799	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.304	67	359103	35.083	ng/ul	0.01
11) 2-Chlorophenol-d4	7.487	132	443904	37.288	ng/ul	0.01
15) 4-Methylphenol-d8	8.675	113	434403	36.322	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	222374	37.448	ng/ul	0.01
24) 2-Nitrophenol-d4	9.857	143	238457	39.360	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.387	165	389527	36.449	ng/ul	0.01
31) 4-Chloroaniline-d4	10.916	131	604837	33.698	ng/ul	0.01
46) Dimethylphthalate-d6	14.027	166	1272389	38.883	ng/ul	0.01
49) Acenaphthylene-d8	14.298	160	1522359	40.435	ng/ul	0.01
54) 4-Nitrophenol-d4	14.816	143	79570	12.220	ng/ul	0.02
60) Fluorene-d10	15.592	176	1131938	40.869	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.716	200	80956	14.930	ng/ul	0.00
73) Anthracene-d10	17.451	188	1691494	40.593	ng/ul	0.01
81) Pyrene-d10	19.745	212	1895290	43.285	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.815	264	1717214	42.112	ng/ul	0.02
Target Compounds						Qvalue
18) 4-Methylphenol	8.734	108	17145	1.330	ng/ul	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044444.D
Acq On : 29 Feb 2024 17:53
Operator : MA/JU
Sample : P1512-07
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0SA5

Quant Time: Feb 29 22:33:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 29 03:37:20 2024
Response via : Initial Calibration

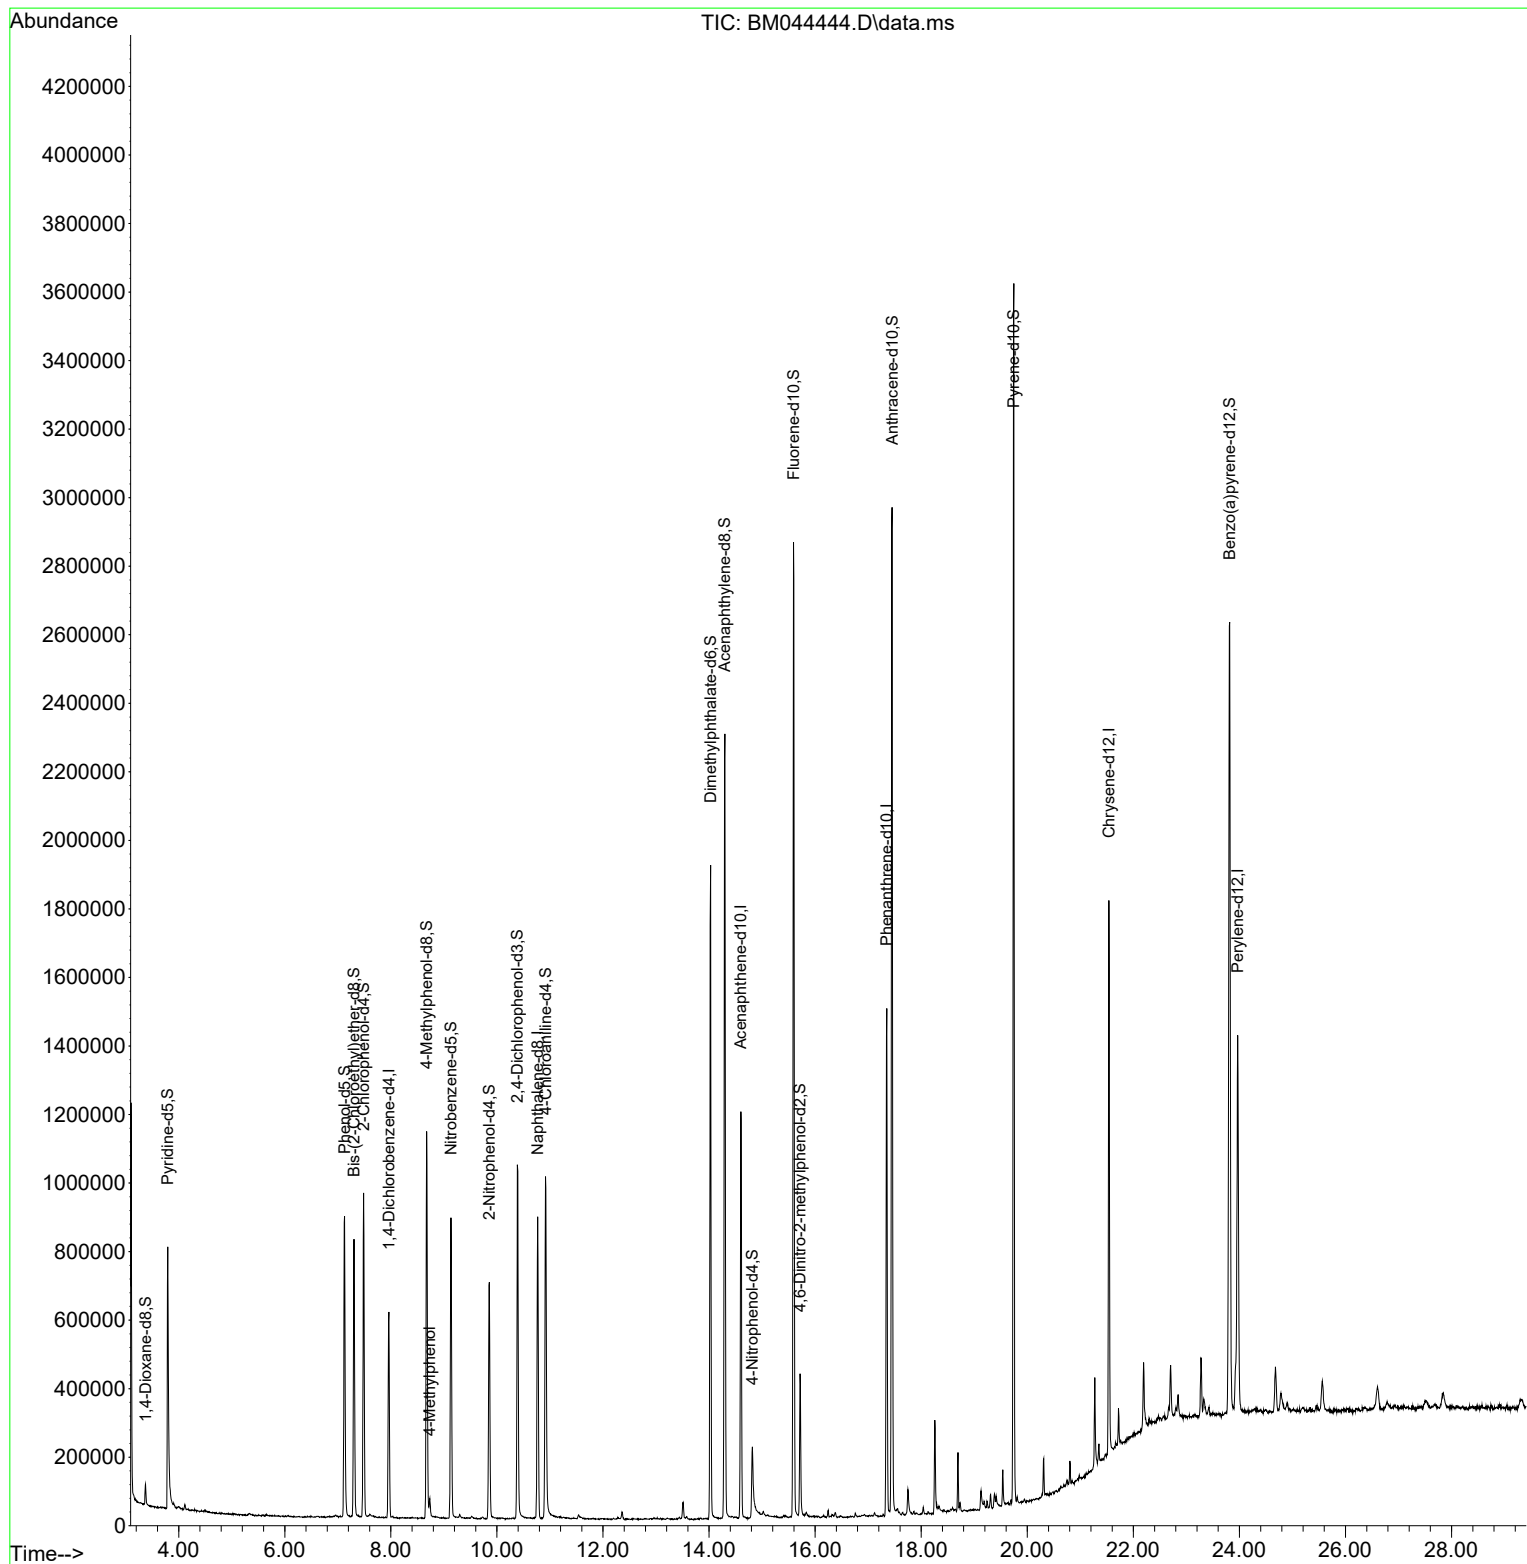

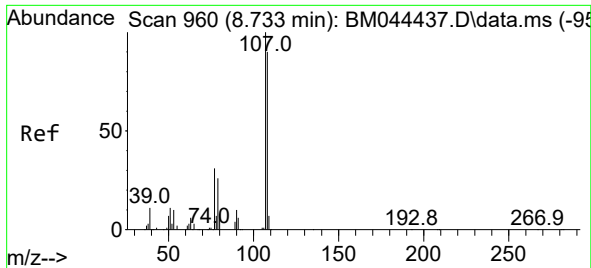

#18
 4-Methylphenol
 Concen: 1.330 ng/ul
 RT: 8.734 min Scan# 90
 Delta R.T. 0.006 min
 Lab File: BM044444.D
 Acq: 29 Feb 2024 17:53

Instrument :
 BNA_M
 ClientSampleId :
 E0SA5

Tgt Ion:108 Resp: 17145
 Ion Ratio Lower Upper
 108 100
 107 126.6 86.8 130.2

