




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044424.D
Acq On : 29 Feb 2024 03:53
Operator : MA/JU
Sample : P1535-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF9

Manual IntegrationsAPPROVED

Quant Time: Feb 29 04:22:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 29 03:37:20 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2024
Supervised By :mohammad ahmed 03/02/2024

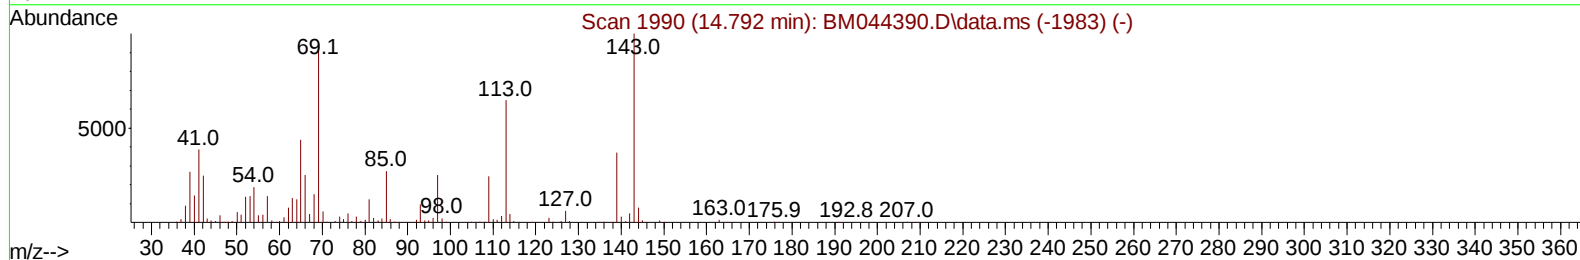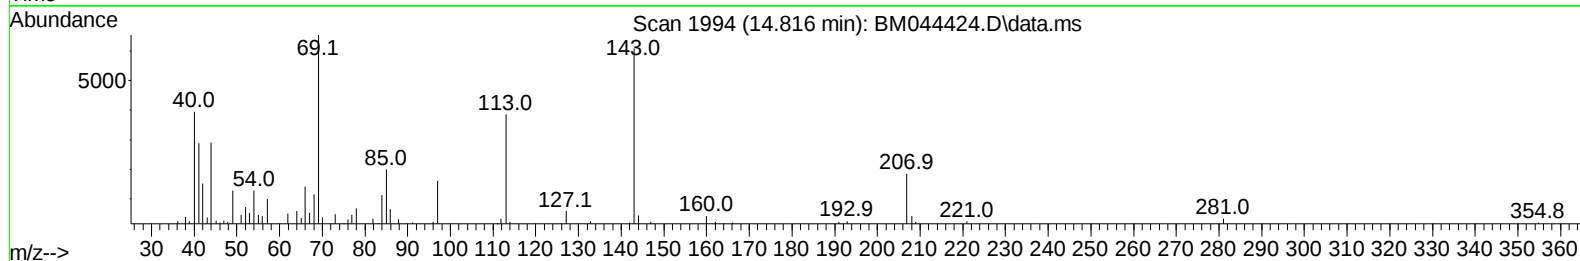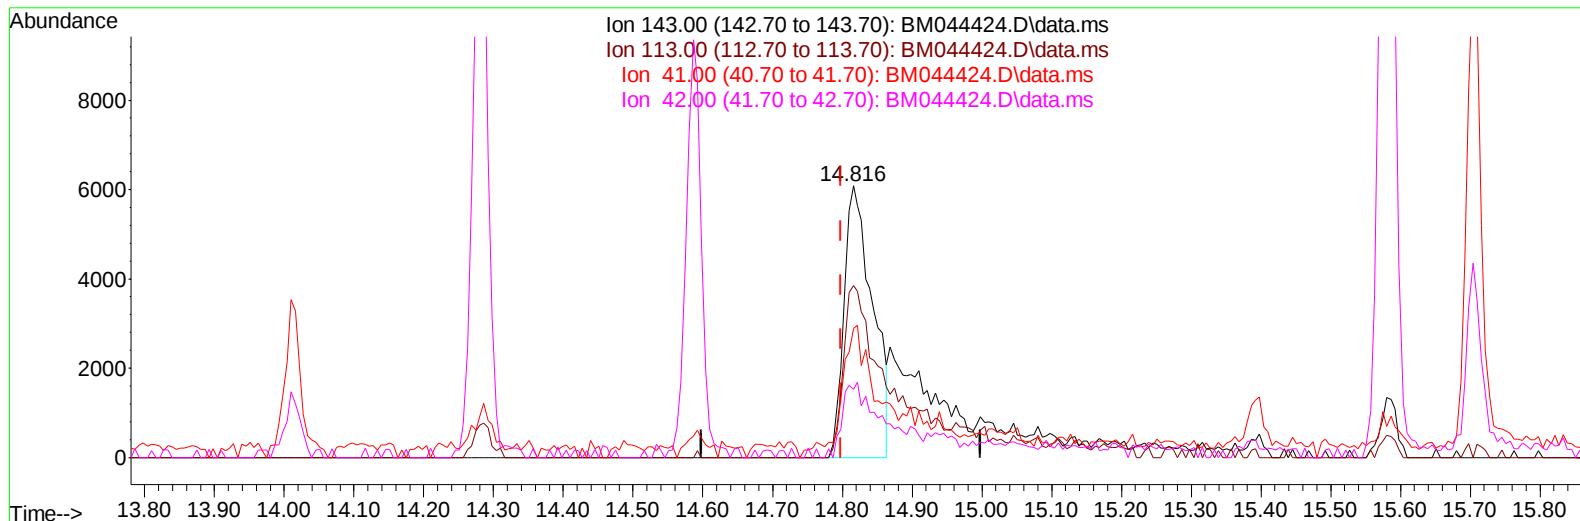

TIC: BM044424.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.816min (+ 0.018) 2.42 ng/u1

response 17206

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	63.27
41.00	38.20	47.57#
42.00	25.30	25.04




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044424.D
 Acq On : 29 Feb 2024 03:53
 Operator : MA/JU
 Sample : P1535-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF9

Manual IntegrationsAPPROVED

Quant Time: Feb 29 04:22:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 29 03:37:20 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2024
 Supervised By :mohammad ahmed 03/02/2024

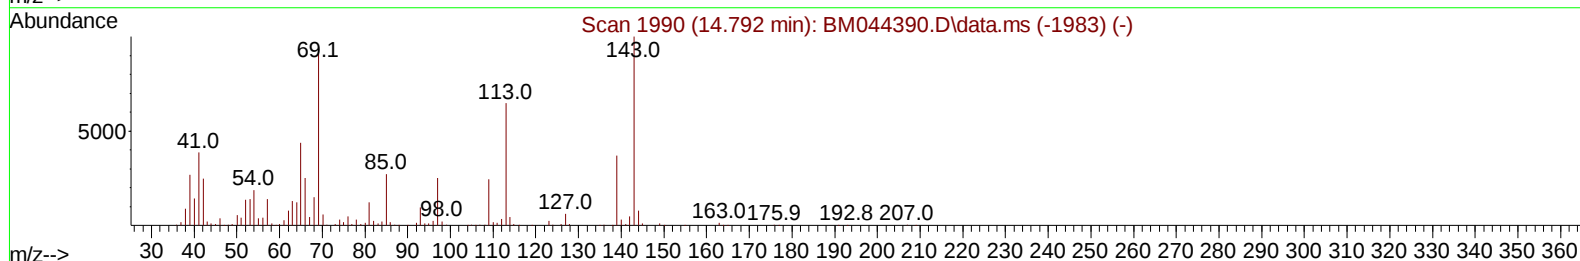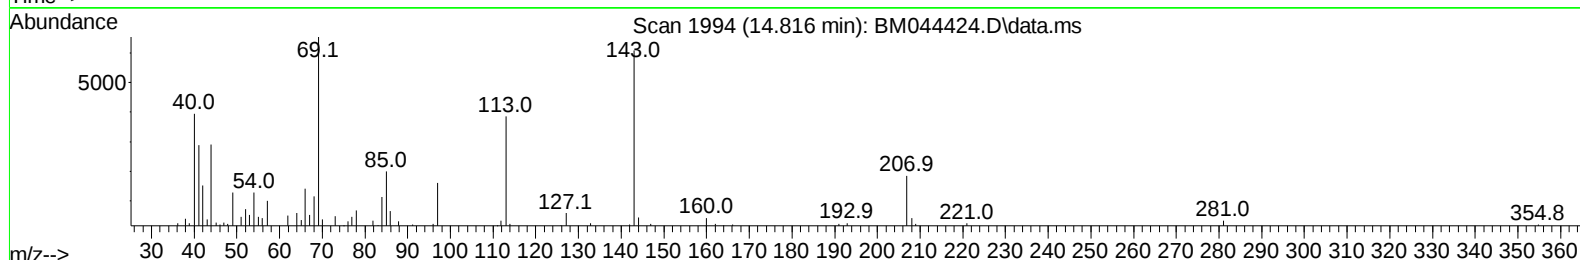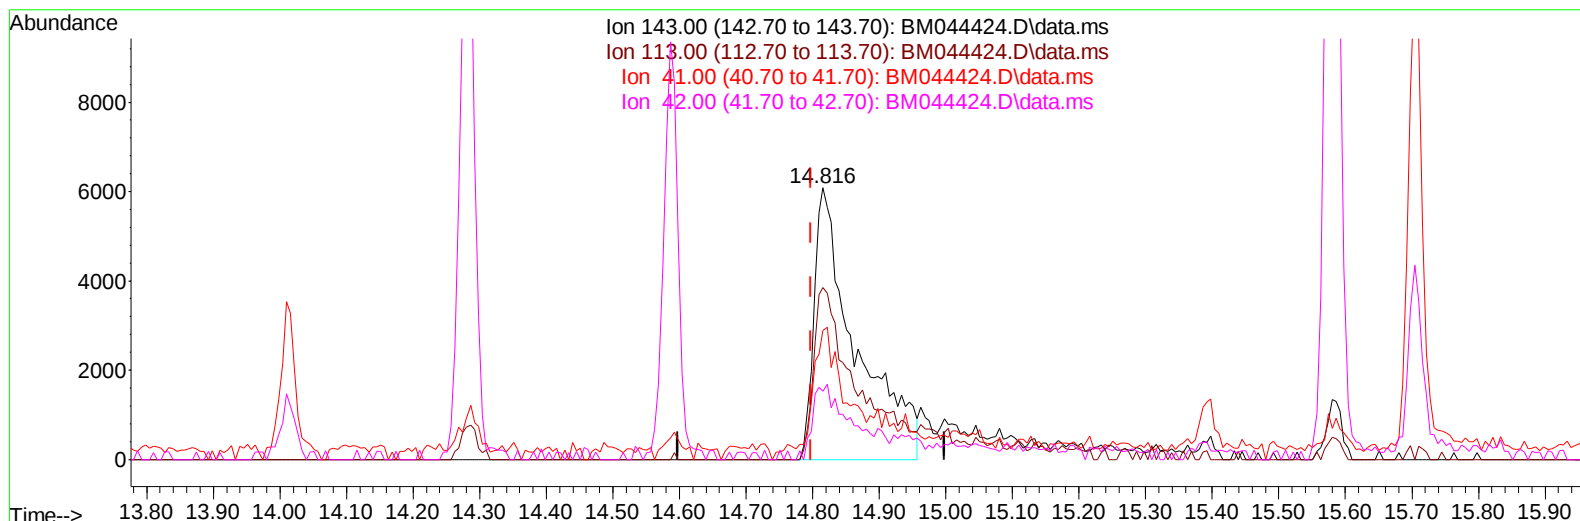

TIC: BM044424.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.816min (+ 0.018) 3.71 ng/ul m

response 26412

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	63.27
41.00	38.20	47.57#
42.00	25.30	25.04

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044424.D
 Acq On : 29 Feb 2024 03:53
 Operator : MA/JU
 Sample : P1535-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/01/2024
 Supervised By :mohammad ahmed 03/02/2024

Quant Time: Feb 29 04:23:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 29 03:37:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	179872	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	794597	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	463274	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	955020	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	768709	20.000	ng/ul	0.00
88) Perylene-d12	23.950	264	848085	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	24455	4.290	ng/uL	0.00
4) Pyridine-d5	3.805	84	51108	3.283	ng/ul	0.02
7) Phenol-d5	7.110	99	115920	6.727	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	401771	36.006	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	350725	27.025	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	211584	16.228	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	246235	38.113	ng/ul	0.00
24) 2-Nitrophenol-d4	9.839	143	228413	34.653	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	359307	30.902	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	176441	9.035	ng/ul	0.00
46) Dimethylphthalate-d6	14.016	166	1444670	40.433	ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	1666982	40.551	ng/ul	0.00
54) 4-Nitrophenol-d4	14.816	143	26412m	3.715	ng/ul	0.02
60) Fluorene-d10	15.580	176	1295530	42.839	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	164298	27.726	ng/ul	0.00
73) Anthracene-d10	17.439	188	2098541	46.085	ng/ul	0.00
81) Pyrene-d10	19.733	212	2349877	50.812	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.797	264	2086019	48.002	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044424.D
Acq On : 29 Feb 2024 03:53
Operator : MA/JU
Sample : P1535-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF9

Manual IntegrationsAPPROVED

Quant Time: Feb 29 04:23:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 29 03:37:20 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2024
Supervised By :mohammad ahmed 03/02/2024

