




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044426.D
Acq On : 29 Feb 2024 05:42
Operator : MA/JU
Sample : P1535-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual IntegrationsAPPROVED

Quant Time: Feb 29 06:11:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 29 03:37:20 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2024
Supervised By :mohammad ahmed 03/02/2024

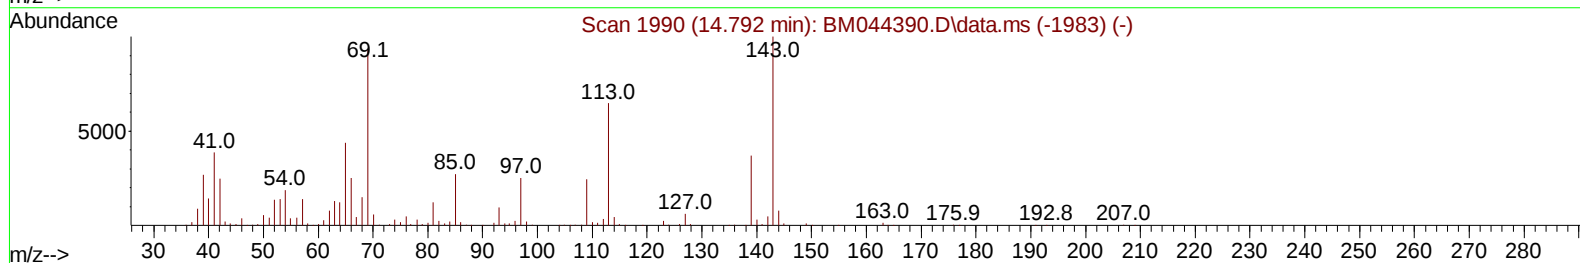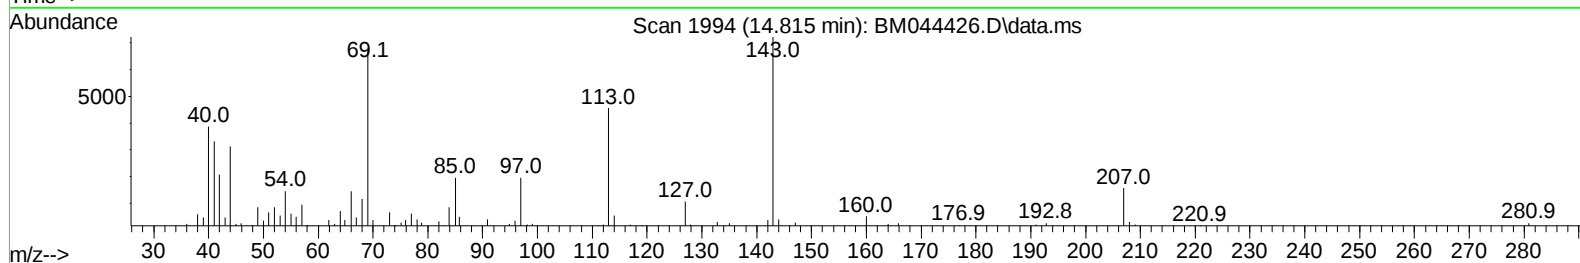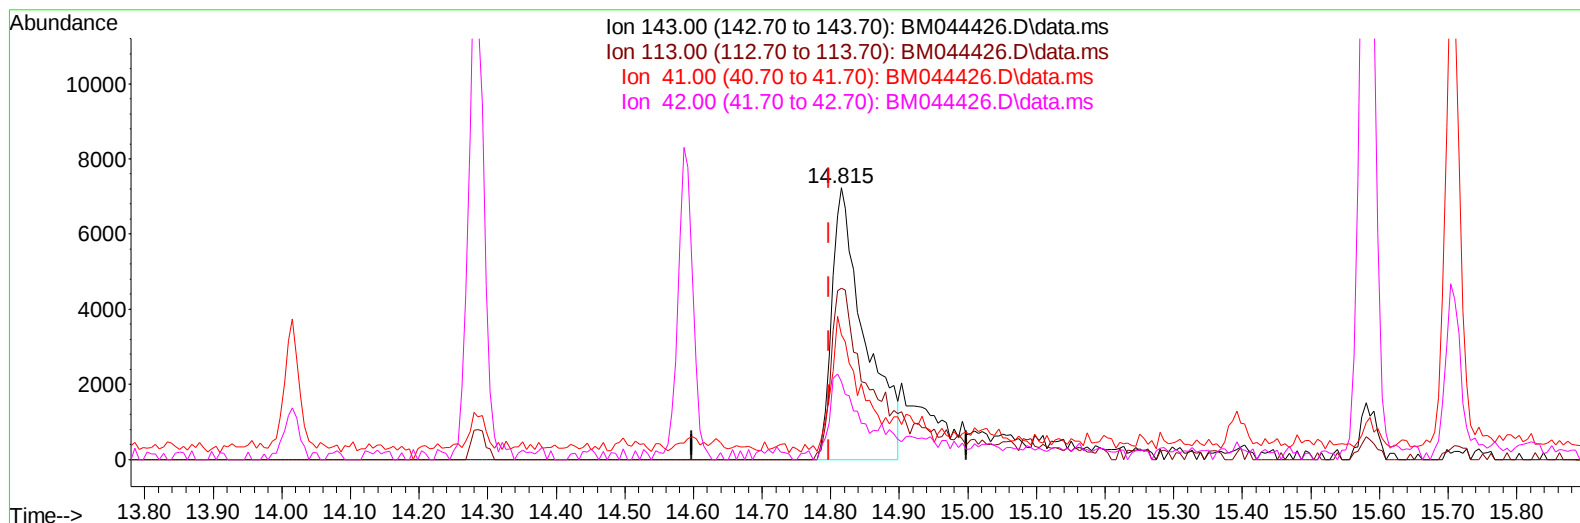

TIC: BM044426.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.815min (+ 0.018) 3.93 ng/u1

response 24128

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	63.11
41.00	38.20	45.90#
42.00	25.30	28.63




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044426.D
 Acq On : 29 Feb 2024 05:42
 Operator : MA/JU
 Sample : P1535-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD0

Manual IntegrationsAPPROVED

Quant Time: Feb 29 06:11:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 29 03:37:20 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2024
 Supervised By :mohammad ahmed 03/02/2024

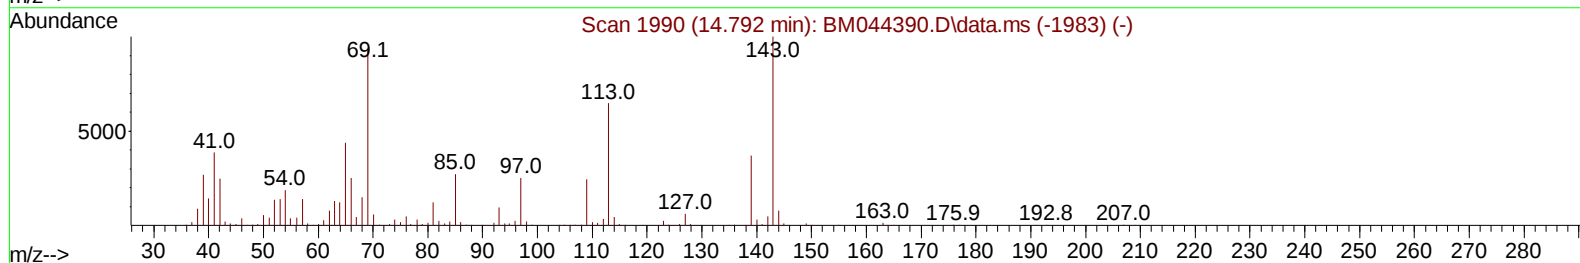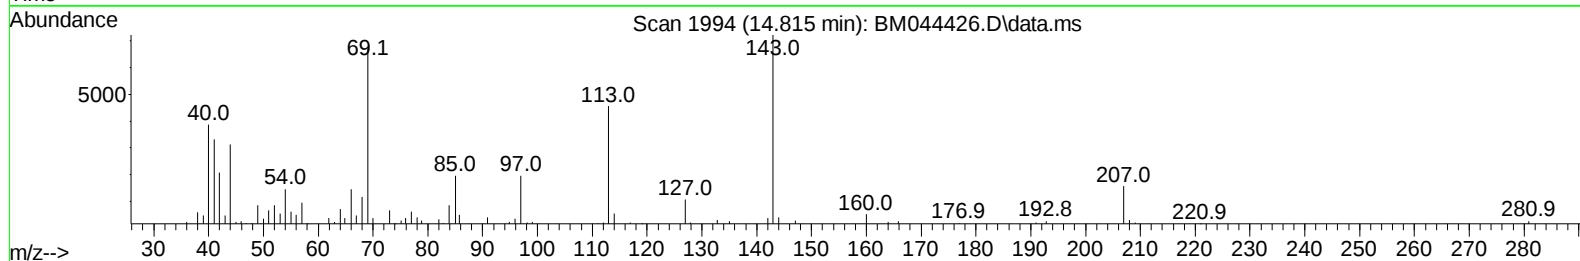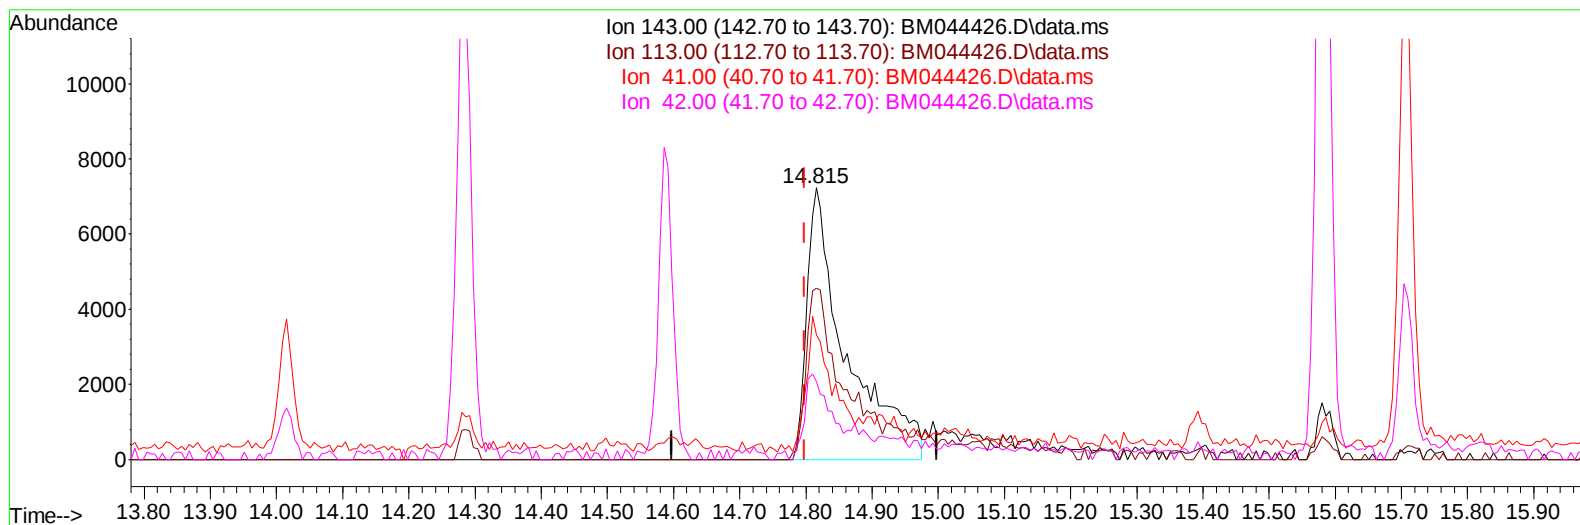

TIC: BM044426.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.815min (+ 0.018) 4.87 ng/ul m

response 29896

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	63.11
41.00	38.20	45.90#
42.00	25.30	28.63

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044426.D
 Acq On : 29 Feb 2024 05:42
 Operator : MA/JU
 Sample : P1535-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/01/2024
 Supervised By :mohammad ahmed 03/02/2024

Quant Time: Feb 29 07:18:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 29 03:37:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	154150	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	691871	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.592	164	399906	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	820797	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	655838	20.000	ng/ul	0.00
88) Perylene-d12	23.956	264	732912	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	23862	4.884	ng/uL	0.00
4) Pyridine-d5	3.804	84	43516	3.261	ng/ul	0.02
7) Phenol-d5	7.116	99	127251	8.617	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.292	67	429472	44.911	ng/ul	0.00
11) 2-Chlorophenol-d4	7.475	132	401380	36.089	ng/ul	0.00
15) 4-Methylphenol-d8	8.663	113	241981	21.657	ng/ul	0.00
21) Nitrobenzene-d5	9.122	128	263824	46.898	ng/ul	0.00
24) 2-Nitrophenol-d4	9.845	143	266624	46.455	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	416856	41.174	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	198037	11.647	ng/ul	0.00
46) Dimethylphthalate-d6	14.015	166	1484558	48.133	ng/ul	0.00
49) Acenaphthylene-d8	14.286	160	1731537	48.795	ng/ul	0.00
54) 4-Nitrophenol-d4	14.815	143	29896m	4.871	ng/ul	0.02
60) Fluorene-d10	15.586	176	1306479	50.047	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	194503	38.191	ng/ul	0.00
73) Anthracene-d10	17.439	188	2149527	54.923	ng/ul	0.00
81) Pyrene-d10	19.733	212	2360812	59.834	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.803	264	2099096	55.894	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044426.D
Acq On : 29 Feb 2024 05:42
Operator : MA/JU
Sample : P1535-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Manual IntegrationsAPPROVED

Quant Time: Feb 29 07:18:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 29 03:37:20 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/01/2024
Supervised By :mohammad ahmed 03/02/2024

