




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044463.D
Acq On : 01 Mar 2024 06:04
Operator : MA/JU
Sample : P1501-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A7

Manual IntegrationsAPPROVED

Quant Time: Mar 01 06:38:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 01 01:46:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2024
Supervised By :mohammad ahmed 03/02/2024

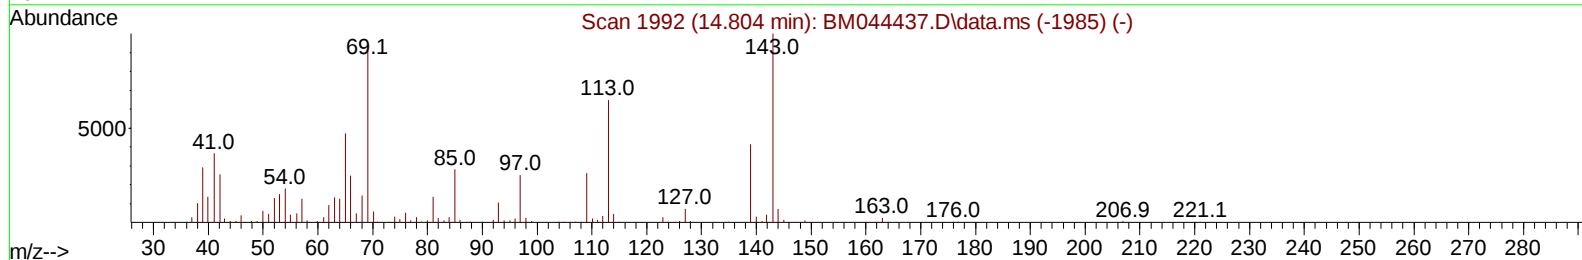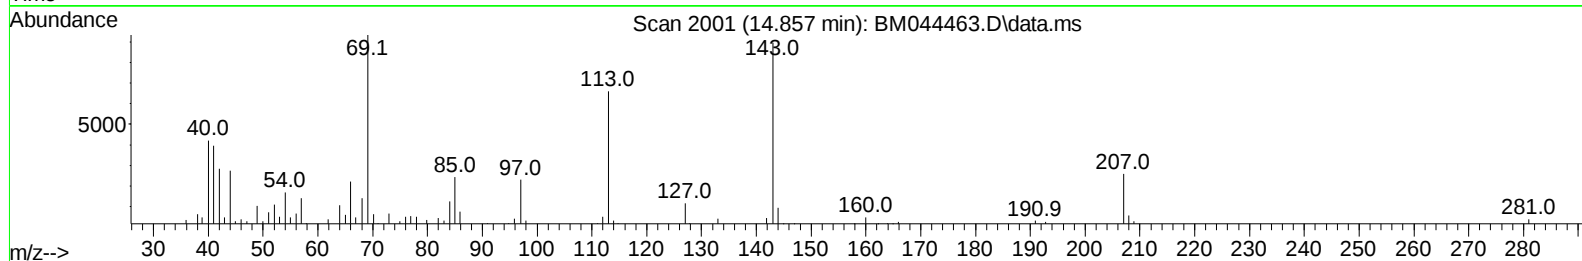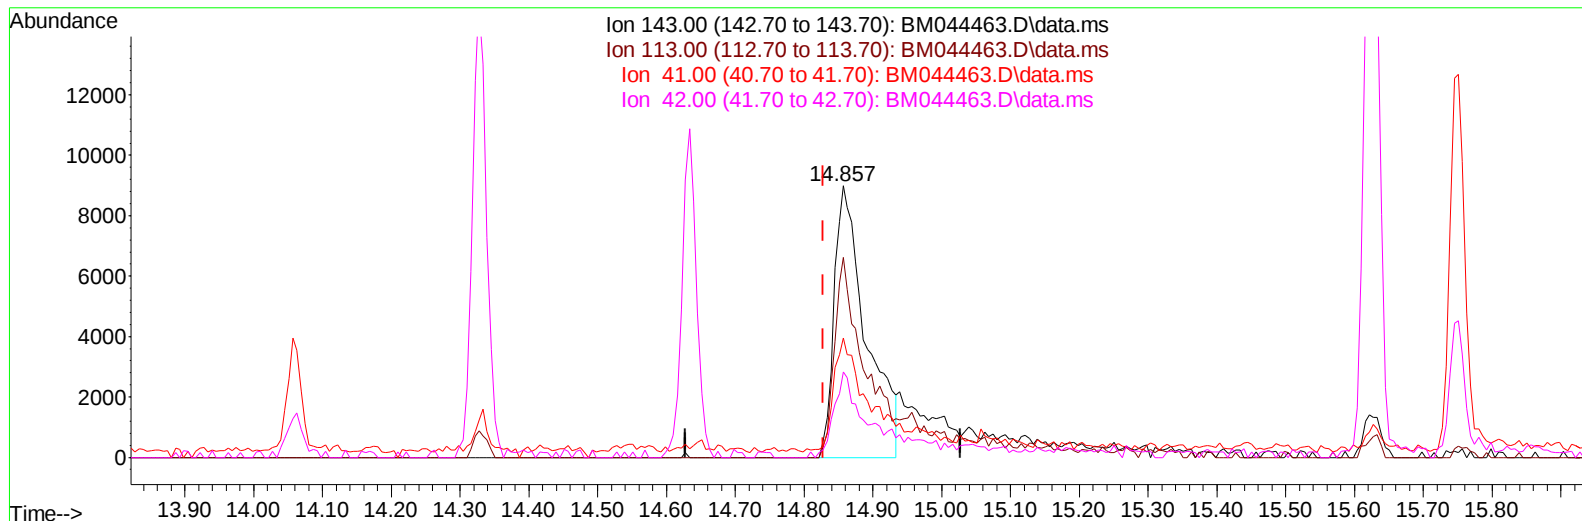

TIC: BM044463.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.857min (+ 0.029) 3.57 ng/u1

response 28983

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	73.59#
41.00	38.20	44.06
42.00	25.30	31.39#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044463.D
Acq On : 01 Mar 2024 06:04
Operator : MA/JU
Sample : P1501-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A7

Manual IntegrationsAPPROVED

Quant Time: Mar 01 06:38:58 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 01 01:46:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2024
Supervised By :mohammad ahmed 03/02/2024

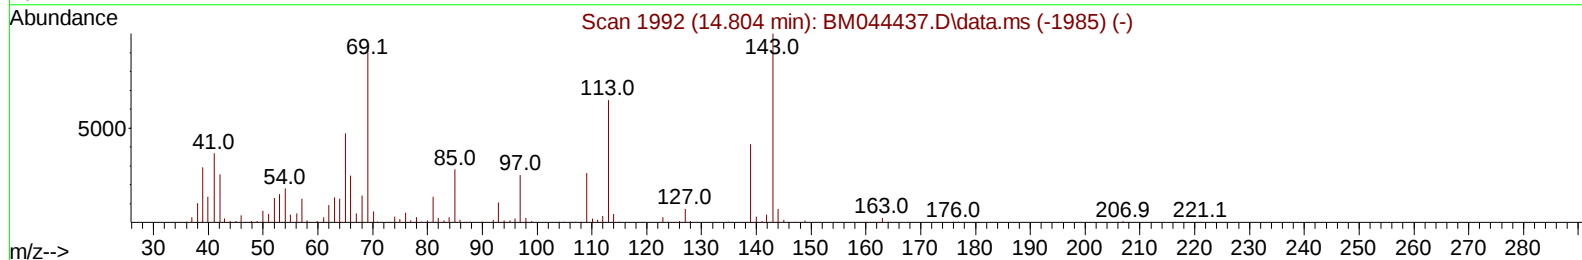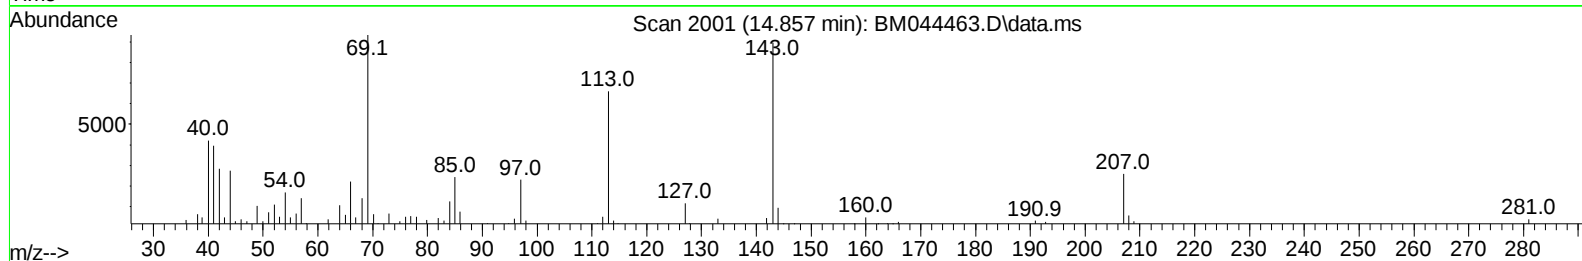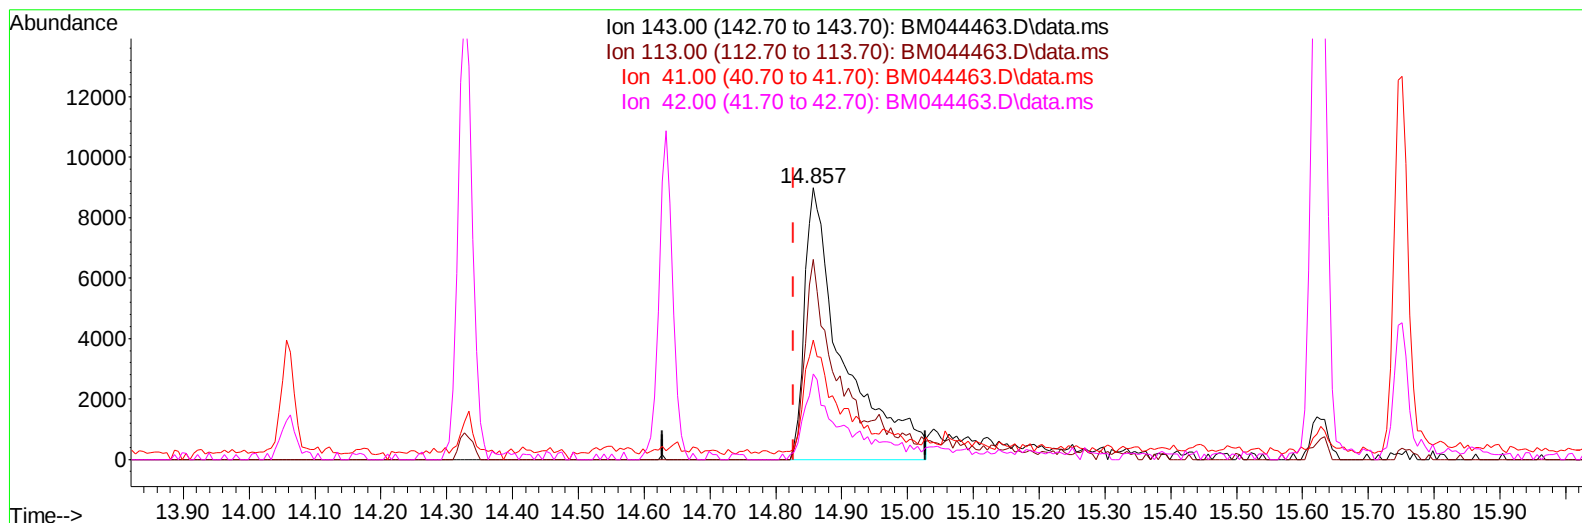

TIC: BM044463.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.857min (+ 0.029) 4.51 ng/ul m

response 36603

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	73.59#
41.00	38.20	44.06
42.00	25.30	31.39#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044463.D
 Acq On : 01 Mar 2024 06:04
 Operator : MA/JU
 Sample : P1501-07
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E10A7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/01/2024
 Supervised By :mohammad ahmed 03/02/2024

Quant Time: Mar 01 06:40:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 01 01:46:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.998	152	201220	20.000	ng/ul	0.02
20) Naphthalene-d8	10.810	136	876672	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.633	164	529118	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.380	188	1054721	20.000	ng/ul	0.01
79) Chrysene-d12	21.568	240	851171	20.000	ng/ul	0.01
88) Perylene-d12	24.015	264	951529	20.000	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	26306	4.125	ng/uL	0.00
4) Pyridine-d5	3.816	84	205430	11.795	ng/ul	0.02
7) Phenol-d5	7.163	99	158354	8.215	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.340	67	465755	37.312	ng/ul	0.02
11) 2-Chlorophenol-d4	7.522	132	453953	31.268	ng/ul	0.02
15) 4-Methylphenol-d8	8.716	113	273557	18.756	ng/ul	0.02
21) Nitrobenzene-d5	9.175	128	287454	40.327	ng/ul	0.02
24) 2-Nitrophenol-d4	9.892	143	293207	40.318	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.428	165	451512	35.196	ng/ul	0.02
31) 4-Chloroaniline-d4	10.957	131	653721	30.342	ng/ul	0.02
46) Dimethylphthalate-d6	14.063	166	1522651	37.313	ng/ul	0.02
49) Acenaphthylene-d8	14.327	160	1844067	39.276	ng/ul	0.01
54) 4-Nitrophenol-d4	14.857	143	36603m	4.508	ng/ul	0.03
60) Fluorene-d10	15.627	176	1380526	39.969	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.751	200	196527	30.030	ng/ul	0.01
73) Anthracene-d10	17.480	188	2170390	43.157	ng/ul	0.01
81) Pyrene-d10	19.768	212	2364732	46.179	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.856	264	2115821	43.395	ng/ul	0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044463.D
Acq On : 01 Mar 2024 06:04
Operator : MA/JU
Sample : P1501-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A7

Manual IntegrationsAPPROVED

Quant Time: Mar 01 06:40:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 01 01:46:17 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/01/2024
Supervised By :mohammad ahmed 03/02/2024

