

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044420.D
 Acq On : 29 Feb 2024 00:50
 Operator : MA/JU
 Sample : PB159332BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS332

Quant Time: Feb 29 01:19:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 23:05:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	189136	20.000	ng/u1	0.01
20) Naphthalene-d8	10.757	136	838496	20.000	ng/u1	0.01
38) Acenaphthene-d10	14.592	164	479279	20.000	ng/u1	0.01
64) Phenanthrene-d10	17.339	188	981496	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	810862	20.000	ng/u1	0.00
88) Perylene-d12	23.956	264	854459	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	39931	6.661	ng/uL	0.00
4) Pyridine-d5	3.781	84	577654	35.284	ng/u1	0.00
7) Phenol-d5	7.116	99	671620	37.068	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.293	67	419397	35.745	ng/u1	0.01
11) 2-Chlorophenol-d4	7.475	132	522690	38.303	ng/u1	0.00
15) 4-Methylphenol-d8	8.669	113	505045	36.839	ng/u1	0.01
21) Nitrobenzene-d5	9.122	128	255295	37.446	ng/u1	0.01
24) 2-Nitrophenol-d4	9.840	143	277920	39.956	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	496119	40.434	ng/u1	0.00
31) 4-Chloroaniline-d4	10.904	131	671542	32.588	ng/u1	0.01
46) Dimethylphthalate-d6	14.016	166	1370577	37.079	ng/u1	0.01
49) Acenaphthylene-d8	14.286	160	1640912	38.583	ng/u1	0.01
54) 4-Nitrophenol-d4	14.798	143	277010	37.661	ng/u1	0.01
60) Fluorene-d10	15.580	176	1185821	37.902	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	222998	36.617	ng/u1	0.00
73) Anthracene-d10	17.439	188	1770379	37.829	ng/u1	0.00
81) Pyrene-d10	19.733	212	1968534	40.353	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.797	264	1771950	40.471	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.399	88	123137	19.488	ng/uL	96
5) Pyridine	3.799	79	893913	52.192	ng/u1	98
6) Benzaldehyde	7.093	77	460260	58.521	ng/u1	98
8) Phenol	7.140	94	1042614	55.359	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.387	93	840968	53.347	ng/u1	99
12) 2-Chlorophenol	7.510	128	812779	57.571	ng/u1	97
13) 2-Methylphenol	8.398	108	771650	55.613	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.481	45	1128284	52.348	ng/u1	98
16) Acetophenone	8.787	105	1223358	55.854	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.775	70	628217	57.257	ng/u1	99
18) 4-Methylphenol	8.734	108	835522	56.528	ng/u1	98
19) Hexachloroethane	9.022	117	331919	55.420	ng/u1	95
22) Nitrobenzene	9.163	77	912769	55.360	ng/u1	100
23) Isophorone	9.692	82	1797175	56.241	ng/u1	99
25) 2-Nitrophenol	9.875	139	452947	58.714	ng/u1	97
26) 2,4-Dimethylphenol	9.934	107	694349	47.137	ng/u1	100
27) Bis(2-Chloroethoxy)met...	10.187	93	1131273	54.458	ng/u1	100
29) 2,4-Dichlorophenol	10.404	162	714312	57.523	ng/u1	99
30) Naphthalene	10.804	128	2575624	54.010	ng/u1	100
32) 4-Chloroaniline	10.928	127	799919	39.835	ng/u1	99
33) Hexachlorobutadiene	11.081	225	410906	54.925	ng/u1	98
34) Caprolactam	11.722	113	250432	58.342	ng/u1	99
35) 4-Chloro-3-methylphenol	12.051	107	798736	60.374	ng/u1	99
36) 2-Methylnaphthalene	12.416	142	1683243	55.416	ng/u1	100


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044420.D
 Acq On : 29 Feb 2024 00:50
 Operator : MA/JU
 Sample : PB159332BS
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SLCS332

Quant Time: Feb 29 01:19:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 23:05:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.633	142	1652754	55.042	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.781	216	790375	55.707	ng/ul	97
40) Hexachlorocyclopentadiene	12.751	237	441077	46.207	ng/ul	99
41) 2,4,6-Trichlorophenol	13.028	196	518067	57.285	ng/ul	98
42) 2,4,5-Trichlorophenol	13.098	196	573208	58.631	ng/ul	99
43) 1,1'-Biphenyl	13.433	154	2115137	54.208	ng/ul	98
44) 2-Chloronaphthalene	13.469	162	1683260	55.095	ng/ul	99
45) 2-Nitroaniline	13.686	65	524943	62.059	ng/ul	97
47) Dimethylphthalate	14.063	163	2091015	55.348	ng/ul	100
48) 2,6-Dinitrotoluene	14.186	165	429071	60.730	ng/ul	99
50) Acenaphthylene	14.316	152	2797906	55.542	ng/ul	99
51) 3-Nitroaniline	14.510	138	466379	62.572	ng/ul	96
52) Acenaphthene	14.657	153	1815134	54.582	ng/ul	99
53) 2,4-Dinitrophenol	14.716	184	230275	52.525	ng/ul	100
55) 4-Nitrophenol	14.816	109	283350	56.076	ng/ul	96
56) Dibenzofuran	14.992	168	2422923	54.274	ng/ul	99
57) 2,4-Dinitrotoluene	14.969	165	625575	61.633	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.216	232	438092	55.681	ng/ul	97
59) Diethylphthalate	15.427	149	2176508	55.969	ng/ul	99
61) Fluorene	15.639	166	1950643	54.402	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.639	204	927669	54.897	ng/ul	99
63) 4-Nitroaniline	15.674	138	492888	68.371	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.727	198	352406	52.898	ng/ul	97
67) N-Nitrosodiphenylamine	15.857	169	1668703	56.103	ng/ul	99
68) 4-Bromophenyl-phenylether	16.533	248	563212	57.754	ng/ul	99
69) Hexachlorobenzene	16.633	284	633208	56.731	ng/ul	97
70) Atrazine	16.816	200	324025	33.256	ng/ul	99
71) Pentachlorophenol	16.980	266	373819	50.822	ng/ul	99
72) Phenanthrene	17.380	178	3104269	55.133	ng/ul	100
74) Anthracene	17.474	178	3132477	55.256	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.386	216	786110	57.217	ng/ul	98
76) Pentachlorobenzene	14.904	250	737143	56.202	ng/ul	98
77) Carbazole	17.751	167	2951283	55.366	ng/ul	100
78) Di-n-butylphthalate	18.327	149	4026905	59.665	ng/ul	100
80) Fluoranthene	19.398	202	3474165	59.381	ng/ul	99
82) Pyrene	19.762	202	3615666	58.928	ng/ul	99
83) Butylbenzylphthalate	20.680	149	1835778	66.613	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.456	252	1037045	57.178	ng/ul	100
85) Benzo(a)anthracene	21.521	228	3458110	57.182	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.462	149	2758019	65.366	ng/ul	99
87) Chrysene	21.574	228	3230334	56.826	ng/ul	99
89) Di-n-octyl phthalate	22.409	149	4815514	65.778	ng/ul	100
90) Benzo(b)fluoranthene	23.221	252	3385552	61.805	ng/ul	100
91) Benzo(k)fluoranthene	23.268	252	3287454	58.432	ng/ul	99
93) Benzo(a)pyrene	23.850	252	3159381	59.822	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.491	276	3761093	58.889	ng/ul	99
95) Dibenzo(a,h)anthracene	26.521	278	3168312	59.363	ng/ul	99
96) Benzo(g,h,i)perylene	27.268	276	3024118	58.536	ng/ul	98





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 19.488 ng/uL
RT: 3.399 min Scan# 51
Delta R.T. 0.000 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion: 88 Resp: 123137
Ion Ratio Lower Upper
88 100
43 29.1 21.2 31.8
58 75.4 58.3 87.5

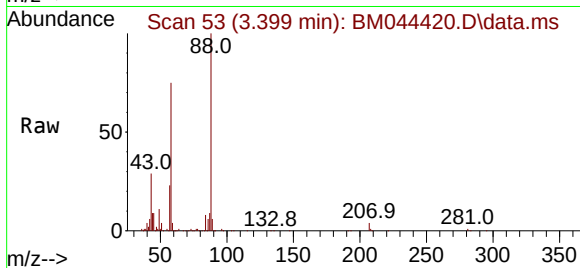

#5
Pyridine
Concen: 52.192 ng/uL
RT: 3.799 min Scan# 121
Delta R.T. 0.000 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion: 79 Resp: 893913
Ion Ratio Lower Upper
79 100
52 72.1 58.9 88.3
51 33.9 27.8 41.8




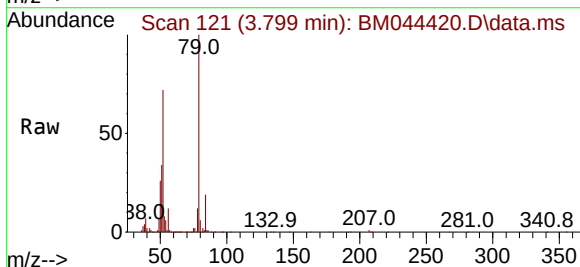




#6
Benzaldehyde
Concen: 58.521 ng/ul
RT: 7.093 min Scan# 681
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion: 77 Resp: 460260
Ion Ratio Lower Upper
77 100
105 96.7 79.0 118.6
106 94.7 77.4 116.2



#8
Phenol
Concen: 55.359 ng/ul
RT: 7.140 min Scan# 689
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion: 94 Resp: 1042614
Ion Ratio Lower Upper
94 100
65 26.7 20.6 31.0
66 31.9 25.4 38.0









#10
Bis(2-Chloroethyl)ether
Concen: 53.347 ng/ul
RT: 7.387 min Scan# 731
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion: 93 Resp: 840968
Ion Ratio Lower Upper
93 100
63 75.8 61.0 91.6
95 32.9 25.1 37.7



#12
2-Chlorophenol
Concen: 57.571 ng/ul
RT: 7.510 min Scan# 752
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:128 Resp: 812779
Ion Ratio Lower Upper
128 100
64 46.2 39.0 58.6
130 32.6 25.4 38.0









#13
2-Methylphenol
Concen: 55.613 ng/ul
RT: 8.398 min Scan# 903
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:108 Resp: 771650
Ion Ratio Lower Upper
108 100
107 88.7 70.6 105.8

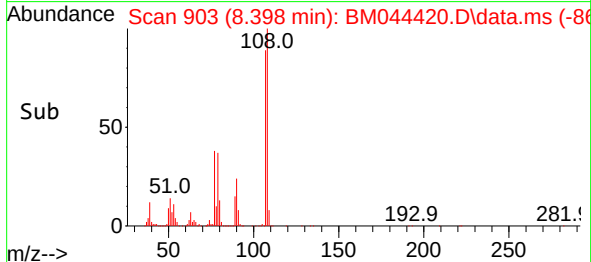

#14
2,2'-oxybis(1-Chloropropane)
Concen: 52.348 ng/ul
RT: 8.481 min Scan# 917
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion: 45 Resp: 1128284
Ion Ratio Lower Upper
45 100
77 15.3 11.3 16.9
79 10.8 8.5 12.7









#16
Acetophenone
Concen: 55.854 ng/ul
RT: 8.787 min Scan# 969
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:105 Resp: 1223358
Ion Ratio Lower Upper
105 100
77 76.2 61.2 91.8
51 25.6 21.1 31.7



#17
N-Nitroso-di-n-propylamine
Concen: 57.257 ng/ul
RT: 8.775 min Scan# 967
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion: 70 Resp: 628217
Ion Ratio Lower Upper
70 100
42 54.4 44.4 66.6
101 9.1 7.5 11.3
130 20.9 17.0 25.4



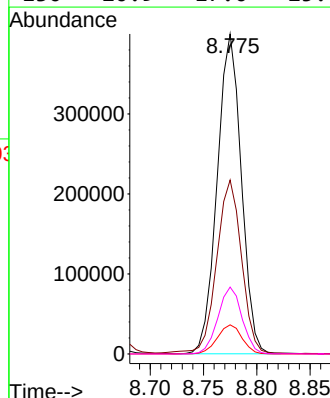





#18
4-Methylphenol
Concen: 56.528 ng/ul
RT: 8.734 min Scan# 90
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:108 Resp: 835522
Ion Ratio Lower Upper
108 100
107 106.3 86.8 130.2

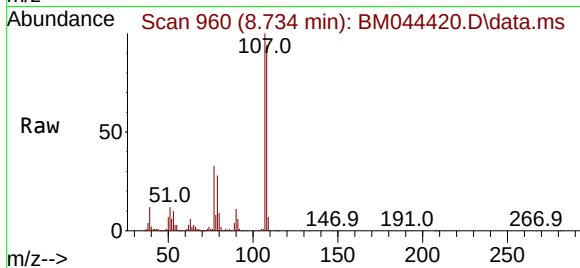

#19
Hexachloroethane
Concen: 55.420 ng/ul
RT: 9.022 min Scan# 1009
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:117 Resp: 331919
Ion Ratio Lower Upper
117 100
201 89.3 69.8 104.6
199 56.9 40.8 61.2

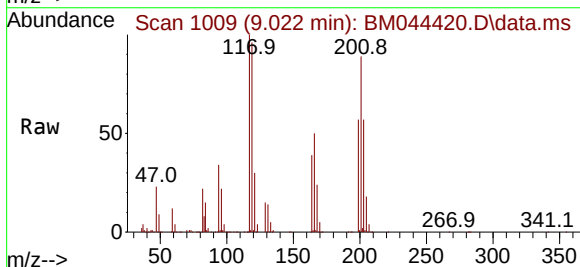



#22

Nitrobenzene

Concen: 55.360 ng/ul

RT: 9.163 min Scan# 1033

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion: 77 Resp: 912769

Ion Ratio Lower Upper

77 100

123 45.9 36.9 55.3

65 12.6 10.2 15.2

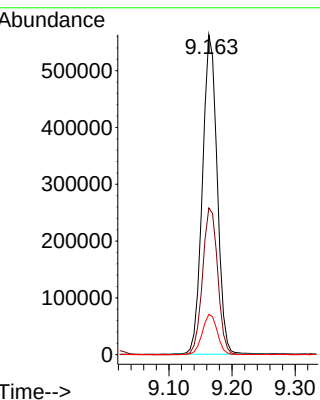

#23

Isophorone

Concen: 56.241 ng/ul

RT: 9.692 min Scan# 1123

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion: 82 Resp: 1797175


Ion Ratio Lower Upper

82 100

95 6.1 4.6 7.0

138 17.1 13.5 20.3



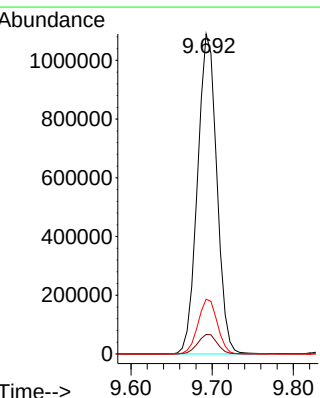





#25
2-Nitrophenol
Concen: 58.714 ng/ul
RT: 9.875 min Scan# 1154
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:139 Resp: 452947
Ion Ratio Lower Upper
139 100
65 48.4 41.0 61.4
109 25.7 20.5 30.7



#26
2,4-Dimethylphenol
Concen: 47.137 ng/ul
RT: 9.934 min Scan# 1164
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:107 Resp: 694349
Ion Ratio Lower Upper
107 100
121 51.0 41.1 61.7
122 90.1 72.3 108.5

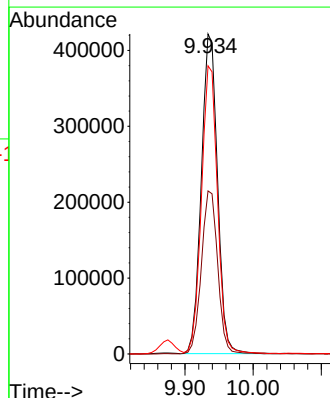



#27

Bis(2-Chloroethoxy)methane

Concen: 54.458 ng/ul

RT: 10.187 min Scan# 1

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion: 93 Resp: 1131273

Ion Ratio Lower Upper

93 100

95 32.6 26.0 39.0

123 11.3 9.0 13.6

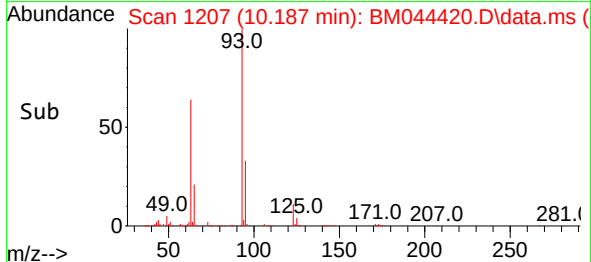

#29

2,4-Dichlorophenol

Concen: 57.523 ng/ul

RT: 10.404 min Scan# 1244

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion:162 Resp: 714312


Ion Ratio Lower Upper

162 100

164 65.7 51.8 77.8

98 37.0 29.6 44.4









#30
Naphthalene
Concen: 54.010 ng/ul
RT: 10.804 min Scan# 1312
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:128 Resp: 2575624
Ion Ratio Lower Upper
128 100
129 11.1 8.8 13.2
127 12.6 10.2 15.2

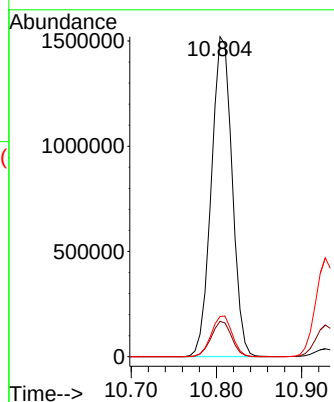

#32
4-Chloroaniline
Concen: 39.835 ng/ul
RT: 10.928 min Scan# 1333
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:127 Resp: 799919
Ion Ratio Lower Upper
127 100
129 32.1 25.3 37.9



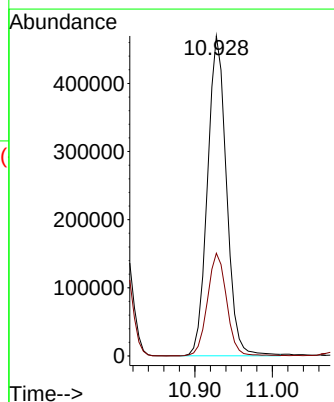





#33
Hexachlorobutadiene
Concen: 54.925 ng/ul
RT: 11.081 min Scan# 11
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:225 Resp: 410906
Ion Ratio Lower Upper
225 100
223 62.3 49.7 74.5
227 62.8 52.2 78.2



#34
Caprolactam
Concen: 58.342 ng/ul
RT: 11.722 min Scan# 1468
Delta R.T. 0.024 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:113 Resp: 250432
Ion Ratio Lower Upper
113 100
55 173.3 140.7 211.1
56 127.4 102.4 153.6









#35
 4-Chloro-3-methylphenol
 Concen: 60.374 ng/ul
 RT: 12.051 min Scan# 1524
 Delta R.T. 0.012 min
 Lab File: BM044420.D
 Acq: 29 Feb 2024 00:50




Instrument :
 BNA_M
 ClientSampleId :
 SLCS332


Tgt Ion:107 Resp: 798736
 Ion Ratio Lower Upper
 107 100
 144 26.3 20.6 30.8
 142 81.7 64.3 96.5

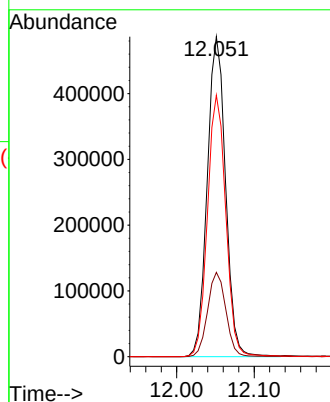

#36
 2-Methylnaphthalene
 Concen: 55.416 ng/ul
 RT: 12.416 min Scan# 1586
 Delta R.T. 0.006 min
 Lab File: BM044420.D
 Acq: 29 Feb 2024 00:50

Tgt Ion:142 Resp: 1683243
 Ion Ratio Lower Upper
 142 100
 141 88.5 70.5 105.7

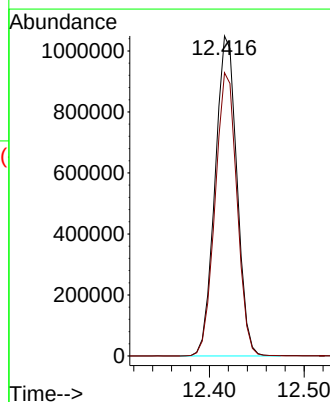



#37

1-Methylnaphthalene

Concen: 55.042 ng/ul

RT: 12.633 min Scan# 1

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:142 Resp: 1652754

Ion Ratio Lower Upper

142 100

141 91.0 73.0 109.4

116 3.7 2.7 4.1

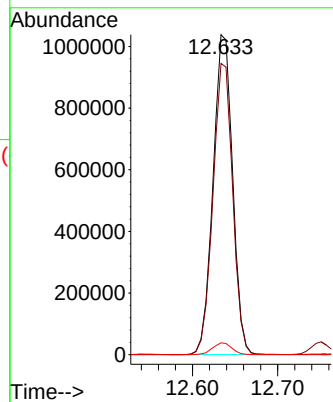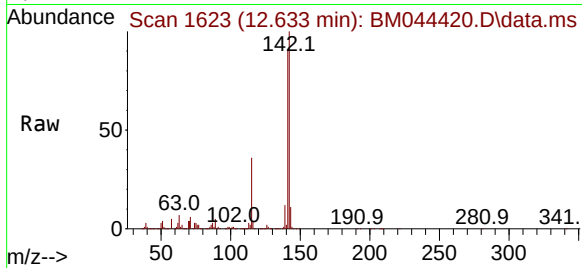

#39

1,2,4,5-Tetrachlorobenzene

Concen: 55.707 ng/ul

RT: 12.781 min Scan# 1648

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Tgt Ion:216 Resp: 790375




Ion Ratio Lower Upper


216 100

214 77.6 63.9 95.9

179 21.0 17.5 26.3

108 18.5 16.2 24.4



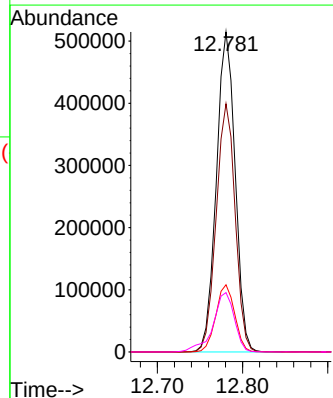
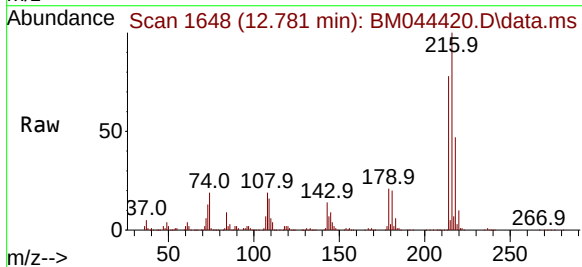




#40
Hexachlorocyclopentadiene
Concen: 46.207 ng/ul
RT: 12.751 min Scan# 1643
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:237 Resp: 441077
Ion Ratio Lower Upper
237 100
235 62.8 49.4 74.2
272 12.7 10.6 16.0

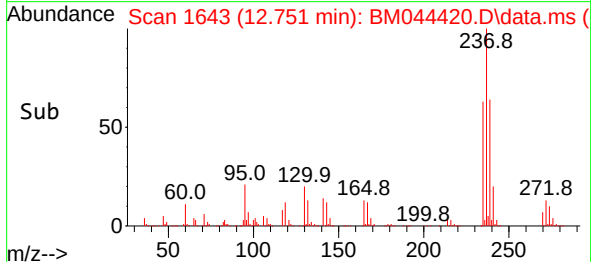

#41
2,4,6-Trichlorophenol
Concen: 57.285 ng/ul
RT: 13.028 min Scan# 1690
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:196 Resp: 518067
Ion Ratio Lower Upper
196 100
198 97.1 76.1 114.1
200 31.4 25.1 37.7





#42

2,4,5-Trichlorophenol

Concen: 58.631 ng/ul

RT: 13.098 min Scan# 1

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:196 Resp: 573208

Ion Ratio Lower Upper

196 100

198 96.5 77.4 116.2

200 31.1 25.6 38.4



#43

1,1'-Biphenyl

Concen: 54.208 ng/ul

RT: 13.433 min Scan# 1759

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion:154 Resp: 2115137


Ion Ratio Lower Upper

154 100

153 39.4 32.4 48.6

76 13.5 11.6 17.4



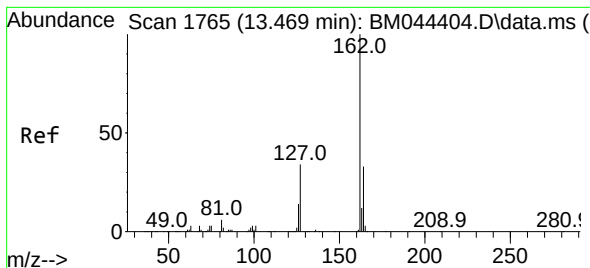

#44

2-Chloronaphthalene

Concen: 55.095 ng/ul

RT: 13.469 min Scan# 1765

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:162 Resp: 1683260

Ion Ratio Lower Upper

162 100

164 32.6 26.1 39.1

127 39.4 30.9 46.3

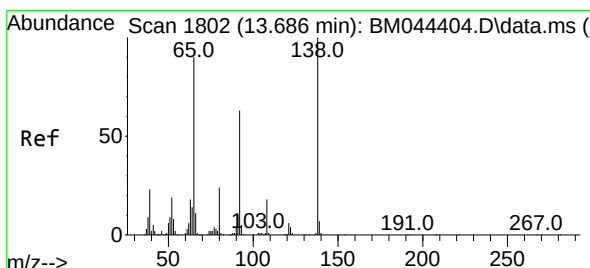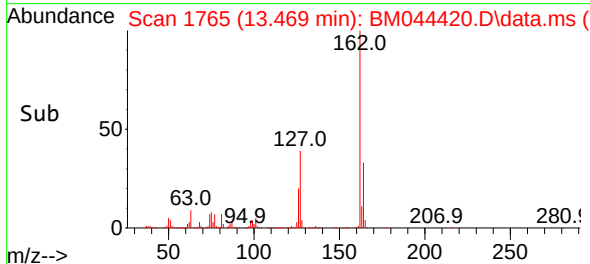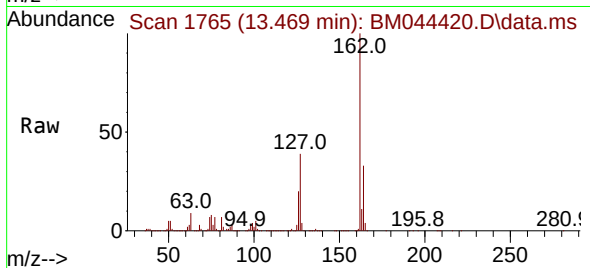

#45

2-Nitroaniline

Concen: 62.059 ng/ul

RT: 13.686 min Scan# 1802

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion: 65 Resp: 524943


Ion Ratio Lower Upper

65 100

92 69.3 52.5 78.7

138 109.4 86.4 129.6


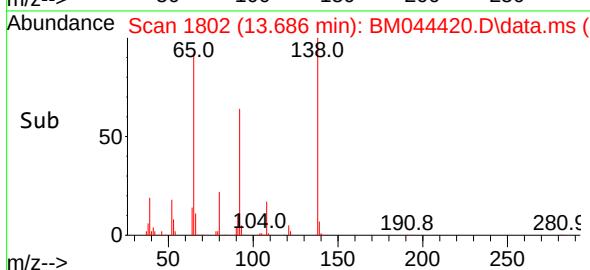

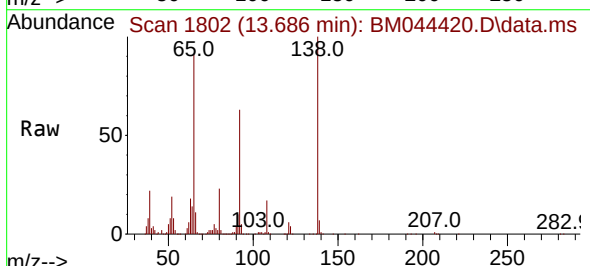


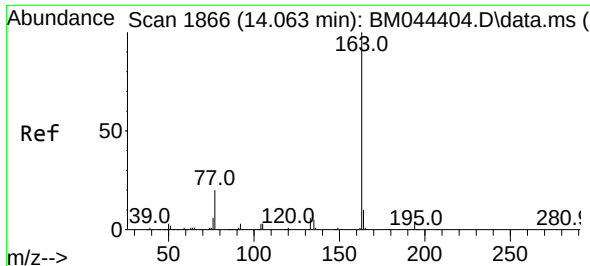

#47
Dimethylphthalate
Concen: 55.348 ng/ul
RT: 14.063 min Scan# 1866
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:163 Resp: 2091015
Ion Ratio Lower Upper
163 100
194 3.8 3.0 4.6
164 10.2 8.1 12.1

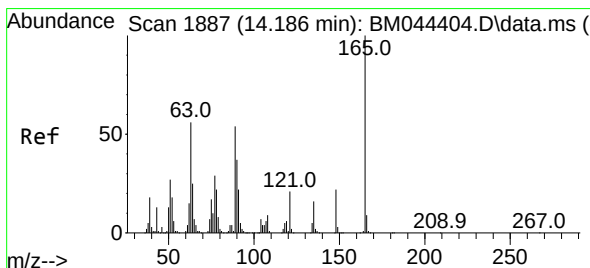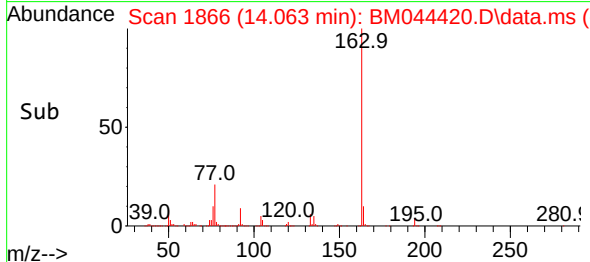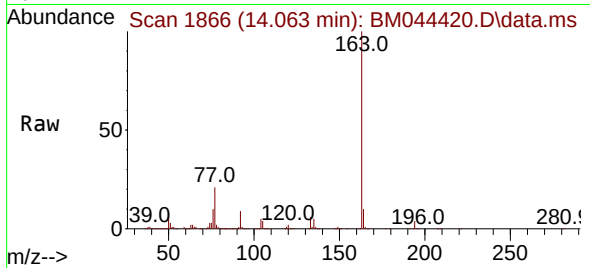

#48
2,6-Dinitrotoluene
Concen: 60.730 ng/ul
RT: 14.186 min Scan# 1887
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:165 Resp: 429071
Ion Ratio Lower Upper
165 100
89 59.9 48.2 72.2
121 21.7 18.7 28.1

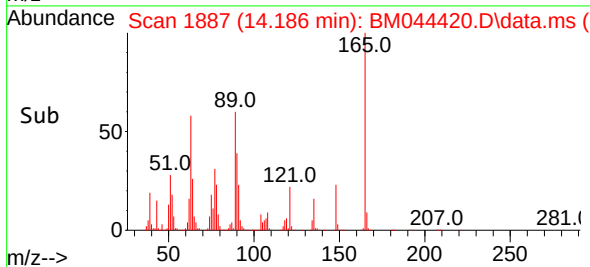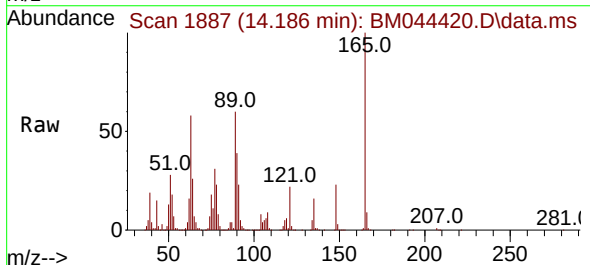



#50

Acenaphthylene

Concen: 55.542 ng/ul

RT: 14.316 min Scan# 1908

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:152 Resp: 2797906

Ion Ratio Lower Upper

152 100

151 20.3 15.8 23.6

153 13.4 10.4 15.6

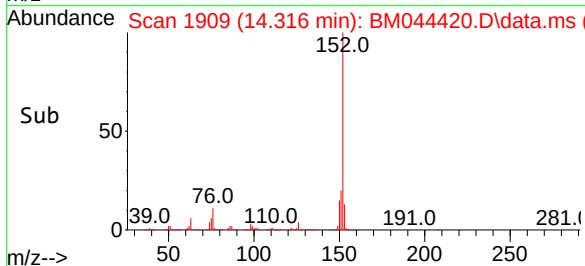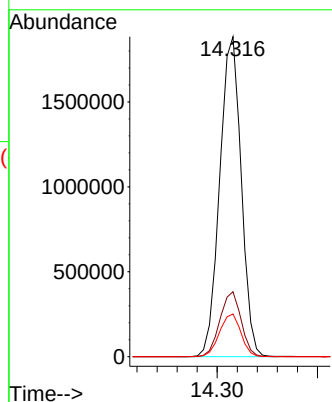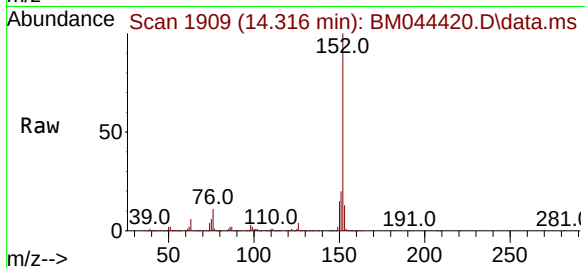

#51

3-Nitroaniline

Concen: 62.572 ng/ul

RT: 14.510 min Scan# 1942

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion:138 Resp: 466379


Ion Ratio Lower Upper

138 100

108 8.9 8.6 12.8

92 112.4 93.8 140.6

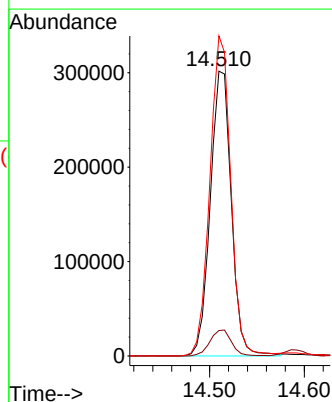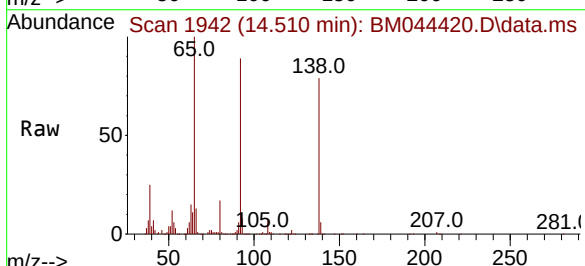



#52

Acenaphthene

Concen: 54.582 ng/ul

RT: 14.657 min Scan# 1966

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:153 Resp: 1815134

Ion Ratio Lower Upper

153 100

152 47.8 38.5 57.7

154 88.0 70.8 106.2

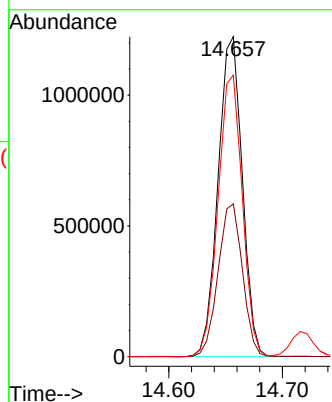

#53

2,4-Dinitrophenol

Concen: 52.525 ng/ul

RT: 14.716 min Scan# 1977

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion:184 Resp: 230275


Ion Ratio Lower Upper

184 100

63 72.9 58.4 87.6

154 58.4 46.4 69.6





#55

4-Nitrophenol

Concen: 56.076 ng/ul

RT: 14.816 min Scan# 1993

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:109 Resp: 283350

Ion Ratio Lower Upper

109 100

139 158.8 123.0 184.6

65 147.7 122.2 183.2

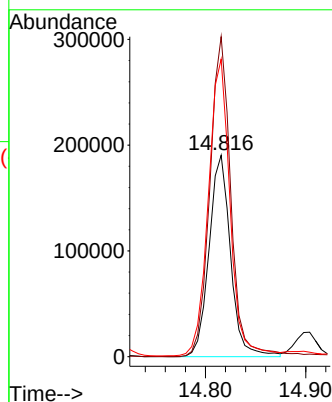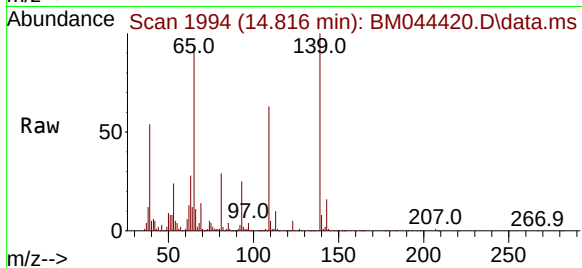

#56

Dibenzofuran

Concen: 54.274 ng/ul

RT: 14.992 min Scan# 2024

Delta R.T. 0.012 min

Lab File: BM044420.D




Acq: 29 Feb 2024 00:50


Tgt Ion:168 Resp: 2422923

Ion Ratio Lower Upper

168 100

139 37.8 29.9 44.9




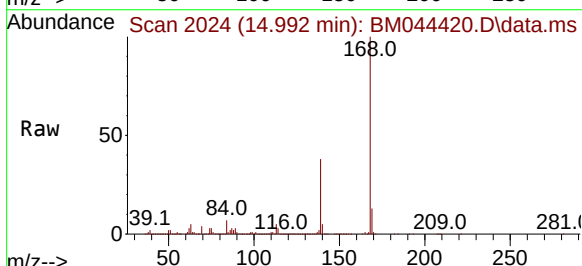




#57
 2,4-Dinitrotoluene
 Concen: 61.633 ng/ul
 RT: 14.969 min Scan# 2020
 Delta R.T. 0.012 min
 Lab File: BM044420.D
 Acq: 29 Feb 2024 00:50




Instrument :
 BNA_M
 ClientSampleId :
 SLCS332


Tgt Ion:165 Resp: 625575
 Ion Ratio Lower Upper
 165 100
 63 46.4 37.9 56.9
 182 2.5 1.8 2.6



#58
 2,3,4,6-Tetrachlorophenol
 Concen: 55.681 ng/ul
 RT: 15.216 min Scan# 2062
 Delta R.T. 0.012 min
 Lab File: BM044420.D
 Acq: 29 Feb 2024 00:50

Tgt Ion:232 Resp: 438092
 Ion Ratio Lower Upper
 232 100
 131 50.1 41.9 62.9
 130 2.5 1.8 2.8
 166 32.6 26.9 40.3









#59
Diethylphthalate
Concen: 55.969 ng/ul
RT: 15.427 min Scan# 2097
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:149 Resp: 2176508
Ion Ratio Lower Upper
149 100
177 20.7 17.0 25.6
150 12.2 9.6 14.4

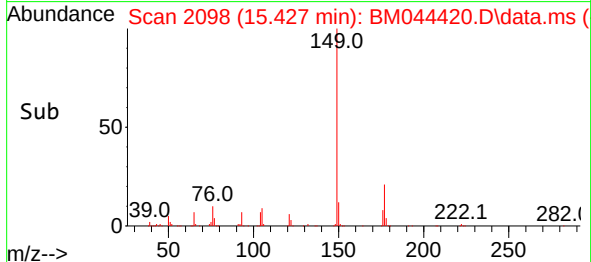

#61
Fluorene
Concen: 54.402 ng/ul
RT: 15.639 min Scan# 2134
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:166 Resp: 1950643
Ion Ratio Lower Upper
166 100
165 95.8 77.4 116.0
167 13.7 10.8 16.2









#62
4-Chlorophenyl-phenylether
Concen: 54.897 ng/ul
RT: 15.639 min Scan# 2134
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:204 Resp: 927669
Ion Ratio Lower Upper
204 100
206 32.5 26.9 40.3
141 59.7 48.3 72.5



#63
4-Nitroaniline
Concen: 68.371 ng/ul
RT: 15.674 min Scan# 2140
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:138 Resp: 492888
Ion Ratio Lower Upper
138 100
92 49.1 40.9 61.3
108 67.7 55.1 82.7









#66
 4,6-Dinitro-2-methylphenol
 Concen: 52.898 ng/ul
 RT: 15.727 min Scan# 2149
 Delta R.T. 0.012 min
 Lab File: BM044420.D
 Acq: 29 Feb 2024 00:50




Instrument :
 BNA_M
 ClientSampleId :
 SLCS332


Tgt Ion:198 Resp: 352406
 Ion Ratio Lower Upper
 198 100
 182 3.9 3.8 5.8
 77 27.0 20.6 30.8



#67
 N-Nitrosodiphenylamine
 Concen: 56.103 ng/ul
 RT: 15.857 min Scan# 2171
 Delta R.T. 0.012 min
 Lab File: BM044420.D
 Acq: 29 Feb 2024 00:50

Tgt Ion:169 Resp: 1668703
 Ion Ratio Lower Upper
 169 100
 168 67.8 53.6 80.4
 167 36.7 29.2 43.8









#68
4-Bromophenyl-phenylether
Concen: 57.754 ng/ul
RT: 16.533 min Scan# 2286
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:248 Resp: 563212
Ion Ratio Lower Upper
248 100
250 98.1 79.8 119.8
141 81.4 65.8 98.8



#69
Hexachlorobenzene
Concen: 56.731 ng/ul
RT: 16.633 min Scan# 2303
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:284 Resp: 633208
Ion Ratio Lower Upper
284 100
142 40.0 33.4 50.2
249 29.7 24.7 37.1

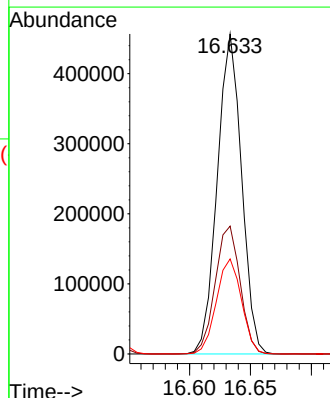



#70

Atrazine

Concen: 33.256 ng/ul

RT: 16.816 min Scan# 21

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:200 Resp: 324025

Ion Ratio Lower Upper

200 100

173 28.4 22.5 33.7

215 48.2 37.8 56.6

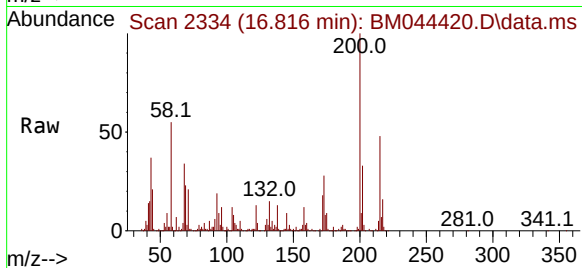

#71

Pentachlorophenol

Concen: 50.822 ng/ul

RT: 16.980 min Scan# 2362

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion:266 Resp: 373819


Ion Ratio Lower Upper

266 100

264 64.0 50.9 76.3

268 63.5 51.1 76.7

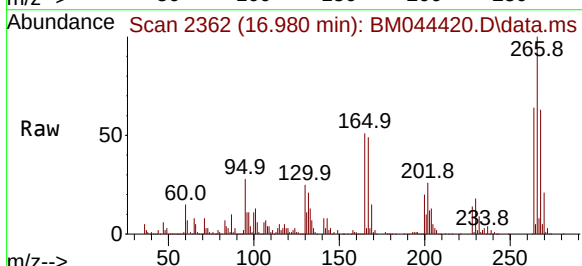



#72

Phenanthrene

Concen: 55.133 ng/ul

RT: 17.380 min Scan# 2430

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:178 Resp: 3104269

Ion Ratio Lower Upper

178 100

179 15.5 12.2 18.4

176 19.4 15.6 23.4

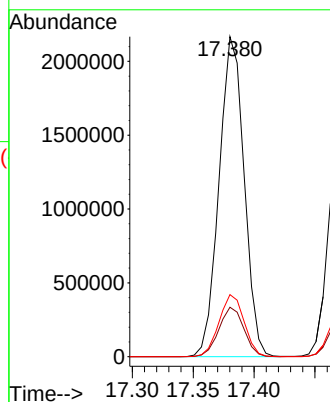

#74

Anthracene

Concen: 55.256 ng/ul

RT: 17.474 min Scan# 2446

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion:178 Resp: 3132477


Ion Ratio Lower Upper

178 100

179 15.6 12.2 18.2

176 18.8 15.4 23.0





#75

1,2,3,4-Tetrachlorobenzene

Concen: 57.217 ng/uL

RT: 13.386 min Scan# 1

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:216 Resp: 786110

Ion Ratio Lower Upper

216 100

214 76.0 61.9 92.9

218 46.1 37.9 56.9

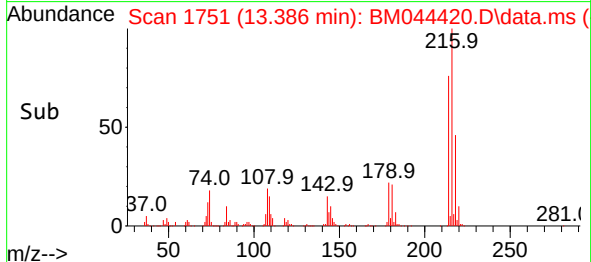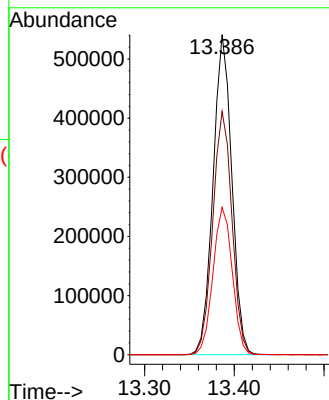

#76

Pentachlorobenzene

Concen: 56.202 ng/uL

RT: 14.904 min Scan# 2009

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion:250 Resp: 737143


Ion Ratio Lower Upper

250 100

248 62.4 48.6 73.0

252 63.9 50.0 75.0

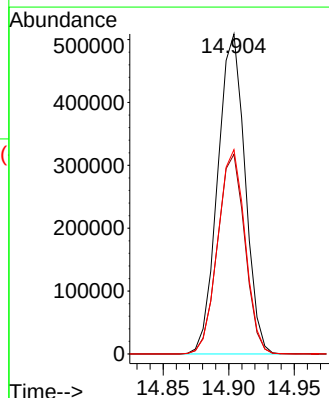



#77

Carbazole

Concen: 55.366 ng/ul

RT: 17.751 min Scan# 2493

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:167 Resp: 2951283

Ion Ratio Lower Upper

167 100

166 21.5 17.1 25.7

139 13.1 10.7 16.1



#78

Di-n-butylphthalate

Concen: 59.665 ng/ul

RT: 18.327 min Scan# 2591

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion:149 Resp: 4026905


Ion Ratio Lower Upper

149 100

150 9.2 7.3 10.9

104 4.8 3.8 5.8









#80
Fluoranthene
Concen: 59.381 ng/u1
RT: 19.398 min Scan# 21
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:202 Resp: 3474165
Ion Ratio Lower Upper
202 100
101 13.8 11.1 16.7
100 10.6 8.2 12.2



#82
Pyrene
Concen: 58.928 ng/u1
RT: 19.762 min Scan# 2835
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:202 Resp: 3615666
Ion Ratio Lower Upper
202 100
101 15.4 12.6 18.8
100 12.4 10.2 15.2



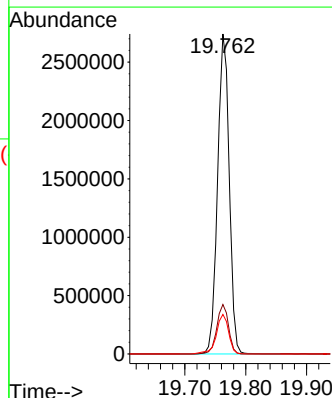





#83
Butylbenzylphthalate
Concen: 66.613 ng/ul
RT: 20.680 min Scan# 2991
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:149 Resp: 1835778
Ion Ratio Lower Upper
149 100
91 71.8 58.1 87.1
206 18.5 15.0 22.4



#84
3,3'-Dichlorobenzidine
Concen: 57.178 ng/ul
RT: 21.456 min Scan# 3123
Delta R.T. 0.000 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:252 Resp: 1037045
Ion Ratio Lower Upper
252 100
254 64.3 51.6 77.4
126 13.6 11.2 16.8









#85
Benzo(a)anthracene
Concen: 57.182 ng/ul
RT: 21.521 min Scan# 3134
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:228 Resp: 3458110
Ion Ratio Lower Upper
228 100
229 19.9 15.4 23.0
226 27.4 21.2 31.8



#86
Bis(2-ethylhexyl)phthalate
Concen: 65.366 ng/ul
RT: 21.462 min Scan# 3124
Delta R.T. 0.000 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:149 Resp: 2758019
Ion Ratio Lower Upper
149 100
167 27.1 22.1 33.1
279 3.3 2.4 3.6





#87

Chrysene

Concen: 56.826 ng/ul

RT: 21.574 min Scan# 3143

Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:228 Resp: 3230334

Ion Ratio Lower Upper

228 100

226 30.3 23.8 35.6

229 20.1 16.0 24.0



#89

Di-n-octyl phthalate

Concen: 65.778 ng/ul




RT: 22.409 min Scan# 3285


Delta R.T. 0.006 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Tgt Ion:149 Resp: 4815514



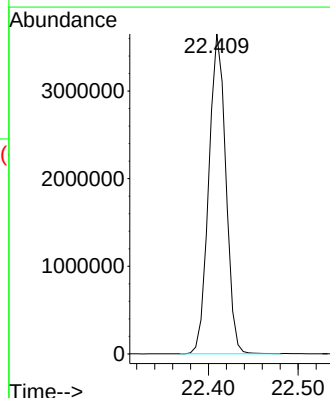





#90
Benzo(b)fluoranthene
Concen: 61.805 ng/u1
RT: 23.221 min Scan# 34
Delta R.T. 0.012 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50




Instrument :
BNA_M
ClientSampleId :
SLCS332


Tgt Ion:252 Resp: 3385552
Ion Ratio Lower Upper
252 100
253 22.0 17.6 26.4
125 12.0 9.8 14.8



#91
Benzo(k)fluoranthene
Concen: 58.432 ng/u1
RT: 23.268 min Scan# 3431
Delta R.T. 0.006 min
Lab File: BM044420.D
Acq: 29 Feb 2024 00:50

Tgt Ion:252 Resp: 3287454
Ion Ratio Lower Upper
252 100
253 21.8 17.4 26.0
125 12.4 9.4 14.2





#93

Benzo(a)pyrene

Concen: 59.822 ng/ul

RT: 23.850 min Scan# 31

Delta R.T. 0.012 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:252 Resp: 3159381

Ion Ratio Lower Upper

252 100

253 22.2 17.4 26.2

125 13.3 10.8 16.2



#94

Indeno(1,2,3-cd)pyrene

Concen: 58.889 ng/ul

RT: 26.491 min Scan# 3979

Delta R.T. 0.024 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50




Tgt Ion:276 Resp: 3761093


Ion Ratio Lower Upper

276 100

138 27.2 22.1 33.1

277 24.6 19.9 29.9





#95

Dibenzo(a,h)anthracene

Concen: 59.363 ng/ul

RT: 26.521 min Scan# 3984

Delta R.T. 0.024 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Instrument :

BNA_M

ClientSampleId :

SLCS332





Tgt Ion:278 Resp: 3168312

Ion Ratio Lower Upper

278 100

139 19.1 14.9 22.3

279 23.7 19.5 29.3

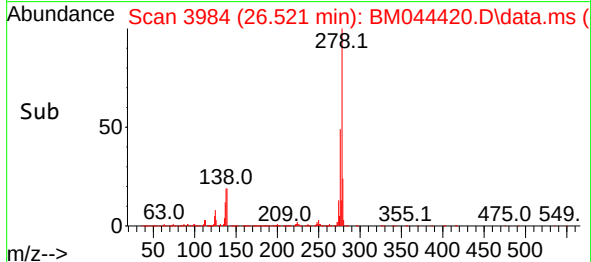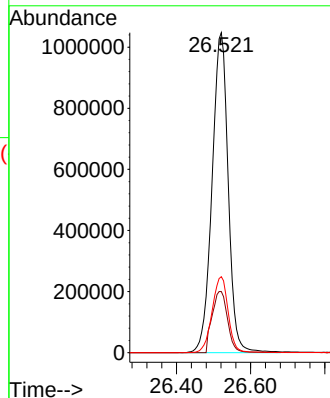

#96

Benzo(g,h,i)perylene

Concen: 58.536 ng/ul

RT: 27.268 min Scan# 4111

Delta R.T. 0.030 min

Lab File: BM044420.D

Acq: 29 Feb 2024 00:50

Tgt Ion:276 Resp: 3024118

Ion Ratio Lower Upper

276 100

138 25.4 21.6 32.4

277 23.4 18.5 27.7

