

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044431.D
 Acq On : 29 Feb 2024 08:44
 Operator : MA/JU
 Sample : P1512-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0S93

Quant Time: Feb 29 09:51:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 29 03:37:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	179767	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	797432	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.592	164	464025	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.339	188	966214	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	794599	20.000	ng/u1	0.00
88) Perylene-d12	23.956	264	855246	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	43362	7.611	ng/uL	0.00
4) Pyridine-d5	3.787	84	664679	42.716	ng/u1	0.00
7) Phenol-d5	7.116	99	790388	45.897	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.292	67	508906	45.634	ng/u1	0.00
11) 2-Chlorophenol-d4	7.475	132	620369	47.831	ng/u1	0.00
15) 4-Methylphenol-d8	8.663	113	612436	47.001	ng/u1	0.00
21) Nitrobenzene-d5	9.122	128	312041	48.127	ng/u1	0.00
24) 2-Nitrophenol-d4	9.845	143	338099	51.111	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	570003	48.848	ng/u1	0.00
31) 4-Chloroaniline-d4	10.904	131	873326	44.563	ng/u1	0.00
46) Dimethylphthalate-d6	14.015	166	1831916	51.188	ng/u1	0.00
49) Acenaphthylene-d8	14.286	160	2159668	52.451	ng/u1	0.00
54) 4-Nitrophenol-d4	14.798	143	274021	38.479	ng/u1	0.00
60) Fluorene-d10	15.586	176	1613670	53.273	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	204796	34.160	ng/u1	0.00
73) Anthracene-d10	17.439	188	2428056	52.703	ng/u1	0.00
81) Pyrene-d10	19.733	212	2713039	56.753	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.803	264	2424140	55.316	ng/u1	0.00
Target Compounds						
					Qvalue	
18) 4-Methylphenol	8.722	108	23625	1.682	ng/u1	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044431.D
Acq On : 29 Feb 2024 08:44
Operator : MA/JU
Sample : P1512-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0S93

Quant Time: Feb 29 09:51:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 29 03:37:20 2024
Response via : Initial Calibration

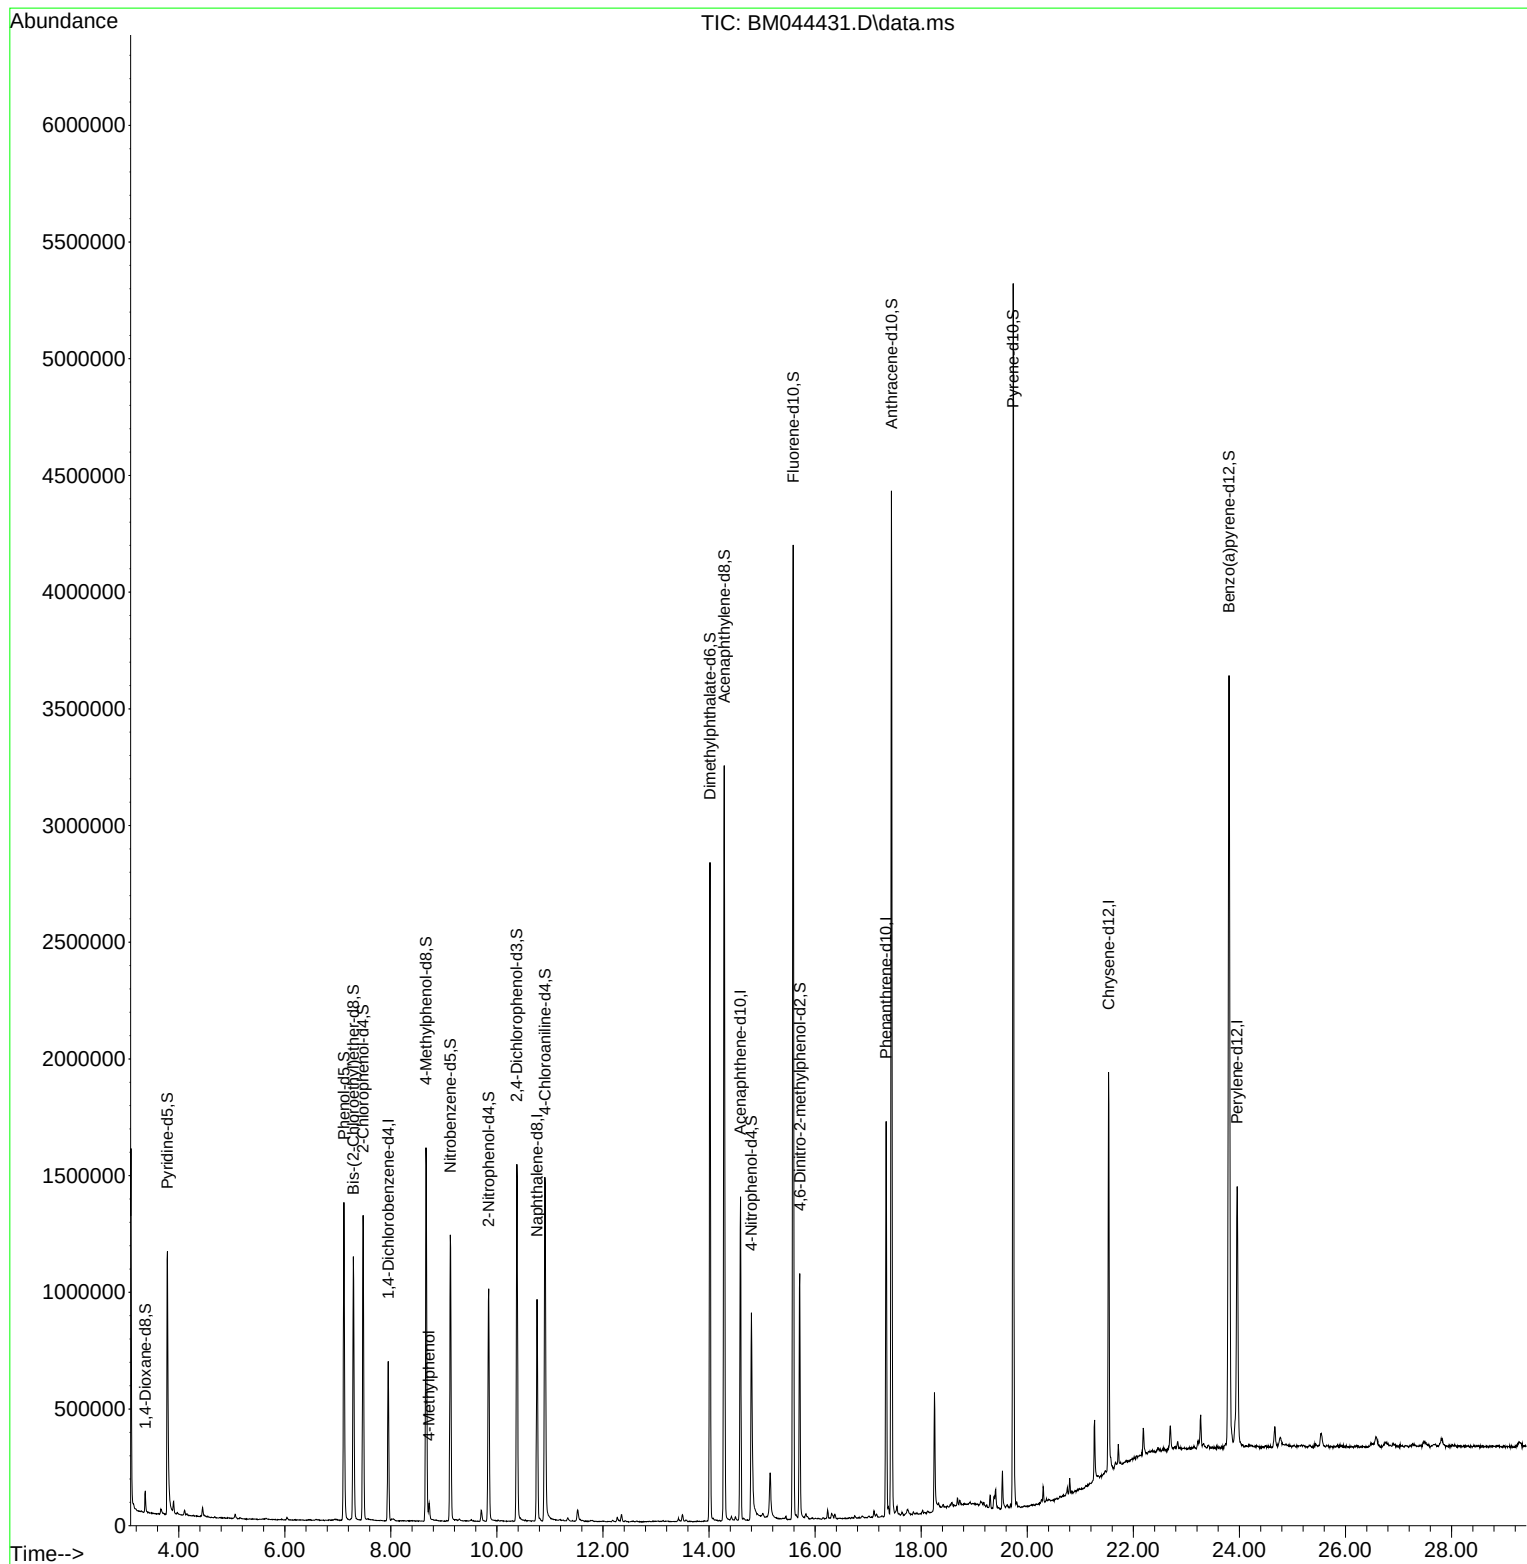

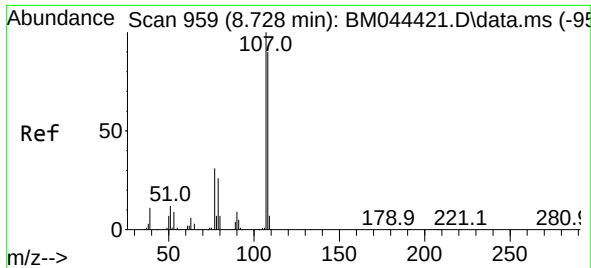

#18
 4-Methylphenol
 Concen: 1.682 ng/ul
 RT: 8.722 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BM044431.D
 Acq: 29 Feb 2024 08:44

Instrument :
 BNA_M
 ClientSampleId :
 E0S93

Tgt Ion:108 Resp: 23625
 Ion Ratio Lower Upper
 108 100
 107 130.0 86.8 130.2

