

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044432.D
 Acq On : 29 Feb 2024 09:21
 Operator : MA/JU
 Sample : P1512-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOS96

Quant Time: Feb 29 10:01:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 29 03:37:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.951	152	185002	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	824479	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.592	164	488441	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.339	188	994301	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	816840	20.000	ng/ul	0.00
88) Perylene-d12	23.956	264	901035	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	37971	6.476	ng/uL	0.00
4) Pyridine-d5	3.787	84	574519	35.877	ng/ul	0.00
7) Phenol-d5	7.116	99	667827	37.682	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.293	67	425029	37.035	ng/ul	0.00
11) 2-Chlorophenol-d4	7.481	132	527282	39.503	ng/ul	0.00
15) 4-Methylphenol-d8	8.669	113	523288	39.023	ng/ul	0.00
21) Nitrobenzene-d5	9.128	128	259906	38.771	ng/ul	0.00
24) 2-Nitrophenol-d4	9.845	143	281279	41.126	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	482568	39.999	ng/ul	0.00
31) 4-Chloroaniline-d4	10.910	131	764438	37.727	ng/ul	0.00
46) Dimethylphthalate-d6	14.016	166	1556798	41.326	ng/ul	0.00
49) Acenaphthylene-d8	14.286	160	1834259	42.321	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	184050	24.553	ng/ul	0.00
60) Fluorene-d10	15.586	176	1372198	43.037	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.710	200	134790	21.848	ng/ul	0.00
73) Anthracene-d10	17.439	188	2087628	44.034	ng/ul	0.00
81) Pyrene-d10	19.733	212	2338536	47.587	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.803	264	2085645	45.173	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.146	94	20922	1.136	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044432.D
Acq On : 29 Feb 2024 09:21
Operator : MA/JU
Sample : P1512-03
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0S96

Quant Time: Feb 29 10:01:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 29 03:37:20 2024
Response via : Initial Calibration

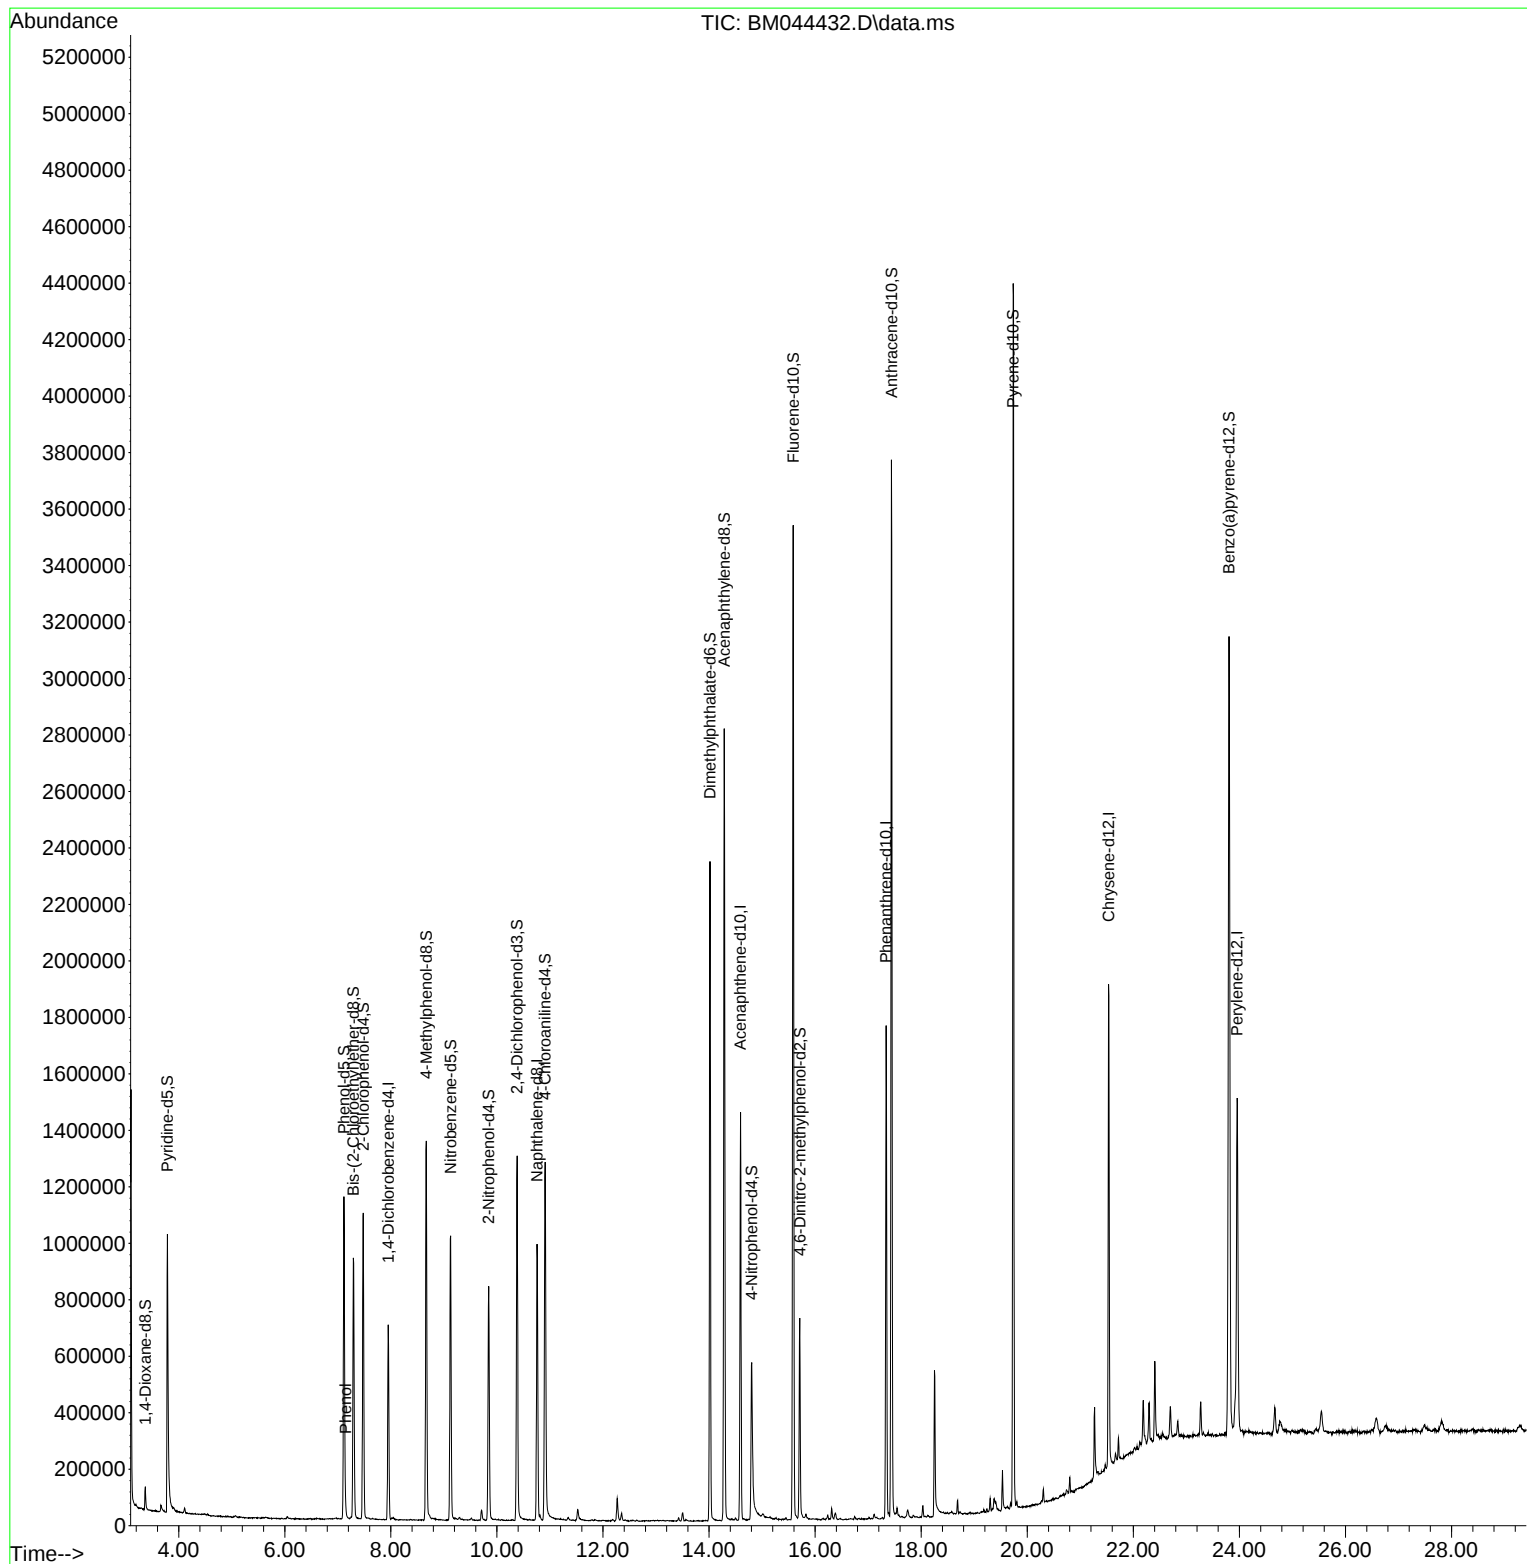

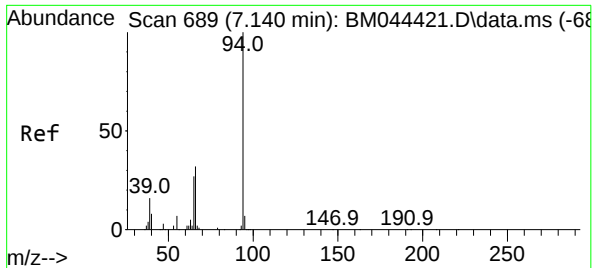

#8
Phenol
Concen: 1.136 ng/ul
RT: 7.146 min Scan# 61
Delta R.T. 0.006 min
Lab File: BM044432.D
Acq: 29 Feb 2024 09:21

Instrument :
BNA_M
ClientSampleId :
E0S96

Tgt Ion: 94	Resp: 20922
Ion Ratio	Lower Upper
94	100
65	26.4 20.6 31.0
66	34.4 25.4 38.0

