

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044443.D
 Acq On : 29 Feb 2024 17:16
 Operator : MA/JU
 Sample : P1512-06
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOS99

Quant Time: Feb 29 18:06:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 29 03:37:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.957	152	162295	20.000	ng/u1	0.00
20) Naphthalene-d8	10.763	136	704997	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.598	164	397004	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	837974	20.000	ng/u1	0.00
79) Chrysene-d12	21.538	240	700121	20.000	ng/u1	0.00
88) Perylene-d12	23.962	264	777221	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	30693	5.967	ng/uL	0.00
4) Pyridine-d5	3.787	84	446189	31.762	ng/u1	0.00
7) Phenol-d5	7.122	99	516784	33.239	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.298	67	329375	32.715	ng/u1	0.00
11) 2-Chlorophenol-d4	7.481	132	409594	34.979	ng/u1	0.00
15) 4-Methylphenol-d8	8.669	113	394925	33.571	ng/u1	0.00
21) Nitrobenzene-d5	9.128	128	196639	34.304	ng/u1	0.00
24) 2-Nitrophenol-d4	9.851	143	212375	36.314	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.386	165	356123	34.521	ng/u1	0.01
31) 4-Chloroaniline-d4	10.916	131	548630	31.665	ng/u1	0.01
46) Dimethylphthalate-d6	14.021	166	1124368	36.722	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	1315956	37.355	ng/u1	0.00
54) 4-Nitrophenol-d4	14.810	143	141121	23.162	ng/u1	0.01
60) Fluorene-d10	15.592	176	986040	38.048	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.715	200	107765	20.726	ng/u1	0.00
73) Anthracene-d10	17.445	188	1510801	37.812	ng/u1	0.00
81) Pyrene-d10	19.739	212	1689551	40.113	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.809	264	1536617	38.584	ng/u1	0.01
Target Compounds						
					Qvalue	
30) Naphthalene	10.816	128	219046	5.463	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044443.D
Acq On : 29 Feb 2024 17:16
Operator : MA/JU
Sample : P1512-06
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0S99

Quant Time: Feb 29 18:06:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 29 03:37:20 2024
Response via : Initial Calibration

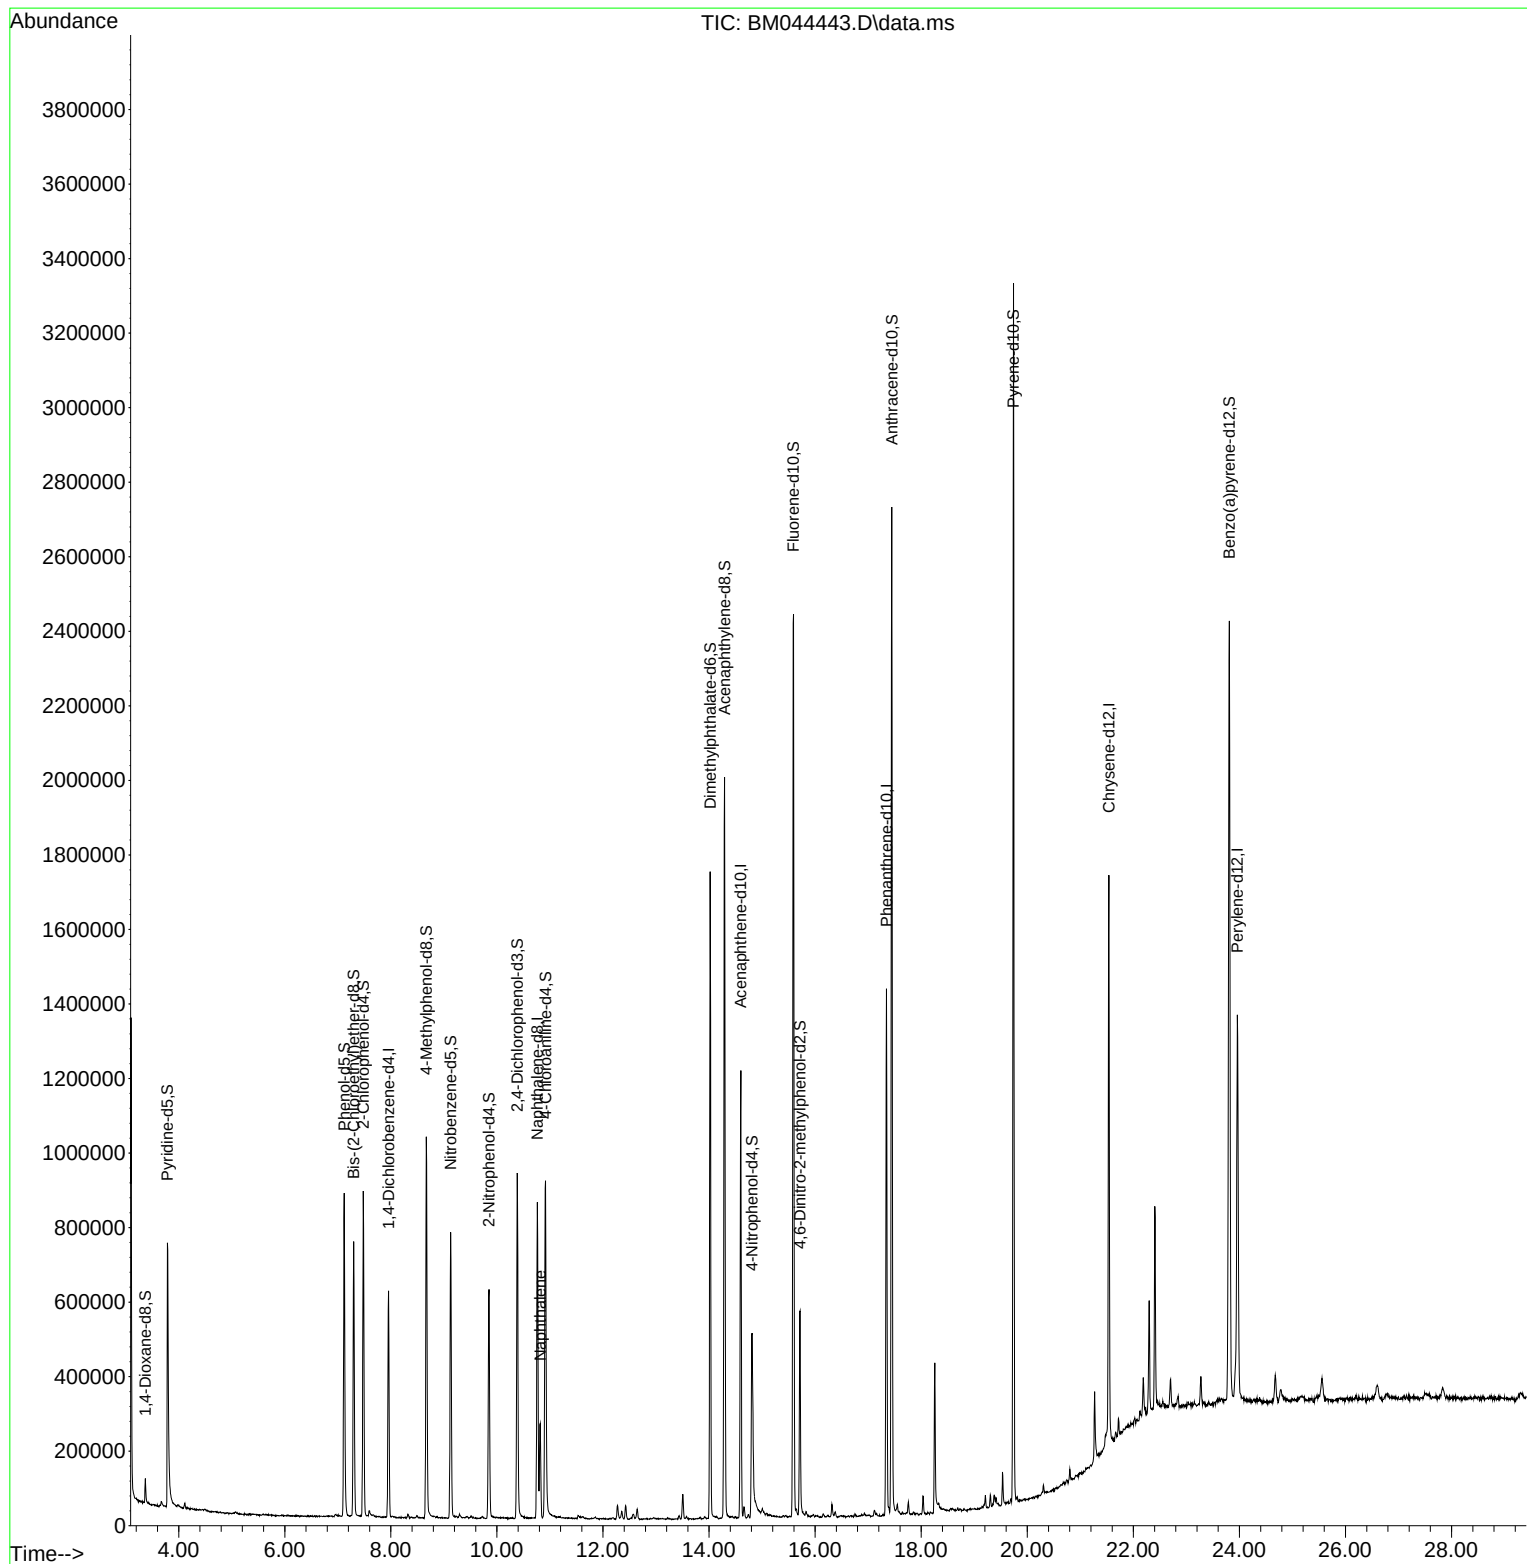

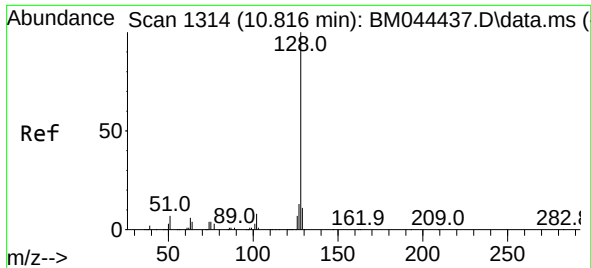

#30
Naphthalene
Concen: 5.463 ng/ul
RT: 10.816 min Scan# 11
Delta R.T. 0.006 min
Lab File: BM044443.D
Acq: 29 Feb 2024 17:16

Instrument :
BNA_M
ClientSampleId :
E0S99

Tgt Ion:128 Resp: 219046
Ion Ratio Lower Upper
128 100
129 10.6 8.8 13.2
127 12.9 10.2 15.2

