

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044409.D
 Acq On : 28 Feb 2024 18:07
 Operator : MA/JU
 Sample : P1535-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	38	42	45	rBV	69831	85494	1.41%	0.168%
2	3.369	45	48	58	rVB2	51558	79169	1.31%	0.156%
3	3.799	118	121	135	rBV	116258	222117	3.67%	0.437%
4	4.110	169	174	179	rBV2	15554	23679	0.39%	0.047%
5	4.634	258	263	275	rVB	104452	153033	2.53%	0.301%
6	5.645	429	435	439	rVV4	5670	11495	0.19%	0.023%
7	7.110	678	684	697	rBV	201814	333142	5.50%	0.656%
8	7.292	708	715	727	rBV	832536	1335572	22.05%	2.629%
9	7.475	739	746	754	rBV	781400	1222547	20.19%	2.406%
10	7.557	758	760	766	rVB6	4804	7480	0.12%	0.015%
11	7.951	820	827	834	rBV	668615	1088949	17.98%	2.143%
12	8.363	893	897	900	rBV6	4446	8083	0.13%	0.016%
13	8.663	941	948	957	rBV	557719	928120	15.33%	1.827%
14	8.845	973	979	980	rBV5	4655	6665	0.11%	0.013%
15	9.122	1018	1026	1036	rBV	887120	1474920	24.36%	2.903%
16	9.839	1140	1148	1162	rBV	678810	1143140	18.88%	2.250%
17	10.375	1232	1239	1255	rBV	952046	1664074	27.48%	3.275%
18	10.757	1296	1304	1314	rBV	938807	1588720	26.23%	3.127%
19	10.904	1322	1329	1350	rBV	394713	777555	12.84%	1.530%
20	11.433	1413	1419	1422	rBV8	2968	6654	0.11%	0.013%
21	12.351	1570	1575	1580	rBV3	16980	27022	0.45%	0.053%
22	13.492	1765	1769	1775	rVB5	9448	16640	0.27%	0.033%
23	14.016	1851	1858	1870	rBV	2040115	2895644	47.82%	5.699%
24	14.286	1896	1904	1913	rBV	2259582	3423267	56.53%	6.737%
25	14.586	1948	1955	1962	rBV	1319772	1979572	32.69%	3.896%
26	14.810	1986	1993	2008	rBV2	51976	171053	2.82%	0.337%
27	15.392	2087	2092	2099	rBV	11463	20926	0.35%	0.041%
28	15.580	2117	2124	2134	rBV	2974568	4446434	73.42%	8.751%
29	15.704	2139	2145	2159	rVV	934762	1370481	22.63%	2.697%
30	15.821	2162	2165	2174	rVB5	14440	26356	0.44%	0.052%
31	16.368	2254	2258	2264	rVB6	9496	16347	0.27%	0.032%
32	16.951	2353	2357	2362	rBV4	6548	9324	0.15%	0.018%
33	17.015	2364	2368	2371	rBV6	5222	6211	0.10%	0.012%
34	17.339	2416	2423	2433	rBV	1593615	2288642	37.79%	4.504%
35	17.439	2433	2440	2454	rVV	3502969	5019559	82.89%	9.879%
36	18.015	2531	2538	2543	rBV9	18303	29013	0.48%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044409.D
Acq On : 28 Feb 2024 18:07
Operator : MA/JU
Sample : P1535-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	18.080	2545	2549	2552	rVB6	4176	6404	0.11%	0.013%
38	18.245	2573	2577	2588	rBV2	51973	82453	1.36%	0.162%
39	18.333	2588	2592	2598	rVB9	6177	11032	0.18%	0.022%
40	18.451	2609	2612	2616	rBV5	5682	7544	0.12%	0.015%
41	18.574	2629	2633	2638	rBV5	12313	22953	0.38%	0.045%
42	18.733	2656	2660	2666	rVB4	17587	24688	0.41%	0.049%
43	19.298	2752	2756	2761	rVB	45406	65812	1.09%	0.130%
44	19.368	2764	2768	2772	rBV	47808	81795	1.35%	0.161%
45	19.533	2791	2796	2800	rBV3	40135	62081	1.03%	0.122%
46	19.686	2819	2822	2824	rBV3	25540	30304	0.50%	0.060%
47	19.733	2824	2830	2841	rVV	4516567	6055831	100.00%	11.918%
48	21.539	3131	3137	3147	rBV	1685487	2302395	38.02%	4.531%
49	23.803	3515	3522	3536	rBV2	2766513	5719497	94.45%	11.256%
50	23.962	3543	3549	3561	rVB	1167601	2431020	40.14%	4.784%




Sum of corrected areas: 50810908

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044409.D
Acq On : 28 Feb 2024 18:07
Operator : MA/JU
Sample : P1535-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

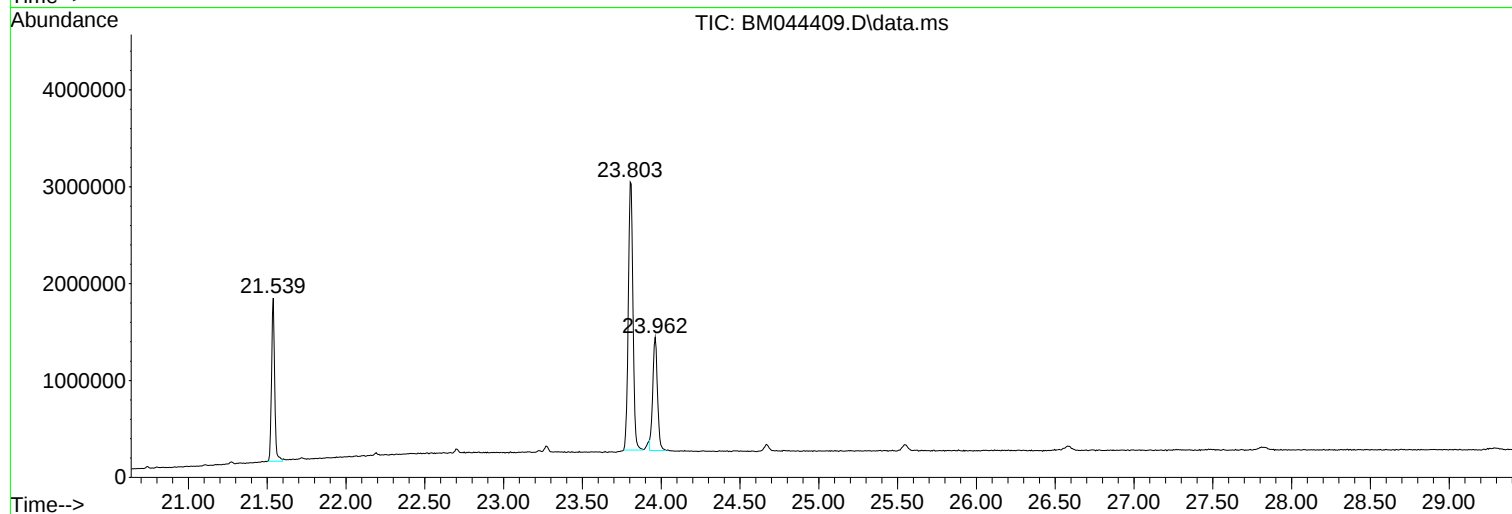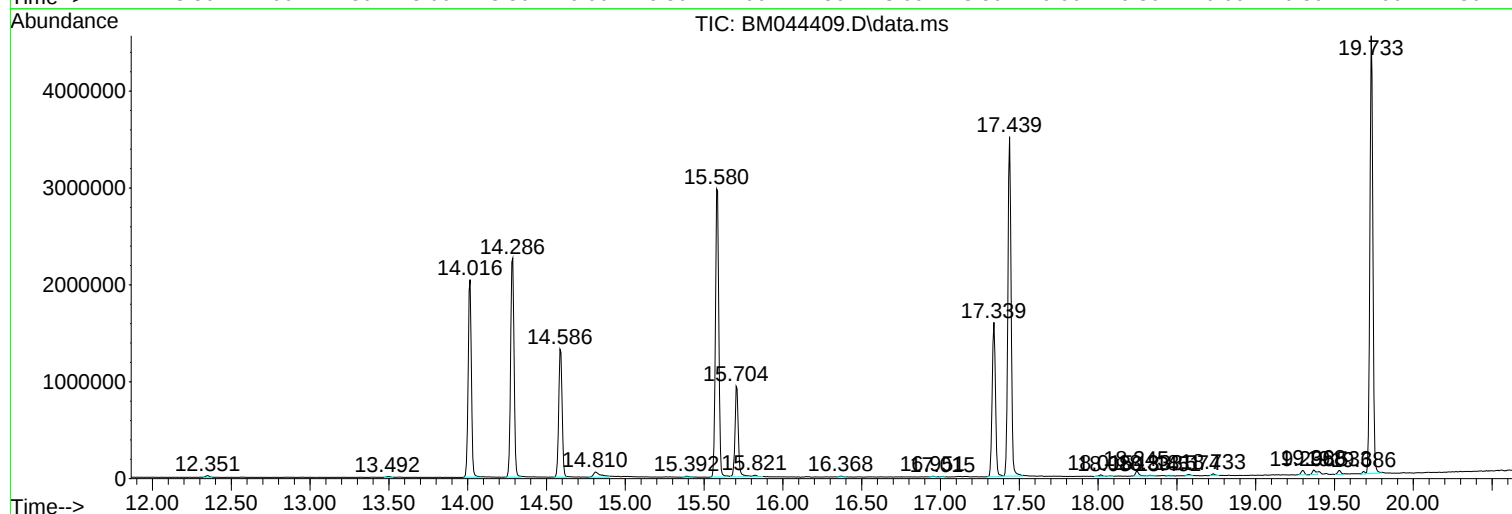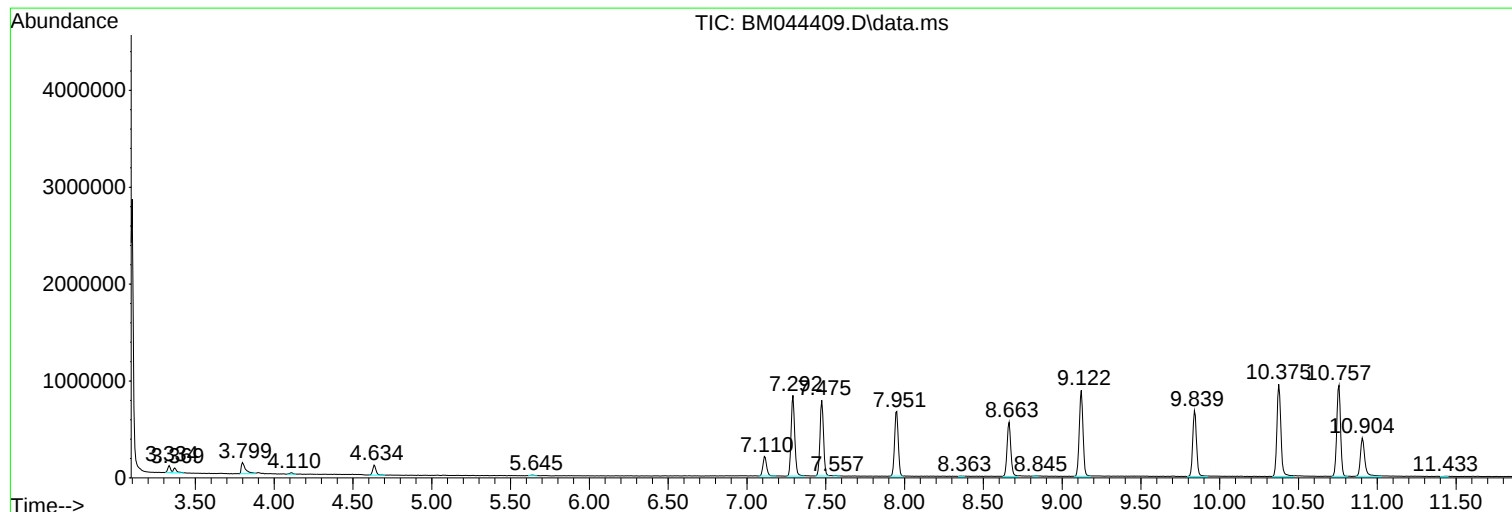

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044409.D
Acq On : 28 Feb 2024 18:07
Operator : MA/JU
Sample : P1535-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044409.D
Acq On : 28 Feb 2024 18:07
Operator : MA/JU
Sample : P1535-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc