

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044410.D
 Acq On : 28 Feb 2024 18:44
 Operator : MA/JU
 Sample : P1535-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M

Title : SVOA CALIBRATION

Signal : TIC: BM044410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	37	42	46	rBV	279282	342103	5.42%	0.619%
2	3.369	46	48	52	rVB	49989	51078	0.81%	0.092%
3	3.799	118	121	137	rBV	133478	261699	4.14%	0.474%
4	4.110	171	174	178	rVB4	14083	19907	0.32%	0.036%
5	4.634	258	263	271	rVB	257761	371117	5.87%	0.672%
6	7.116	678	685	693	rBV	232697	391922	6.20%	0.709%
7	7.293	708	715	730	rBV	1000926	1584947	25.09%	2.869%
8	7.475	737	746	755	rBV	925387	1455672	23.04%	2.635%
9	7.557	758	760	767	rVB7	6896	10928	0.17%	0.020%
10	7.951	819	827	836	rBV	630053	1008097	15.96%	1.825%
11	8.663	941	948	957	rBV	692316	1107471	17.53%	2.004%
12	9.122	1017	1026	1038	rBV	1077441	1809048	28.64%	3.274%
13	9.839	1141	1148	1163	rBV	812460	1402875	22.21%	2.539%
14	10.375	1232	1239	1252	rBV	1172328	2029793	32.13%	3.674%
15	10.757	1296	1304	1313	rVB	893461	1487100	23.54%	2.692%
16	10.904	1320	1329	1344	rBV	508787	976451	15.46%	1.767%
17	12.351	1570	1575	1585	rVB2	23322	43028	0.68%	0.078%
18	13.498	1764	1770	1777	rBV3	19389	34279	0.54%	0.062%
19	14.016	1851	1858	1874	rBV	2370453	3275700	51.86%	5.929%
20	14.286	1896	1904	1917	rBV	2758805	4120124	65.22%	7.457%
21	14.592	1949	1956	1965	rBV	1228248	1897237	30.03%	3.434%
22	14.810	1987	1993	2008	rBV2	56150	202655	3.21%	0.367%
23	15.016	2024	2028	2030	rBV5	5980	7698	0.12%	0.014%
24	15.392	2089	2092	2096	rBV2	11718	15901	0.25%	0.029%
25	15.586	2117	2125	2133	rBV	3407488	5104664	80.81%	9.239%
26	15.710	2139	2146	2156	rBV	1022730	1465007	23.19%	2.652%
27	15.821	2161	2165	2170	rVB4	15190	24689	0.39%	0.045%
28	16.368	2255	2258	2264	rVB6	11215	15747	0.25%	0.029%
29	17.015	2364	2368	2371	rBV5	5404	7674	0.12%	0.014%
30	17.121	2382	2386	2389	rBV5	4405	8701	0.14%	0.016%
31	17.339	2416	2423	2433	rBV	1561403	2168452	34.33%	3.925%
32	17.439	2433	2440	2458	rVV	4029100	5690594	90.08%	10.300%
33	17.639	2471	2474	2479	rVB6	5106	7891	0.12%	0.014%
34	18.021	2536	2539	2544	rVB5	8710	11213	0.18%	0.020%
35	18.245	2573	2577	2584	rBV4	33720	48713	0.77%	0.088%
36	19.298	2751	2756	2761	rBV3	48452	71303	1.13%	0.129%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044410.D
Acq On : 28 Feb 2024 18:44
Operator : MA/JU
Sample : P1535-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.368	2764	2768	2772	rBV	39896	56680	0.90%	0.103%
38	19.533	2792	2796	2802	rBV4	22990	31351	0.50%	0.057%
39	19.686	2818	2822	2824	rBV2	20034	21315	0.34%	0.039%
40	19.733	2824	2830	2840	rVV	4675484	6317002	100.00%	11.433%
41	20.739	2998	3001	3006	rBV6	19063	26569	0.42%	0.048%
42	21.533	3131	3136	3151	rBV2	1472056	2091928	33.12%	3.786%
43	23.803	3514	3522	3534	rBV	3003043	6019314	95.29%	10.895%
44	23.956	3542	3548	3557	rVB	1042345	2154852	34.11%	3.900%




Sum of corrected areas: 55250489

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044410.D
Acq On : 28 Feb 2024 18:44
Operator : MA/JU
Sample : P1535-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

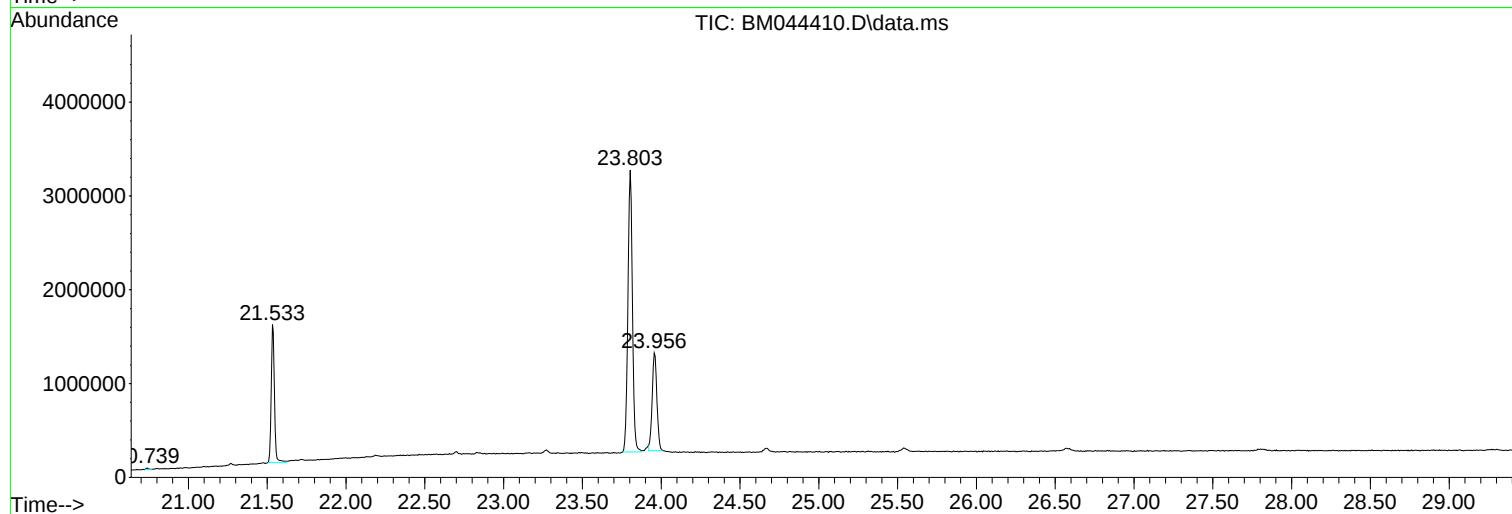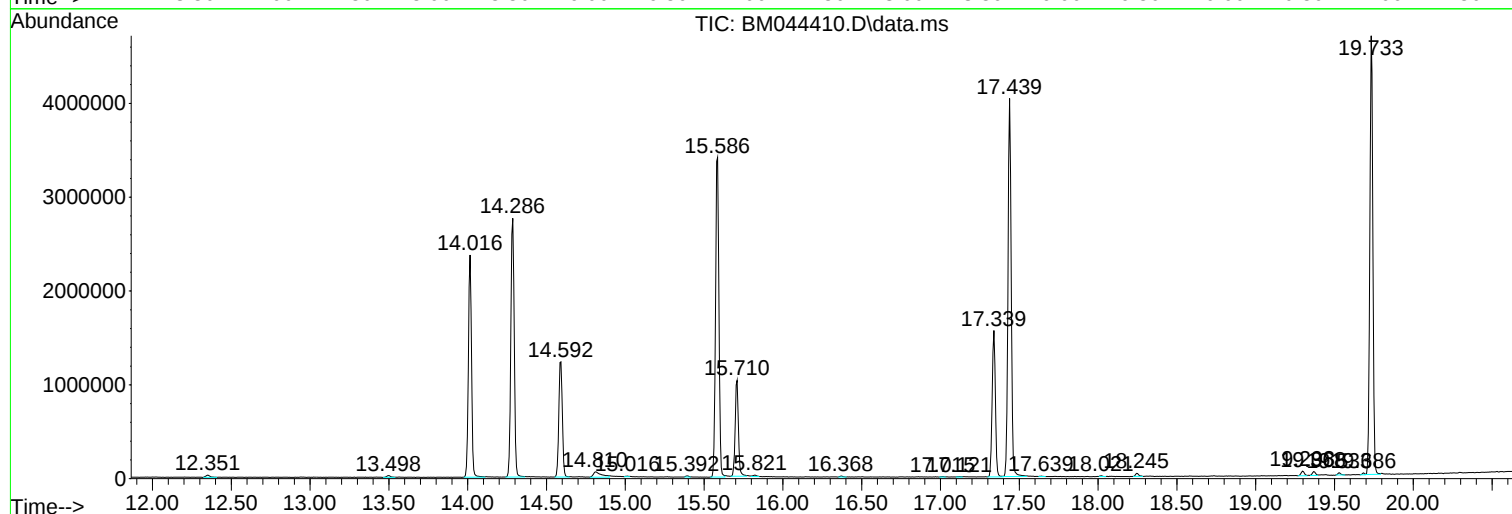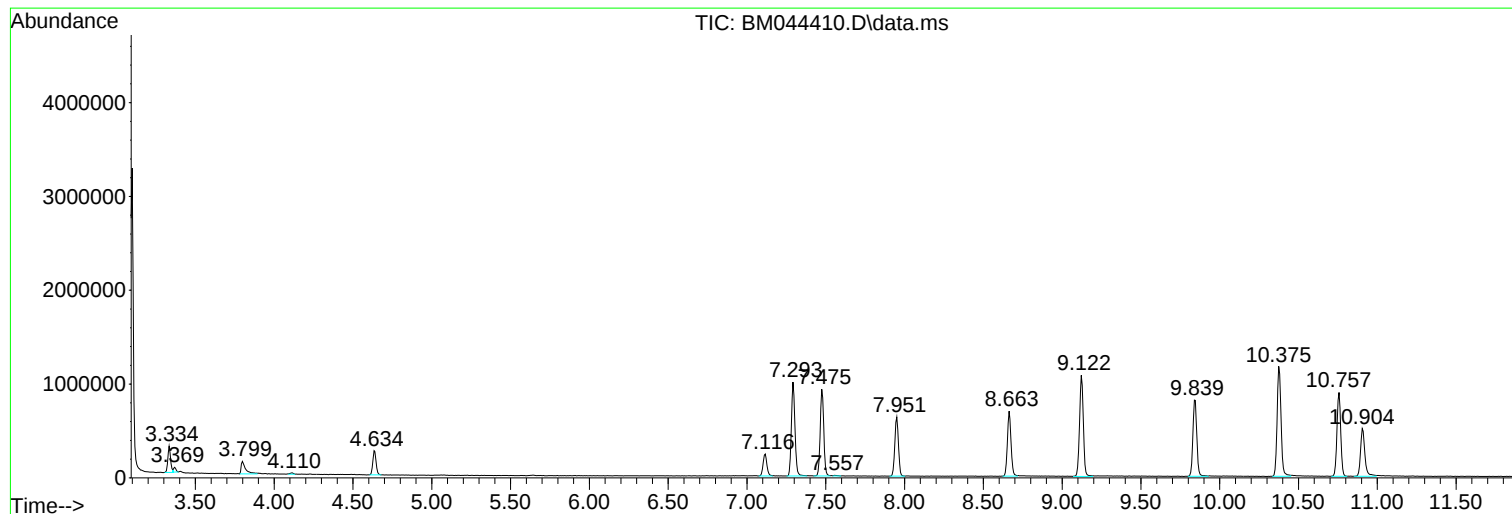

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044410.D
Acq On : 28 Feb 2024 18:44
Operator : MA/JU
Sample : P1535-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044410.D
Acq On : 28 Feb 2024 18:44
Operator : MA/JU
Sample : P1535-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc