

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044411.D
 Acq On : 28 Feb 2024 19:20
 Operator : MA/JU
 Sample : P1535-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	39	42	45	rBV	28202	31898	0.50%	0.057%
2	3.369	45	48	53	rVB	44829	53323	0.83%	0.095%
3	3.799	118	121	138	rBV	148887	290626	4.53%	0.517%
4	4.110	171	174	178	rVB	15587	18559	0.29%	0.033%
5	4.634	259	263	272	rVB	72650	104781	1.63%	0.186%
6	5.646	433	435	441	rVB7	5442	7651	0.12%	0.014%
7	7.116	678	685	699	rVB	236957	396639	6.19%	0.706%
8	7.292	708	715	730	rBV	1043461	1657567	25.85%	2.950%
9	7.475	739	746	756	rBV	945446	1485735	23.17%	2.644%
10	7.951	820	827	835	rBV	652138	1037750	16.18%	1.847%
11	8.663	939	948	965	rBV	691015	1144096	17.84%	2.036%
12	9.122	1018	1026	1039	rBV	1135143	1885757	29.41%	3.356%
13	9.839	1140	1148	1162	rBV	860342	1473311	22.98%	2.622%
14	10.375	1231	1239	1250	rBV	1211123	2096551	32.70%	3.732%
15	10.757	1296	1304	1316	rVB	925743	1548215	24.14%	2.756%
16	10.904	1320	1329	1339	rBV	349946	680676	10.62%	1.211%
17	12.192	1542	1548	1551	rBV6	4822	9281	0.14%	0.017%
18	12.351	1570	1575	1586	rVB2	25050	44120	0.69%	0.079%
19	13.421	1753	1757	1764	rBV8	6953	10758	0.17%	0.019%
20	13.498	1764	1770	1776	rVB3	20753	33980	0.53%	0.060%
21	13.569	1778	1782	1789	rVB7	6126	10196	0.16%	0.018%
22	14.016	1851	1858	1871	rBV	2431651	3347486	52.21%	5.958%
23	14.286	1896	1904	1918	rBV	2900498	4266183	66.53%	7.593%
24	14.498	1936	1940	1943	rVB6	5710	6872	0.11%	0.012%
25	14.592	1948	1956	1967	rBV	1339421	2000545	31.20%	3.561%
26	14.710	1972	1976	1983	rVB9	5110	10745	0.17%	0.019%
27	14.815	1986	1994	2006	rBV2	60622	193316	3.01%	0.344%
28	14.998	2020	2025	2029	rBV8	7477	10204	0.16%	0.018%
29	15.263	2065	2070	2073	rBV7	4707	9083	0.14%	0.016%
30	15.386	2088	2091	2096	rBV4	4598	9040	0.14%	0.016%
31	15.451	2099	2102	2105	rVV4	5835	8076	0.13%	0.014%
32	15.586	2115	2125	2139	rBV	3665368	5266369	82.13%	9.373%
33	15.710	2139	2146	2160	rVV	1065081	1534715	23.93%	2.732%
34	15.821	2160	2165	2172	rVB5	20657	42518	0.66%	0.076%
35	16.315	2244	2249	2252	rVB6	8013	11974	0.19%	0.021%
36	16.368	2254	2258	2265	rVB3	15405	24922	0.39%	0.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044411.D
 Acq On : 28 Feb 2024 19:20
 Operator : MA/JU
 Sample : P1535-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	17.009	2361	2367	2373	rVB9	9677	14838	0.23%	0.026%
38	17.109	2380	2384	2386	rBV4	10144	13414	0.21%	0.024%
39	17.157	2389	2392	2396	rVB6	5315	7618	0.12%	0.014%
40	17.339	2417	2423	2432	rBV	1609455	2230582	34.79%	3.970%
41	17.439	2432	2440	2452	rBV	3930978	5656776	88.22%	10.068%
42	17.633	2471	2473	2478	rVB6	9429	15199	0.24%	0.027%
43	17.739	2489	2491	2498	rVB6	5427	8711	0.14%	0.016%
44	17.851	2506	2510	2515	rBV7	6853	7683	0.12%	0.014%
45	18.021	2534	2539	2543	rVB7	8670	11958	0.19%	0.021%
46	18.245	2572	2577	2584	rBV	71133	115104	1.80%	0.205%
47	18.609	2636	2639	2644	rVB6	15756	23508	0.37%	0.042%
48	18.662	2644	2648	2654	rVB8	20278	31854	0.50%	0.057%
49	18.915	2686	2691	2694	rBV6	7204	9237	0.14%	0.016%
50	19.180	2734	2736	2741	rVB6	6376	8795	0.14%	0.016%
51	19.303	2751	2757	2761	rBV3	49245	74996	1.17%	0.133%
52	19.368	2764	2768	2774	rVV	44127	67390	1.05%	0.120%
53	19.439	2778	2780	2783	rVB4	8530	9125	0.14%	0.016%
54	19.533	2791	2796	2800	rBV3	49700	68893	1.07%	0.123%
55	19.686	2819	2822	2824	rBV2	19213	22033	0.34%	0.039%
56	19.733	2824	2830	2840	rVV	4695015	6412194	100.00%	11.413%
57	20.739	2999	3001	3003	rBV2	15561	12061	0.19%	0.021%
58	21.268	3089	3091	3096	rVB5	30425	35538	0.55%	0.063%
59	21.539	3131	3137	3152	rBV	1586904	2198396	34.28%	3.913%
60	23.803	3514	3522	3535	rBV2	3020080	6090844	94.99%	10.841%
61	23.962	3542	3549	3560	rVB	1079844	2274756	35.48%	4.049%




Sum of corrected areas: 56185021

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044411.D
Acq On : 28 Feb 2024 19:20
Operator : MA/JU
Sample : P1535-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

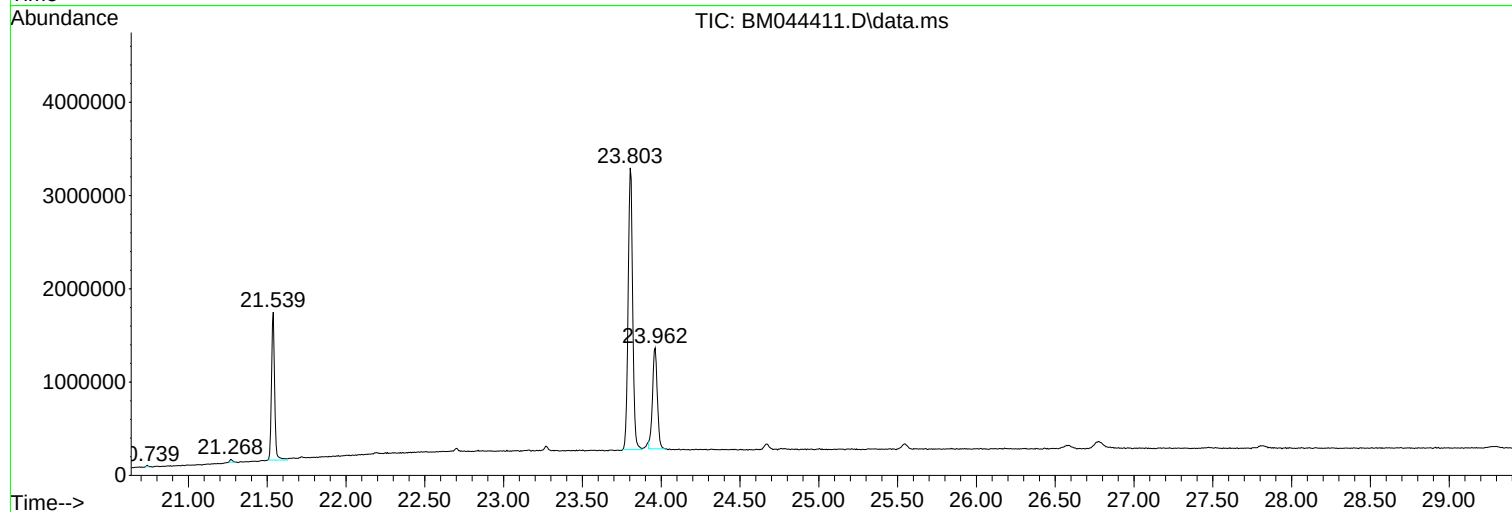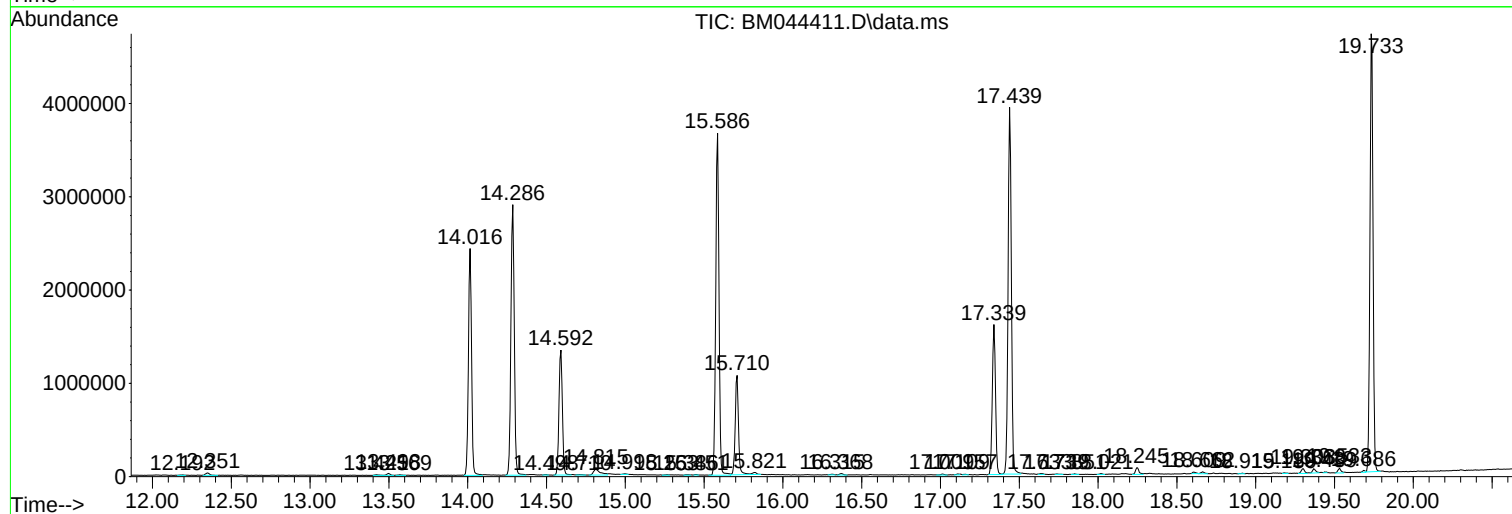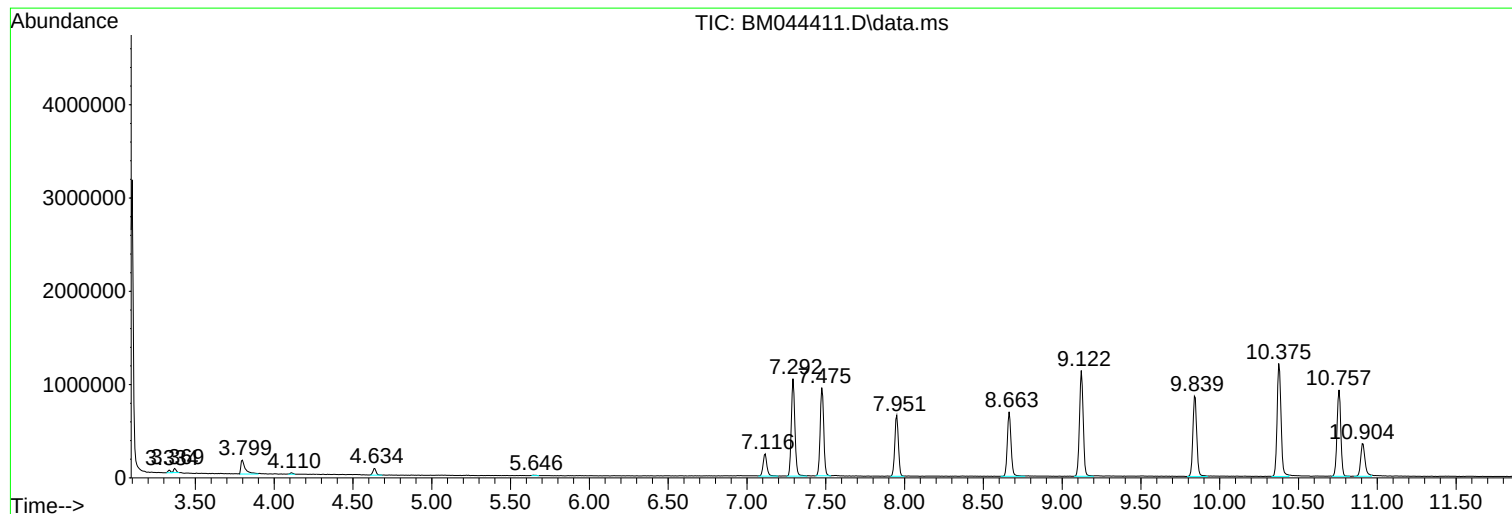

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044411.D
Acq On : 28 Feb 2024 19:20
Operator : MA/JU
Sample : P1535-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044411.D
Acq On : 28 Feb 2024 19:20
Operator : MA/JU
Sample : P1535-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc