

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044412.D
 Acq On : 28 Feb 2024 19:57
 Operator : MA/JU
 Sample : P1535-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	39	42	45	rBV2	23961	29081	0.43%	0.052%
2	3.369	45	48	57	rVB	48751	67884	1.01%	0.121%
3	3.793	117	120	137	rBV	180107	339596	5.05%	0.607%
4	4.110	171	174	180	rVB	15443	22361	0.33%	0.040%
5	4.634	259	263	273	rVB	64512	96740	1.44%	0.173%
6	5.216	360	362	366	rBV5	5364	6983	0.10%	0.012%
7	5.640	429	434	436	rBV6	6079	9983	0.15%	0.018%
8	7.116	679	685	699	rVB	214029	357000	5.31%	0.638%
9	7.293	709	715	727	rBV	916539	1438142	21.37%	2.571%
10	7.475	738	746	757	rBV	828286	1306950	19.42%	2.337%
11	7.951	818	827	835	rBV	629469	996033	14.80%	1.781%
12	8.663	940	948	962	rBV	614081	1029023	15.29%	1.840%
13	9.122	1018	1026	1039	rBV	1007768	1678186	24.94%	3.000%
14	9.839	1141	1148	1156	rBV	737284	1258485	18.70%	2.250%
15	10.375	1232	1239	1258	rBV	1064705	1887604	28.05%	3.375%
16	10.757	1295	1304	1312	rBV	898405	1504993	22.37%	2.691%
17	10.904	1322	1329	1340	rBV	453408	873745	12.98%	1.562%
18	12.310	1563	1568	1570	rBV5	4481	7529	0.11%	0.013%
19	12.351	1570	1575	1582	rVB2	23404	38338	0.57%	0.069%
20	13.498	1765	1770	1776	rVB2	22964	37670	0.56%	0.067%
21	14.016	1851	1858	1872	rBV	2434972	3373036	50.13%	6.031%
22	14.286	1896	1904	1915	rBV	2650472	3989253	59.29%	7.132%
23	14.592	1949	1956	1966	rBV	1279453	1952078	29.01%	3.490%
24	14.816	1988	1994	2005	rBV2	64432	188991	2.81%	0.338%
25	15.004	2022	2026	2029	rVB6	6371	8493	0.13%	0.015%
26	15.274	2071	2072	2078	rVB6	4375	7164	0.11%	0.013%
27	15.392	2088	2092	2096	rBV3	11438	16867	0.25%	0.030%
28	15.586	2118	2125	2134	rBV	3576553	5260593	78.18%	9.406%
29	15.704	2139	2145	2160	rVV	1096525	1623467	24.13%	2.903%
30	15.821	2160	2165	2175	rVB6	22175	51304	0.76%	0.092%
31	16.151	2215	2221	2227	rBV9	5316	10877	0.16%	0.019%
32	16.368	2253	2258	2264	rVB5	12687	19153	0.28%	0.034%
33	17.015	2362	2368	2372	rVB7	7212	11334	0.17%	0.020%
34	17.339	2417	2423	2431	rBV	1556030	2231110	33.16%	3.989%
35	17.439	2431	2440	2457	rVV2	4218764	6055032	89.99%	10.826%
36	17.639	2470	2474	2477	rBV4	7391	8919	0.13%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044412.D
 Acq On : 28 Feb 2024 19:57
 Operator : MA/JU
 Sample : P1535-09
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	18.027	2535	2540	2544	rBV7	14767	23320	0.35%	0.042%
38	18.080	2546	2549	2556	rVV8	6455	13281	0.20%	0.024%
39	18.157	2559	2562	2570	rVB9	7262	13214	0.20%	0.024%
40	18.245	2573	2577	2587	rBV3	39466	62884	0.93%	0.112%
41	18.327	2589	2591	2595	rVB5	5884	7735	0.11%	0.014%
42	18.604	2635	2638	2642	rBV5	11605	16343	0.24%	0.029%
43	18.662	2644	2648	2653	rVB8	11549	19574	0.29%	0.035%
44	18.733	2656	2660	2664	rBV7	6106	11312	0.17%	0.020%
45	19.298	2752	2756	2761	rBV	51624	72595	1.08%	0.130%
46	19.368	2764	2768	2774	rVV	43534	63058	0.94%	0.113%
47	19.533	2792	2796	2801	rBV3	25612	34870	0.52%	0.062%
48	19.686	2818	2822	2824	rBV3	26467	31526	0.47%	0.056%
49	19.739	2824	2831	2838	rVV	4877333	6728924	100.00%	12.031%
50	20.739	2998	3001	3004	rBV3	20635	22609	0.34%	0.040%
51	21.533	3131	3136	3148	rBV	1550762	2190840	32.56%	3.917%
52	23.803	3514	3522	3537	rBV2	3202781	6521037	96.91%	11.659%
53	23.962	3542	3549	3559	rVB	1108698	2303598	34.23%	4.119%




Sum of corrected areas: 55930717

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044412.D
Acq On : 28 Feb 2024 19:57
Operator : MA/JU
Sample : P1535-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

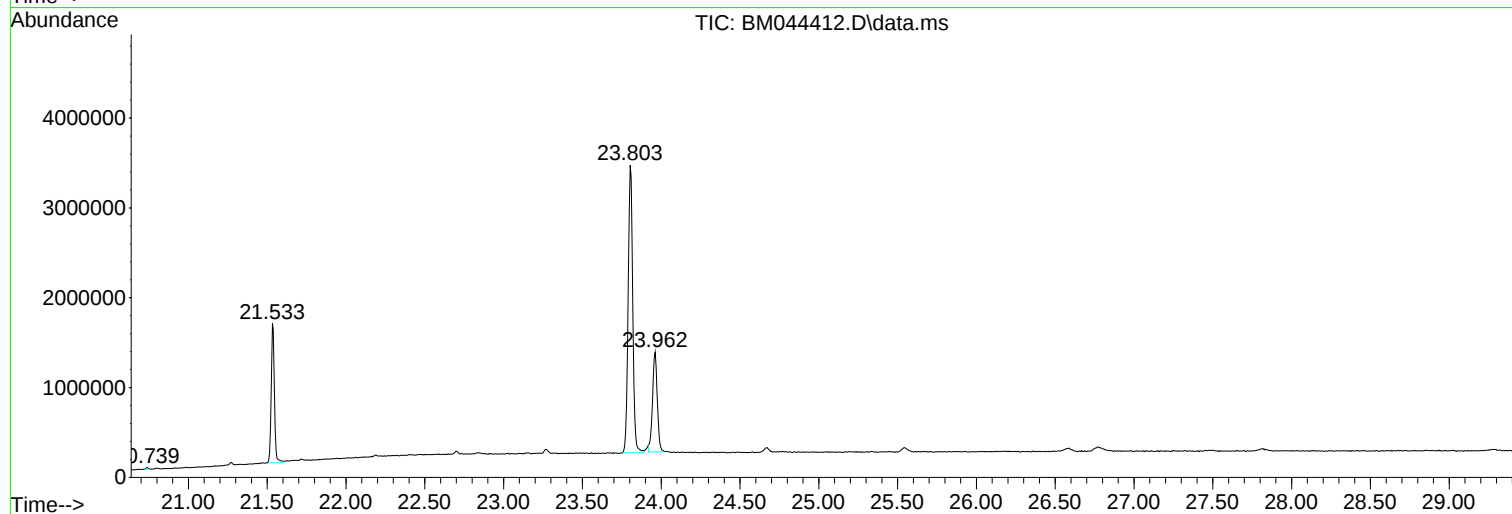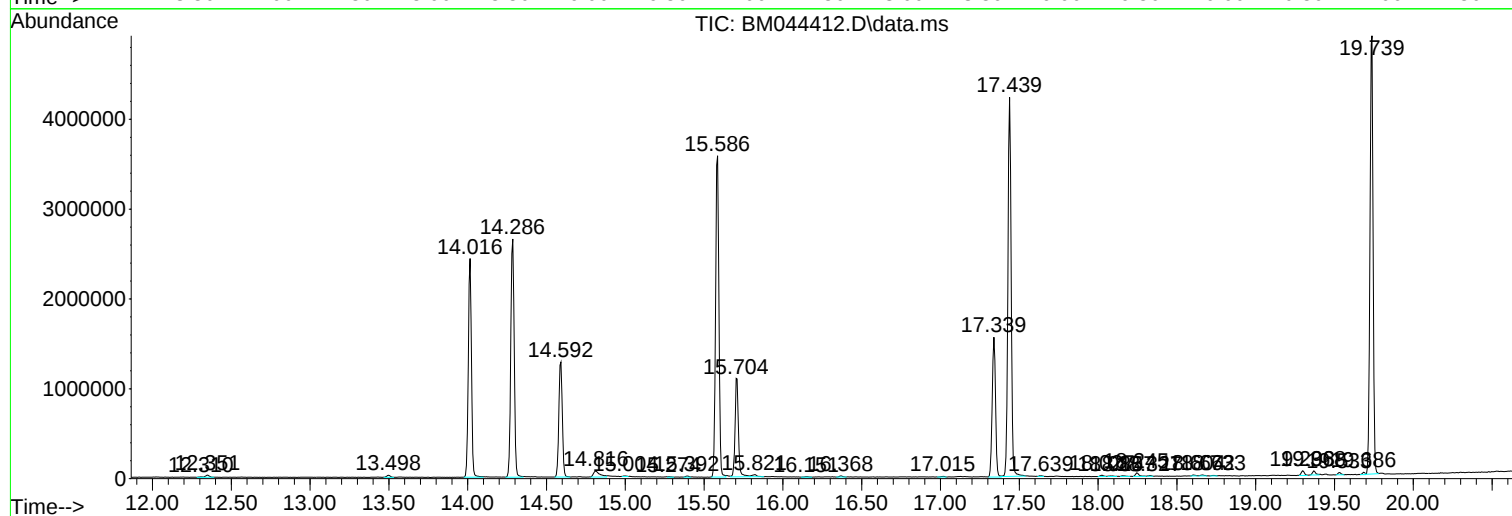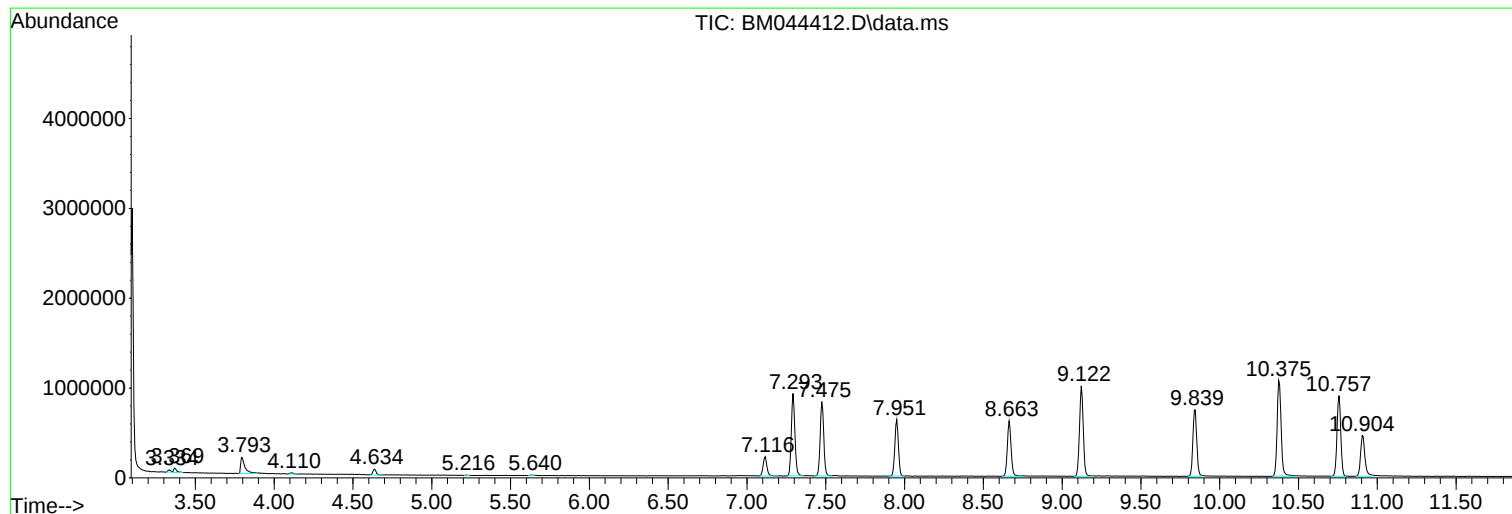

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044412.D
Acq On : 28 Feb 2024 19:57
Operator : MA/JU
Sample : P1535-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044412.D
Acq On : 28 Feb 2024 19:57
Operator : MA/JU
Sample : P1535-09
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc