

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044413.D
 Acq On : 28 Feb 2024 20:34
 Operator : MA/JU
 Sample : P1535-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	39	42	44	rBV4	13729	16122	0.28%	0.032%
2	3.369	44	48	53	rVB	44868	54285	0.96%	0.107%
3	3.793	117	120	144	rVB	198659	366964	6.48%	0.726%
4	4.111	171	174	179	rVB	15461	18672	0.33%	0.037%
5	4.634	258	263	271	rVB	72707	102741	1.81%	0.203%
6	7.110	678	684	693	rBV	188638	323841	5.72%	0.641%
7	7.293	708	715	729	rBV	920016	1464957	25.86%	2.898%
8	7.475	739	746	754	rBV	818933	1284355	22.67%	2.541%
9	7.946	817	826	834	rBV	629189	1027067	18.13%	2.032%
10	8.663	941	948	960	rBV	571230	929947	16.42%	1.840%
11	9.122	1017	1026	1037	rBV	980722	1638088	28.92%	3.241%
12	9.840	1139	1148	1160	rBV	759423	1261651	22.27%	2.496%
13	10.375	1231	1239	1256	rBV	1032721	1802570	31.82%	3.566%
14	10.751	1296	1303	1313	rVB	876893	1506350	26.59%	2.980%
15	10.904	1321	1329	1348	rBV	618290	1161468	20.51%	2.298%
16	12.345	1569	1574	1581	rVB	21915	38338	0.68%	0.076%
17	13.492	1763	1769	1775	rBV	20614	33190	0.59%	0.066%
18	14.010	1851	1857	1870	rBV	1940852	2843907	50.21%	5.626%
19	14.280	1896	1903	1916	rBV	2441222	3663448	64.68%	7.247%
20	14.586	1949	1955	1963	rBV	1299466	1920758	33.91%	3.800%
21	14.816	1988	1994	2006	rBV5	38246	133935	2.36%	0.265%
22	15.392	2087	2092	2096	rBV	21060	28386	0.50%	0.056%
23	15.580	2117	2124	2137	rBV	3116554	4574638	80.76%	9.050%
24	15.704	2139	2145	2160	rVV	895176	1310132	23.13%	2.592%
25	15.822	2162	2165	2170	rVB3	15779	25799	0.46%	0.051%
26	16.369	2254	2258	2265	rVB7	11325	17583	0.31%	0.035%
27	17.021	2360	2369	2371	rBV8	6575	10399	0.18%	0.021%
28	17.157	2388	2392	2401	rVB5	6054	13502	0.24%	0.027%
29	17.339	2416	2423	2433	rBV	1512124	2172348	38.35%	4.298%
30	17.439	2433	2440	2454	rVV	3592542	5084504	89.76%	10.059%
31	18.015	2535	2538	2542	rBV5	14863	19622	0.35%	0.039%
32	18.074	2545	2548	2554	rBV6	4588	8790	0.16%	0.017%
33	18.245	2571	2577	2584	rBV4	39202	59655	1.05%	0.118%
34	18.327	2587	2591	2596	rVB4	6182	8668	0.15%	0.017%
35	19.298	2752	2756	2761	rVB3	41237	55881	0.99%	0.111%
36	19.368	2764	2768	2772	rVV	35570	48916	0.86%	0.097%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044413.D
Acq On : 28 Feb 2024 20:34
Operator : MA/JU
Sample : P1535-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.445	2779	2781	2786	rVB6	8193	9329	0.16%	0.018%
38	19.527	2791	2795	2803	rBV4	26222	38423	0.68%	0.076%
39	19.686	2819	2822	2824	rBV3	20999	20813	0.37%	0.041%
40	19.733	2824	2830	2839	rVV	4253570	5664284	100.00%	11.206%
41	21.533	3131	3136	3147	rBV2	1527796	2118042	37.39%	4.190%
42	23.803	3514	3522	3536	rBV2	2610595	5440254	96.04%	10.762%
43	23.956	3542	3548	3561	rVB	1071488	2226248	39.30%	4.404%




Sum of corrected areas: 50548870

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044413.D
Acq On : 28 Feb 2024 20:34
Operator : MA/JU
Sample : P1535-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

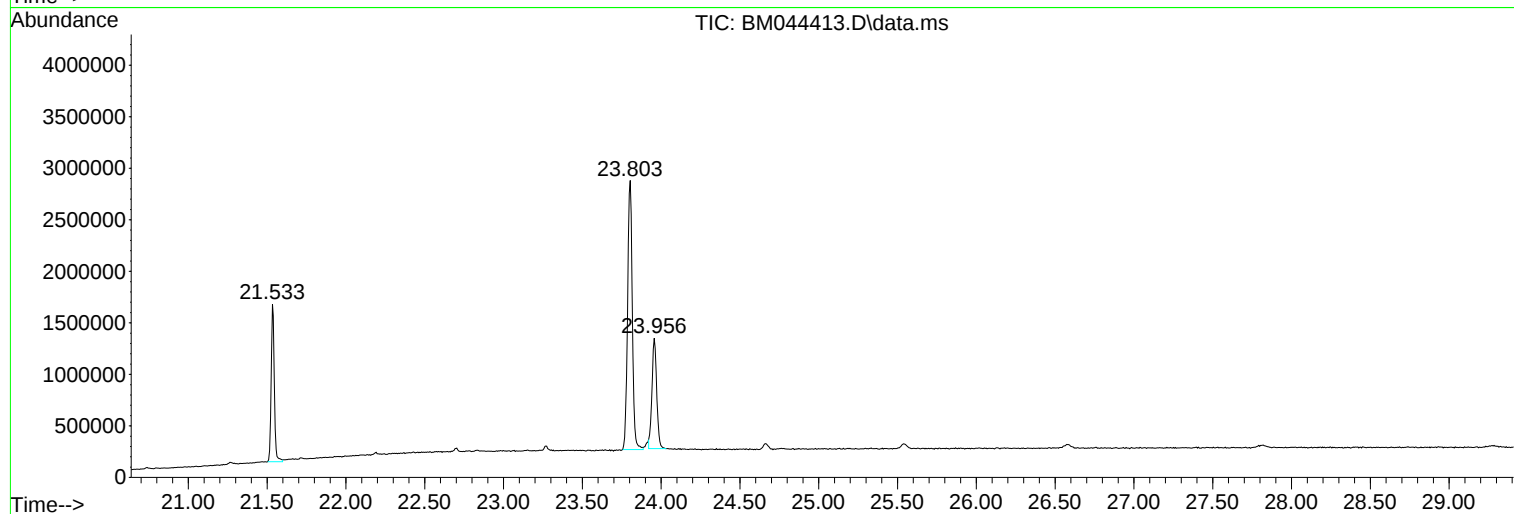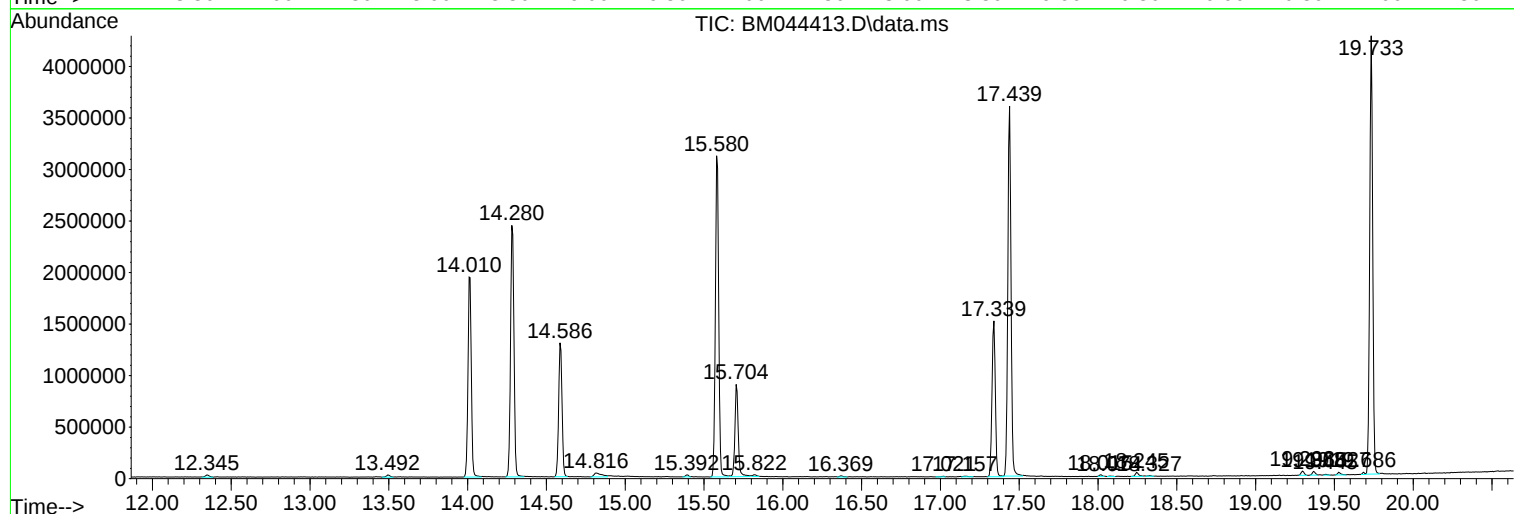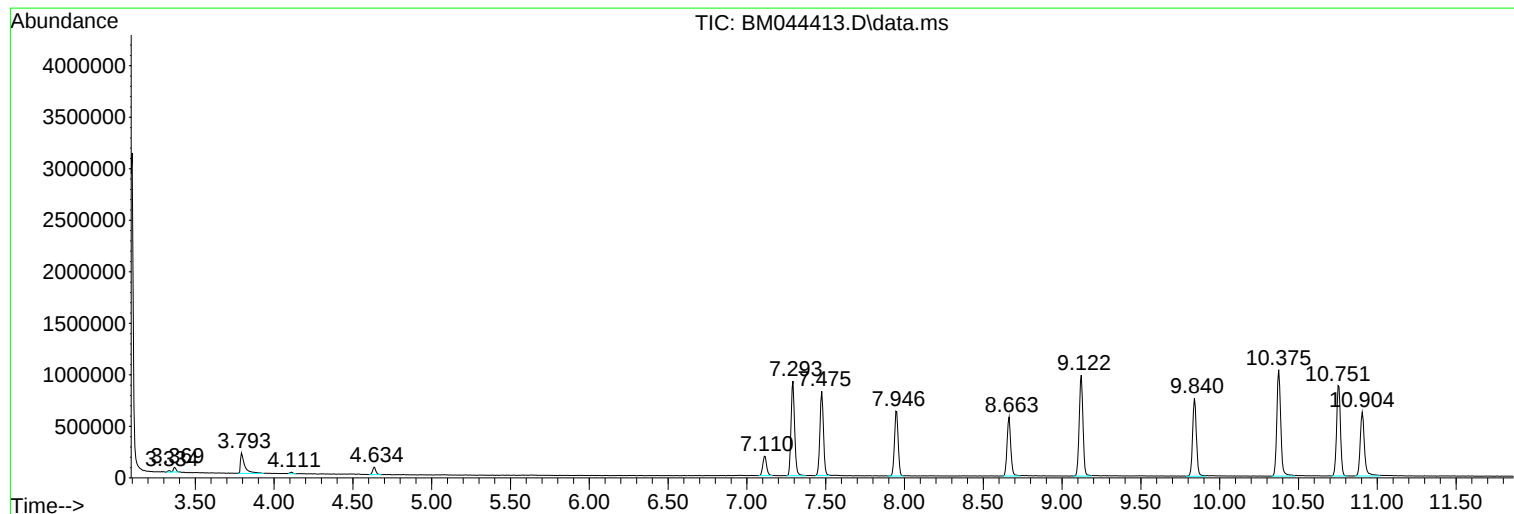

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044413.D
Acq On : 28 Feb 2024 20:34
Operator : MA/JU
Sample : P1535-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044413.D
Acq On : 28 Feb 2024 20:34
Operator : MA/JU
Sample : P1535-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------