

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044416.D
 Acq On : 28 Feb 2024 22:23
 Operator : MA/JU
 Sample : P1535-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	56	rVB	49804	70016	1.10%	0.127%
2	3.793	117	120	134	rBV	293980	500703	7.88%	0.909%
3	4.110	170	174	178	rVB2	13056	17417	0.27%	0.032%
4	5.640	429	434	439	rVB8	3845	7168	0.11%	0.013%
5	7.116	678	685	694	rBV	230593	378040	5.95%	0.687%
6	7.292	709	715	730	rBV	956166	1504937	23.69%	2.734%
7	7.475	739	746	755	rBV	866012	1373759	21.63%	2.495%
8	7.951	820	827	834	rVV	611594	958899	15.10%	1.742%
9	8.016	834	838	843	rVB7	4103	6790	0.11%	0.012%
10	8.663	941	948	959	rBV	662478	1084401	17.07%	1.970%
11	9.122	1019	1026	1039	rBV	1018132	1708938	26.90%	3.104%
12	9.510	1090	1092	1099	rVB6	6459	9722	0.15%	0.018%
13	9.845	1140	1149	1161	rBV	777865	1337458	21.06%	2.429%
14	10.375	1232	1239	1252	rBV	1159955	2017101	31.76%	3.664%
15	10.757	1296	1304	1314	rVB	879018	1457475	22.95%	2.647%
16	10.910	1321	1330	1344	rBV	853446	1615604	25.43%	2.935%
17	12.351	1569	1575	1581	rVB	25299	43832	0.69%	0.080%
18	13.421	1753	1757	1763	rVV4	8351	13593	0.21%	0.025%
19	13.498	1763	1770	1777	rVV2	27663	49163	0.77%	0.089%
20	13.574	1777	1783	1789	rVB8	5407	12609	0.20%	0.023%
21	14.015	1851	1858	1874	rBV	2364461	3305485	52.04%	6.004%
22	14.286	1895	1904	1918	rBV	2772405	4062904	63.96%	7.380%
23	14.492	1936	1939	1943	rVB6	4624	7912	0.12%	0.014%
24	14.592	1949	1956	1966	rBV	1254914	1861932	29.31%	3.382%
25	14.704	1973	1975	1984	rVB9	4144	7862	0.12%	0.014%
26	14.810	1986	1993	2006	rBV3	56812	184832	2.91%	0.336%
27	14.915	2009	2011	2016	rVB6	4142	7379	0.12%	0.013%
28	15.010	2024	2027	2032	rVB7	6972	11340	0.18%	0.021%
29	15.392	2088	2092	2095	rBV4	5032	6501	0.10%	0.012%
30	15.586	2118	2125	2139	rBV	3516304	5107014	80.40%	9.277%
31	15.709	2139	2146	2158	rVV	997449	1464018	23.05%	2.659%
32	15.827	2162	2166	2171	rVB4	16661	27516	0.43%	0.050%
33	16.286	2236	2244	2245	rBV7	3942	7753	0.12%	0.014%
34	16.309	2245	2248	2252	rVV6	7211	11647	0.18%	0.021%
35	16.368	2255	2258	2265	rVB7	13728	19178	0.30%	0.035%
36	17.015	2363	2368	2371	rVB6	6068	9085	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044416.D
 Acq On : 28 Feb 2024 22:23
 Operator : MA/JU
 Sample : P1535-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	17.109	2380	2384	2387	rBV5	9698	14334	0.23%	0.026%
38	17.221	2398	2403	2406	rBV7	5746	8491	0.13%	0.015%
39	17.339	2416	2423	2433	rBV	1499913	2109928	33.22%	3.833%
40	17.439	2433	2440	2452	rBV	3782845	5397656	84.98%	9.805%
41	17.645	2470	2475	2476	rBV4	5244	7293	0.11%	0.013%
42	17.851	2507	2510	2514	rVB5	5171	6718	0.11%	0.012%
43	18.027	2534	2540	2545	rVB	56664	79415	1.25%	0.144%
44	18.251	2573	2578	2586	rBV	101916	158305	2.49%	0.288%
45	18.574	2630	2633	2636	rVB4	12428	13924	0.22%	0.025%
46	18.686	2649	2652	2655	rVB5	8681	9509	0.15%	0.017%
47	18.733	2656	2660	2666	rVV5	16003	24844	0.39%	0.045%
48	19.209	2737	2741	2745	rVB4	18681	21071	0.33%	0.038%
49	19.297	2752	2756	2761	rBV2	48794	70274	1.11%	0.128%
50	19.345	2761	2764	2765	rBV3	13245	13118	0.21%	0.024%
51	19.368	2765	2768	2772	rVV	36611	48015	0.76%	0.087%
52	19.445	2778	2781	2784	rVB4	9793	11699	0.18%	0.021%
53	19.533	2791	2796	2802	rBV2	40211	62425	0.98%	0.113%
54	19.686	2819	2822	2824	rBV2	29117	30473	0.48%	0.055%
55	19.733	2824	2830	2838	rVV	4620818	6351987	100.00%	11.538%
56	20.739	2998	3001	3004	rBV4	23534	28949	0.46%	0.053%
57	21.268	3087	3091	3099	rBV3	115292	172510	2.72%	0.313%
58	21.533	3131	3136	3149	rBV2	1519892	2099377	33.05%	3.813%
59	23.803	3514	3522	3535	rBV2	2925473	5911385	93.06%	10.738%
60	23.956	3542	3548	3559	rVB	1021869	2131113	33.55%	3.871%




Sum of corrected areas: 55052796

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044416.D
Acq On : 28 Feb 2024 22:23
Operator : MA/JU
Sample : P1535-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

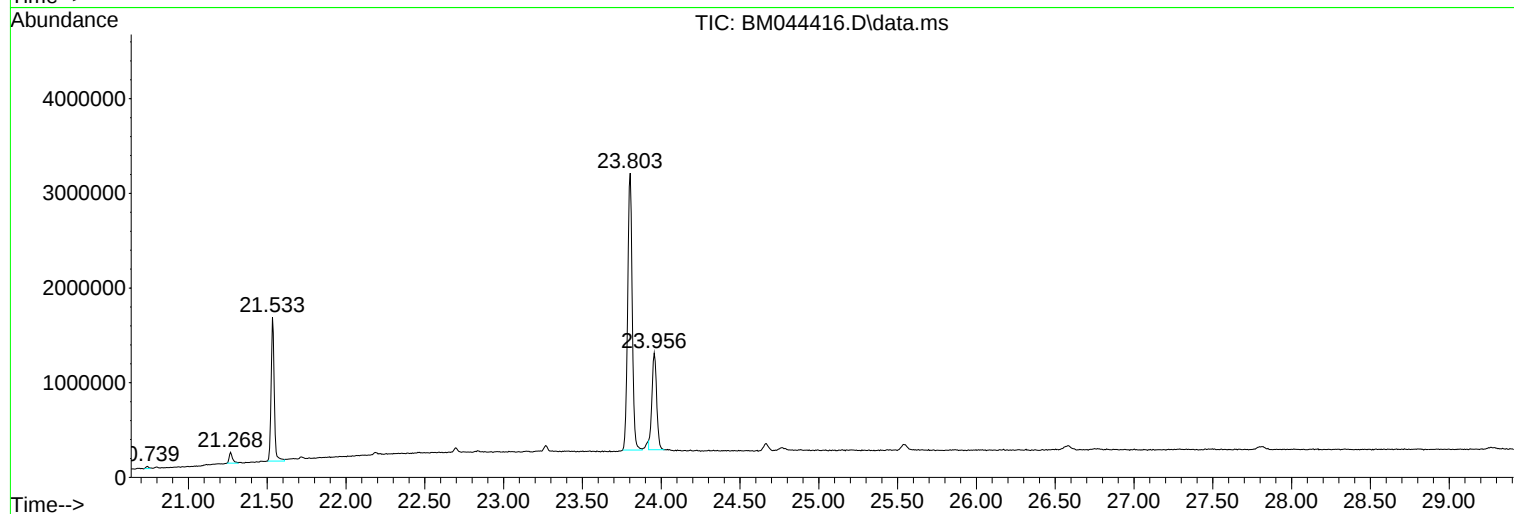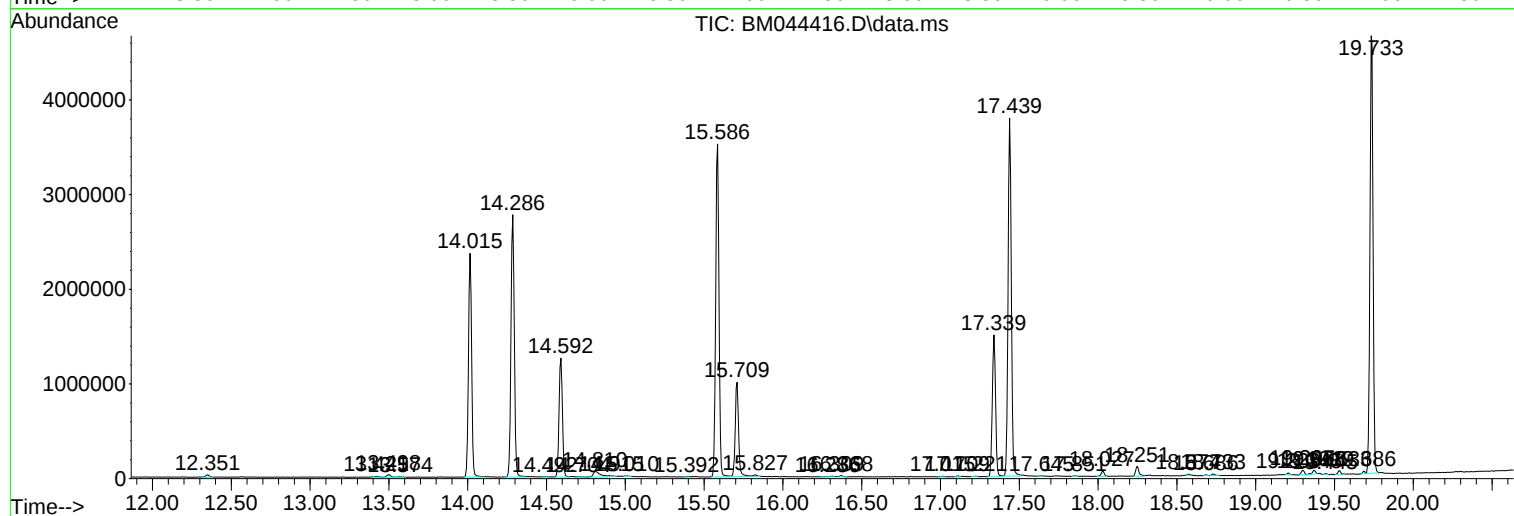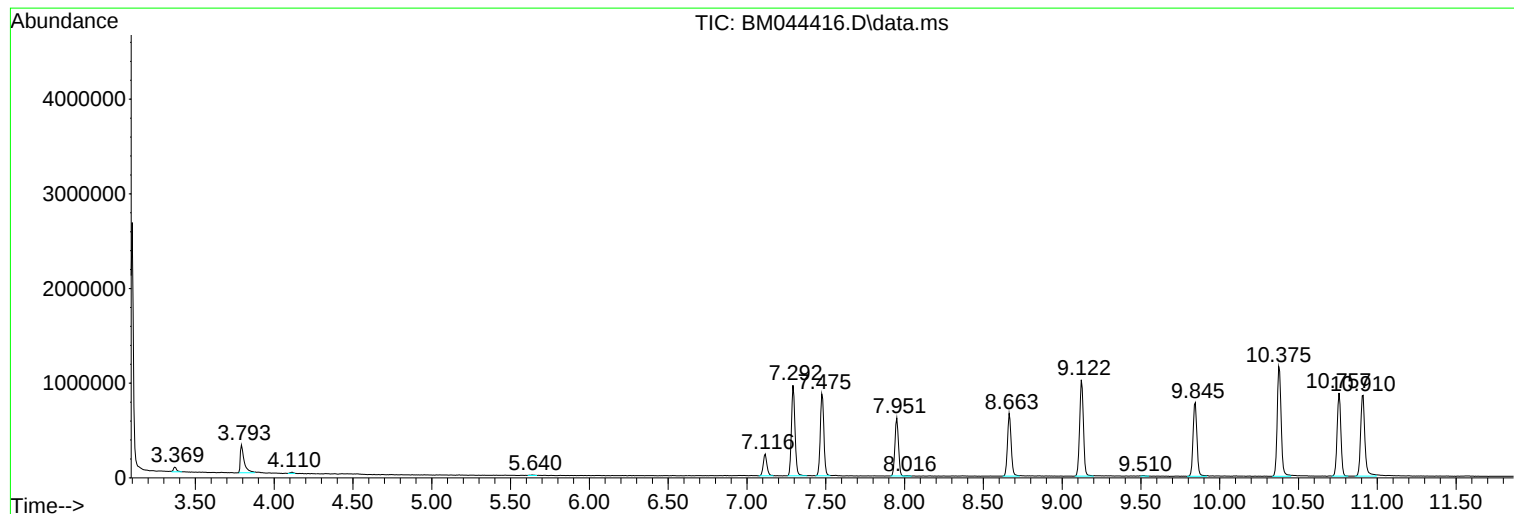

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044416.D
Acq On : 28 Feb 2024 22:23
Operator : MA/JU
Sample : P1535-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044416.D
Acq On : 28 Feb 2024 22:23
Operator : MA/JU
Sample : P1535-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc