

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044423.D
 Acq On : 29 Feb 2024 03:16
 Operator : MA/JU
 Sample : PB159340BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK340

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044423.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	54	rVB	80165	106669	2.13%	0.201%
2	3.781	115	118	144	rBV	957300	1575908	31.53%	2.963%
3	4.110	170	174	181	rVB3	14269	23284	0.47%	0.044%
4	6.498	574	580	581	rBV6	3174	5784	0.12%	0.011%
5	7.110	678	684	696	rBV	1037314	1637515	32.76%	3.078%
6	7.293	709	715	725	rBV	864136	1370103	27.41%	2.576%
7	7.475	738	746	754	rBV	1025985	1631477	32.64%	3.067%
8	7.945	819	826	835	rBV	607386	958388	19.17%	1.802%
9	8.663	937	948	959	rBV	1174024	1995734	39.93%	3.752%
10	9.122	1018	1026	1038	rBV	909315	1560185	31.21%	2.933%
11	9.839	1140	1148	1165	rBV	755837	1275794	25.52%	2.398%
12	10.375	1231	1239	1259	rBV	1137535	1977181	39.56%	3.717%
13	10.751	1296	1303	1311	rBV	838102	1445337	28.92%	2.717%
14	10.904	1321	1329	1349	rBV	1118009	2108255	42.18%	3.963%
15	12.345	1569	1574	1579	rBV	18329	30561	0.61%	0.057%
16	13.492	1764	1769	1775	rBV2	25622	41781	0.84%	0.079%
17	14.010	1851	1857	1872	rBV	1890651	2780332	55.62%	5.227%
18	14.280	1896	1903	1916	rBV	2328949	3519516	70.41%	6.617%
19	14.586	1947	1955	1964	rBV	1247451	1872192	37.46%	3.520%
20	14.798	1984	1991	2014	rBV	458794	1186046	23.73%	2.230%
21	15.263	2068	2070	2075	rVB6	5027	7136	0.14%	0.013%
22	15.580	2117	2124	2138	rBV	2952125	4286564	85.76%	8.059%
23	15.704	2139	2145	2159	rVV	745080	1085095	21.71%	2.040%
24	15.821	2162	2165	2171	rVB5	14079	20408	0.41%	0.038%
25	16.368	2253	2258	2263	rVB4	9435	13786	0.28%	0.026%
26	17.021	2365	2369	2373	rVB6	3986	7092	0.14%	0.013%
27	17.339	2416	2423	2430	rBV	1469791	2126183	42.54%	3.997%
28	17.439	2433	2440	2453	rVV	3147046	4535448	90.74%	8.526%
29	18.251	2574	2578	2584	rBV8	5673	9744	0.19%	0.018%
30	19.298	2751	2756	2760	rBV2	36537	49468	0.99%	0.093%
31	19.368	2763	2768	2773	rBV	31348	49678	0.99%	0.093%
32	19.686	2819	2822	2824	rBV3	7643	8927	0.18%	0.017%
33	19.733	2824	2830	2841	rVV	3711858	4998356	100.00%	9.397%
34	21.527	3130	3135	3147	rBV	1419561	2022730	40.47%	3.803%
35	23.797	3513	3521	3532	rBV2	2256380	4743776	94.91%	8.918%
36	23.950	3541	3547	3558	rVB	979652	2126174	42.54%	3.997%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044423.D
Acq On : 29 Feb 2024 03:16
Operator : MA/JU
Sample : PB159340BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK340

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 53192607

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044423.D
Acq On : 29 Feb 2024 03:16
Operator : MA/JU
Sample : PB159340BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

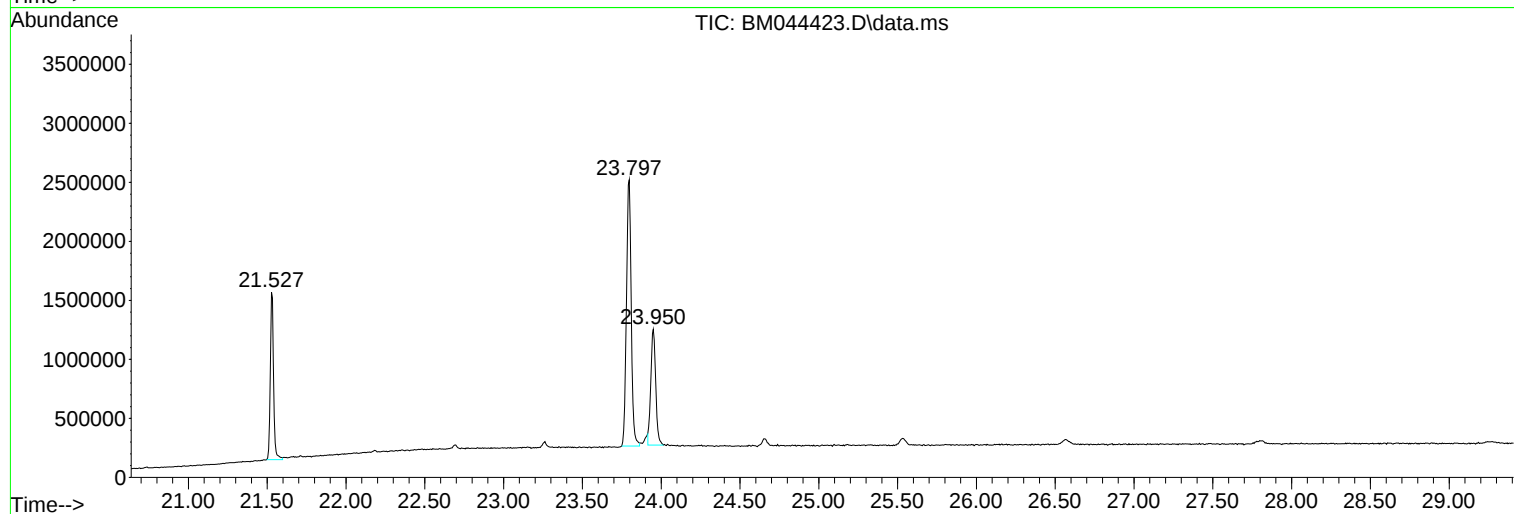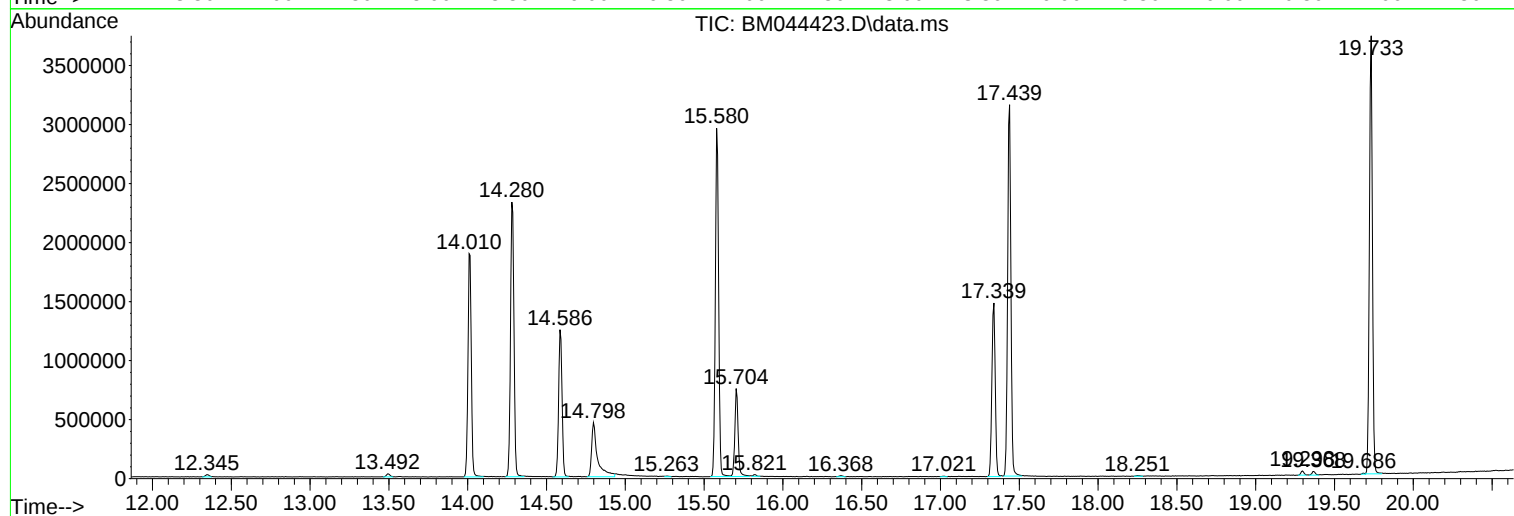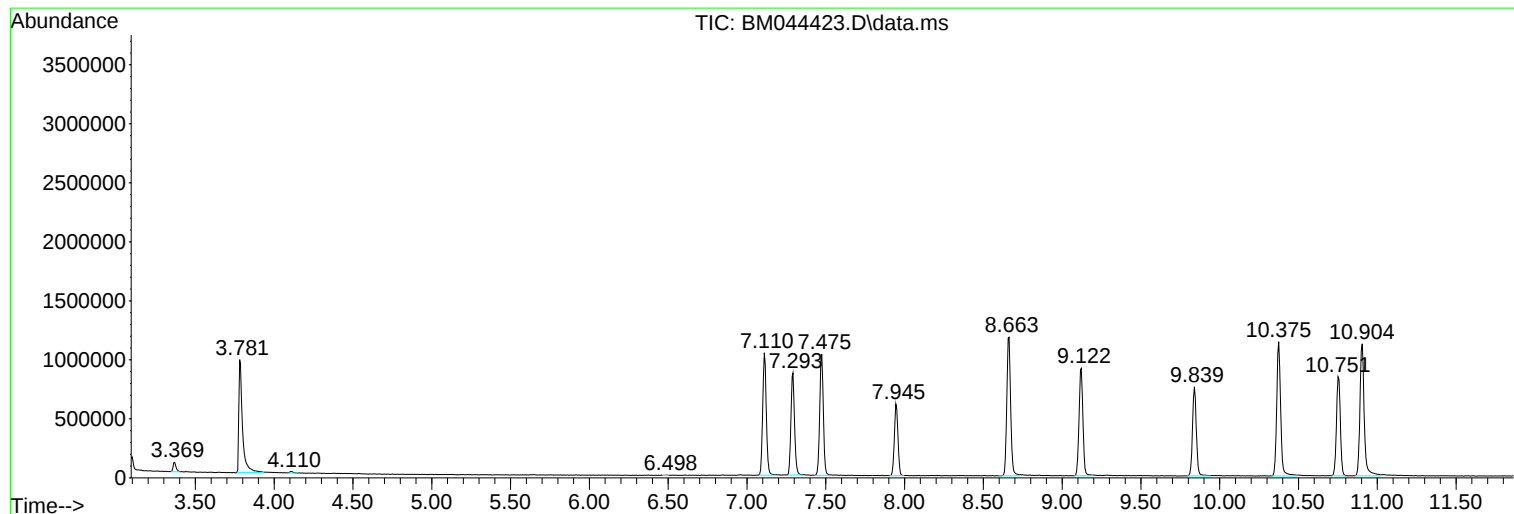

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044423.D
Acq On : 29 Feb 2024 03:16
Operator : MA/JU
Sample : PB159340BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044423.D
Acq On : 29 Feb 2024 03:16
Operator : MA/JU
Sample : PB159340BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK340

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------