

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044424.D
 Acq On : 29 Feb 2024 03:53
 Operator : MA/JU
 Sample : P1535-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	39	42	45	rVB2	12272	11305	0.18%	0.022%
2	3.369	45	48	52	rBV	47262	57602	0.94%	0.111%
3	3.805	118	122	136	rBV	71736	154469	2.52%	0.298%
4	4.110	169	174	181	rVB	97662	124036	2.02%	0.239%
5	4.634	258	263	269	rBV	139592	196918	3.21%	0.380%
6	5.640	430	434	439	rBV7	4286	6429	0.10%	0.012%
7	7.110	679	684	699	rVB	191459	323318	5.26%	0.624%
8	7.293	708	715	729	rBV	866656	1418548	23.10%	2.737%
9	7.475	739	746	757	rBV	748447	1186148	19.32%	2.288%
10	7.946	819	826	835	rBV	656307	1054294	17.17%	2.034%
11	8.663	941	948	957	rBV	553543	912732	14.86%	1.761%
12	9.122	1018	1026	1034	rBV	946383	1608116	26.19%	3.103%
13	9.840	1141	1148	1165	rBV	687309	1146385	18.67%	2.212%
14	10.375	1230	1239	1252	rBV	948462	1670462	27.20%	3.223%
15	10.751	1295	1303	1311	rBV	927952	1595120	25.97%	3.078%
16	10.904	1322	1329	1346	rBV	275173	559767	9.12%	1.080%
17	12.351	1568	1575	1583	rBV	22172	42395	0.69%	0.082%
18	13.422	1754	1757	1762	rVV7	3478	6780	0.11%	0.013%
19	13.498	1765	1770	1777	rVV2	16782	28367	0.46%	0.055%
20	14.016	1850	1858	1866	rBV	2132011	3052310	49.70%	5.889%
21	14.280	1896	1903	1921	rBV	2538389	3789192	61.70%	7.311%
22	14.586	1948	1955	1965	rBV	1370379	2038857	33.20%	3.934%
23	14.816	1987	1994	2007	rBV2	40046	138755	2.26%	0.268%
24	15.010	2023	2027	2030	rBV5	4629	6658	0.11%	0.013%
25	15.392	2086	2092	2099	rBV	24809	37803	0.62%	0.073%
26	15.580	2117	2124	2138	rBV	3308533	4797885	78.13%	9.257%
27	15.704	2139	2145	2158	rVV	847794	1226201	19.97%	2.366%
28	15.821	2162	2165	2169	rVB2	16365	22595	0.37%	0.044%
29	16.157	2216	2222	2226	rVB10	4350	7150	0.12%	0.014%
30	16.369	2254	2258	2262	rVB3	10451	15048	0.25%	0.029%
31	17.339	2416	2423	2433	rBV	1595577	2334424	38.01%	4.504%
32	17.439	2433	2440	2460	rVV	3821907	5430109	88.42%	10.477%
33	18.015	2532	2538	2542	rBV7	15821	22479	0.37%	0.043%
34	18.245	2573	2577	2588	rBV2	51767	76590	1.25%	0.148%
35	18.733	2655	2660	2664	rBV7	5493	10551	0.17%	0.020%
36	19.104	2719	2723	2729	rBV8	8687	14382	0.23%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044424.D
Acq On : 29 Feb 2024 03:53
Operator : MA/JU
Sample : P1535-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.298	2751	2756	2763	rBV2	42545	60244	0.98%	0.116%
38	19.368	2763	2768	2772	rBV	41768	56717	0.92%	0.109%
39	19.445	2778	2781	2785	rVB5	7989	8820	0.14%	0.017%
40	19.527	2791	2795	2801	rBV4	30476	42428	0.69%	0.082%
41	19.680	2818	2821	2824	rBV	21032	25745	0.42%	0.050%
42	19.733	2824	2830	2839	rVV	4602730	6141008	100.00%	11.848%
43	20.733	2997	3000	3004	rBV4	20729	26287	0.43%	0.051%
44	21.533	3130	3136	3145	rBV	1670162	2238422	36.45%	4.319%
45	23.797	3513	3521	3535	rBV2	2809081	5757647	93.76%	11.108%
46	23.950	3541	3547	3559	rVB	1120549	2349730	38.26%	4.533%




Sum of corrected areas: 51831228

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044424.D
Acq On : 29 Feb 2024 03:53
Operator : MA/JU
Sample : P1535-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

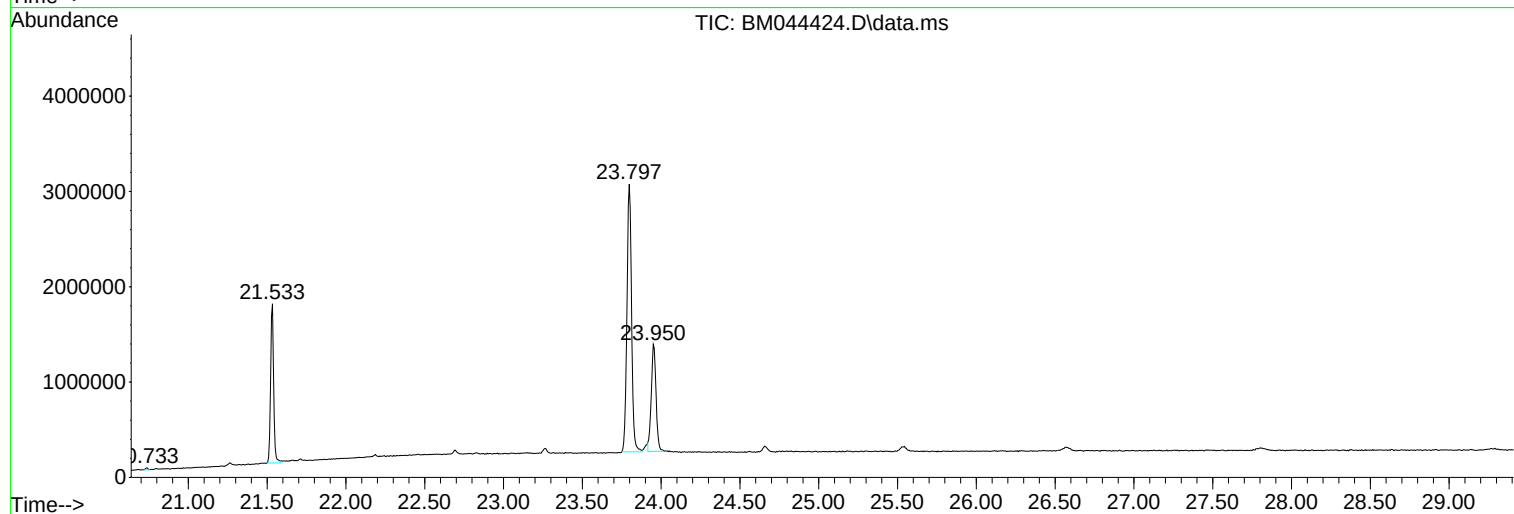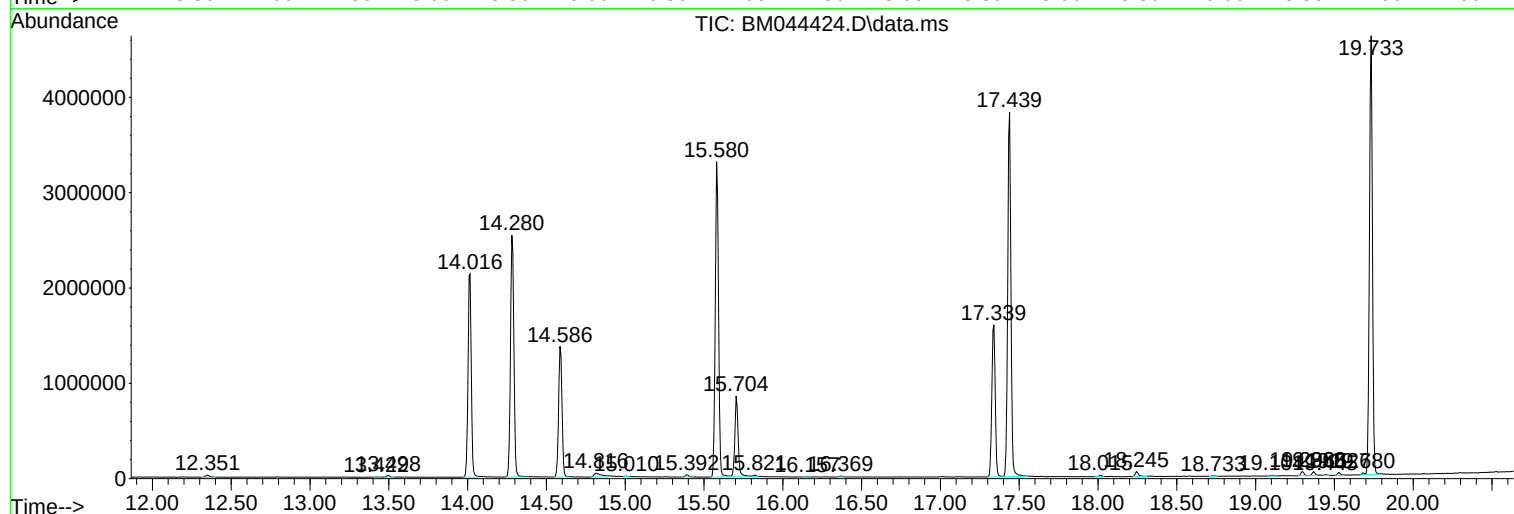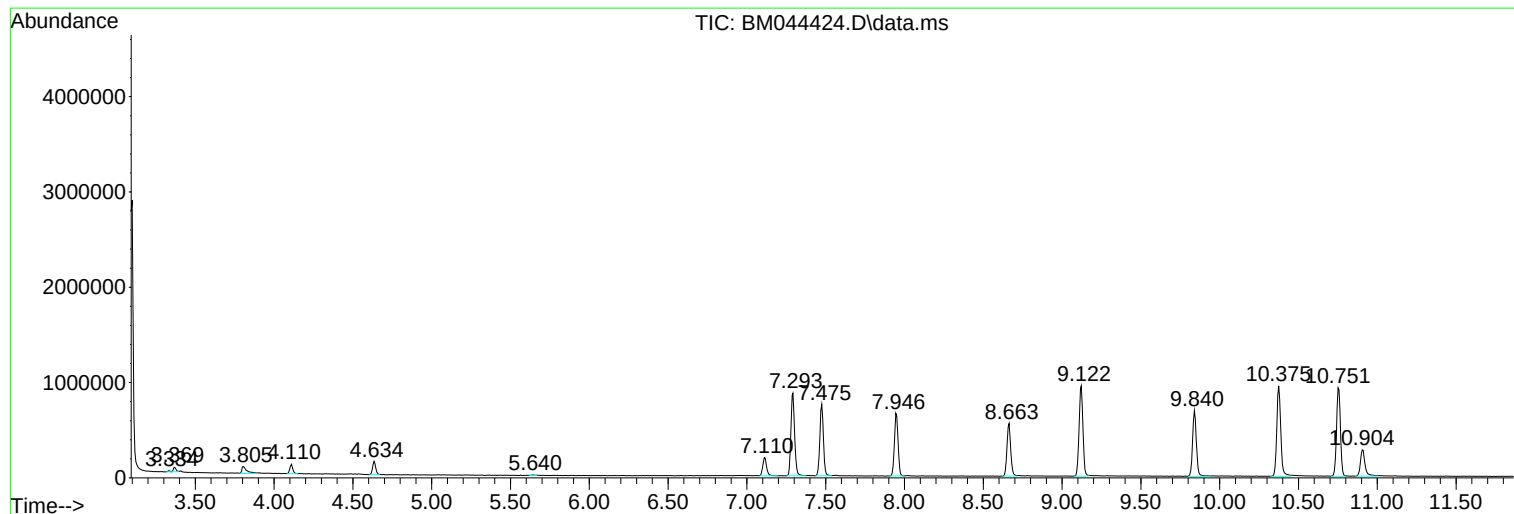

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044424.D
Acq On : 29 Feb 2024 03:53
Operator : MA/JU
Sample : P1535-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044424.D
Acq On : 29 Feb 2024 03:53
Operator : MA/JU
Sample : P1535-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------