

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044425.D
 Acq On : 29 Feb 2024 04:29
 Operator : MA/JU
 Sample : P1535-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	57	rVB	45566	60313	1.10%	0.124%
2	3.810	120	123	130	rBV	43954	80339	1.47%	0.165%
3	4.110	171	174	179	rVB	14762	19591	0.36%	0.040%
4	5.640	430	434	440	rBV7	5395	10349	0.19%	0.021%
5	7.110	678	684	693	rBV	183960	313367	5.72%	0.642%
6	7.293	707	715	730	rBV	837590	1335636	24.37%	2.736%
7	7.475	739	746	756	rBV	723569	1135092	20.71%	2.325%
8	7.551	757	759	764	rVB6	4917	7701	0.14%	0.016%
9	7.951	820	827	837	rBV	677251	1091989	19.93%	2.237%
10	8.369	891	898	900	rBV7	3315	5625	0.10%	0.012%
11	8.663	940	948	959	rBV	550171	917654	16.75%	1.880%
12	9.122	1018	1026	1035	rBV	915928	1507568	27.51%	3.089%
13	9.287	1051	1054	1059	rVB7	4487	5908	0.11%	0.012%
14	9.839	1140	1148	1159	rBV	626956	1074568	19.61%	2.201%
15	10.375	1232	1239	1251	rBV	917279	1642296	29.97%	3.365%
16	10.757	1296	1304	1314	rVB	964992	1655600	30.21%	3.392%
17	10.910	1323	1330	1340	rBV	176498	350317	6.39%	0.718%
18	12.351	1568	1575	1582	rVB2	20984	35098	0.64%	0.072%
19	13.422	1753	1757	1762	rVB6	5392	7662	0.14%	0.016%
20	13.498	1765	1770	1777	rVB	29079	45664	0.83%	0.094%
21	14.016	1851	1858	1869	rBV	2071926	2895921	52.84%	5.933%
22	14.286	1896	1904	1919	rBV	2375231	3600615	65.70%	7.377%
23	14.586	1948	1955	1963	rBV	1387676	2108544	38.48%	4.320%
24	14.816	1988	1994	2005	rBV3	40354	123792	2.26%	0.254%
25	15.016	2027	2028	2032	rVB4	8605	5628	0.10%	0.012%
26	15.580	2117	2124	2134	rBV	3002084	4459177	81.37%	9.135%
27	15.704	2139	2145	2161	rVV	738594	1130400	20.63%	2.316%
28	15.821	2162	2165	2172	rVB6	16966	32309	0.59%	0.066%
29	16.374	2252	2259	2262	rBV5	10395	17000	0.31%	0.035%
30	17.015	2364	2368	2370	rBV5	6393	8072	0.15%	0.017%
31	17.221	2400	2403	2406	rVB4	6018	6495	0.12%	0.013%
32	17.339	2416	2423	2433	rBV	1656019	2396819	43.74%	4.910%
33	17.439	2433	2440	2458	rVV	3268457	4716701	86.07%	9.663%
34	17.639	2472	2474	2479	rVB6	4722	6079	0.11%	0.012%
35	18.015	2536	2538	2544	rVB7	9943	14549	0.27%	0.030%
36	18.245	2573	2577	2586	rBV2	84562	126289	2.30%	0.259%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044425.D
 Acq On : 29 Feb 2024 04:29
 Operator : MA/JU
 Sample : P1535-13
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	18.574	2624	2633	2639	rBV9	18057	46464	0.85%	0.095%
38	18.733	2656	2660	2667	rBV9	8798	15133	0.28%	0.031%
39	19.298	2752	2756	2763	rVB3	41538	53896	0.98%	0.110%
40	19.368	2764	2768	2772	rBV	41870	60700	1.11%	0.124%
41	19.409	2772	2775	2778	rVV4	10161	11551	0.21%	0.024%
42	19.527	2791	2795	2801	rBV4	67899	91646	1.67%	0.188%
43	19.686	2819	2822	2824	rBV2	26303	28057	0.51%	0.057%
44	19.733	2824	2830	2839	rVV	4090062	5480121	100.00%	11.227%
45	20.733	2998	3000	3004	rVB4	26066	26971	0.49%	0.055%
46	21.268	3088	3091	3098	rBV5	43649	68743	1.25%	0.141%
47	21.533	3131	3136	3142	rBV	1734824	2277448	41.56%	4.666%
48	23.797	3513	3521	3535	rBV2	2512654	5179506	94.51%	10.611%
49	23.956	3541	3548	3560	rVB	1142356	2520984	46.00%	5.165%




Sum of corrected areas: 48811947

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044425.D
Acq On : 29 Feb 2024 04:29
Operator : MA/JU
Sample : P1535-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

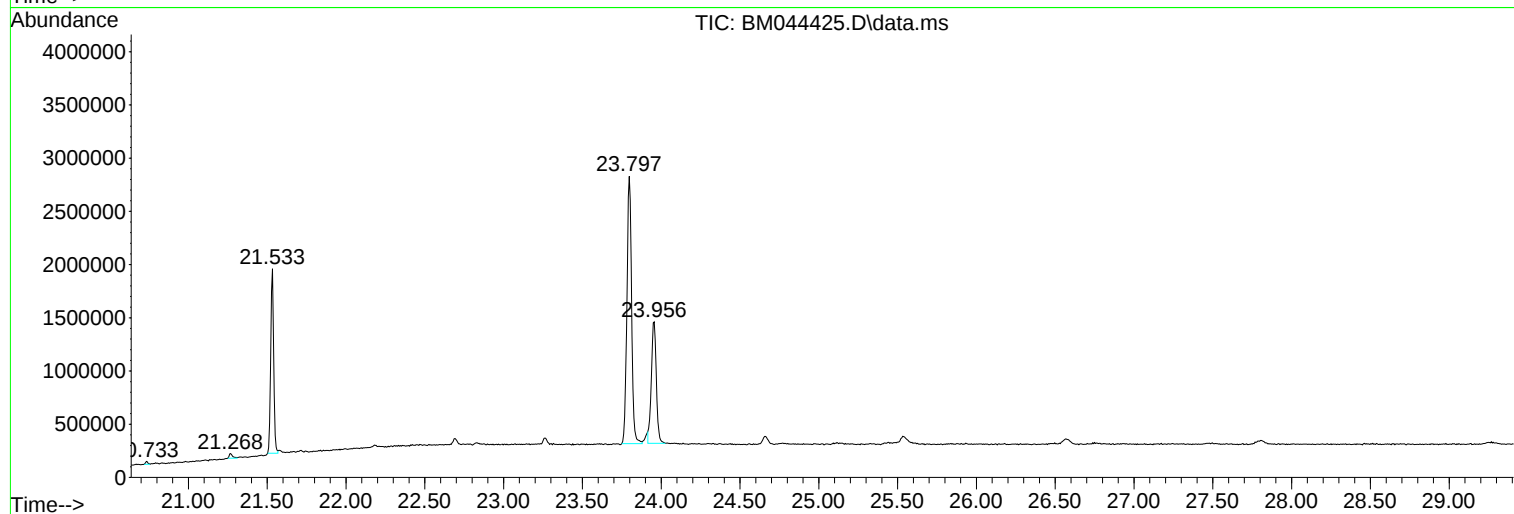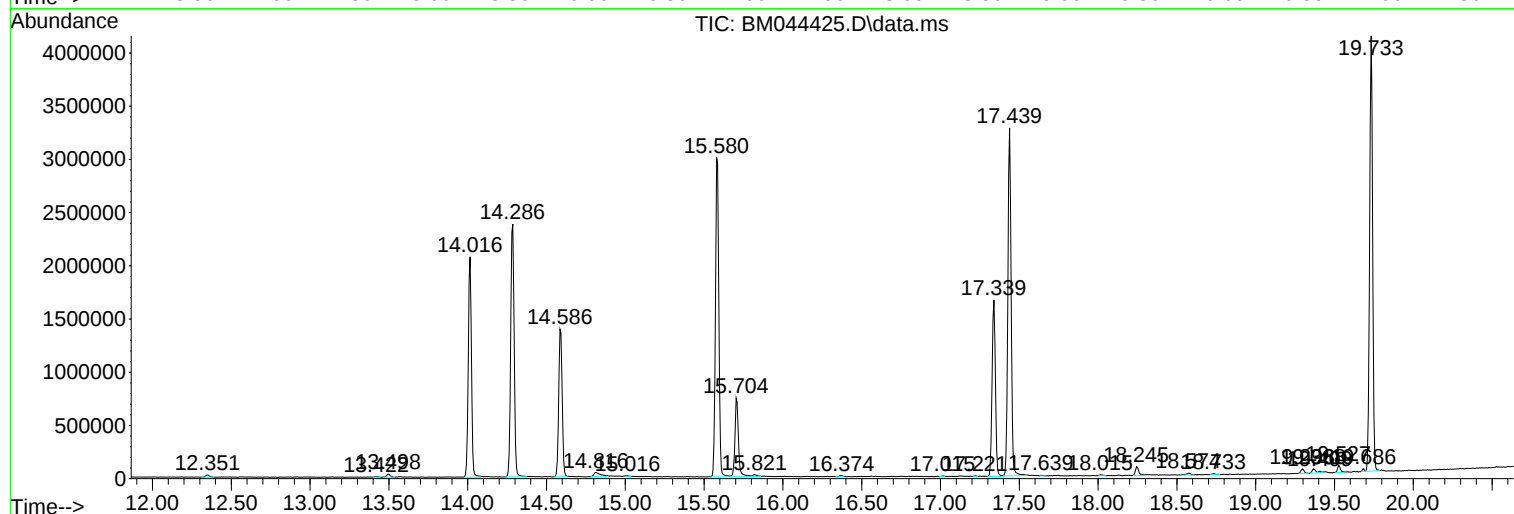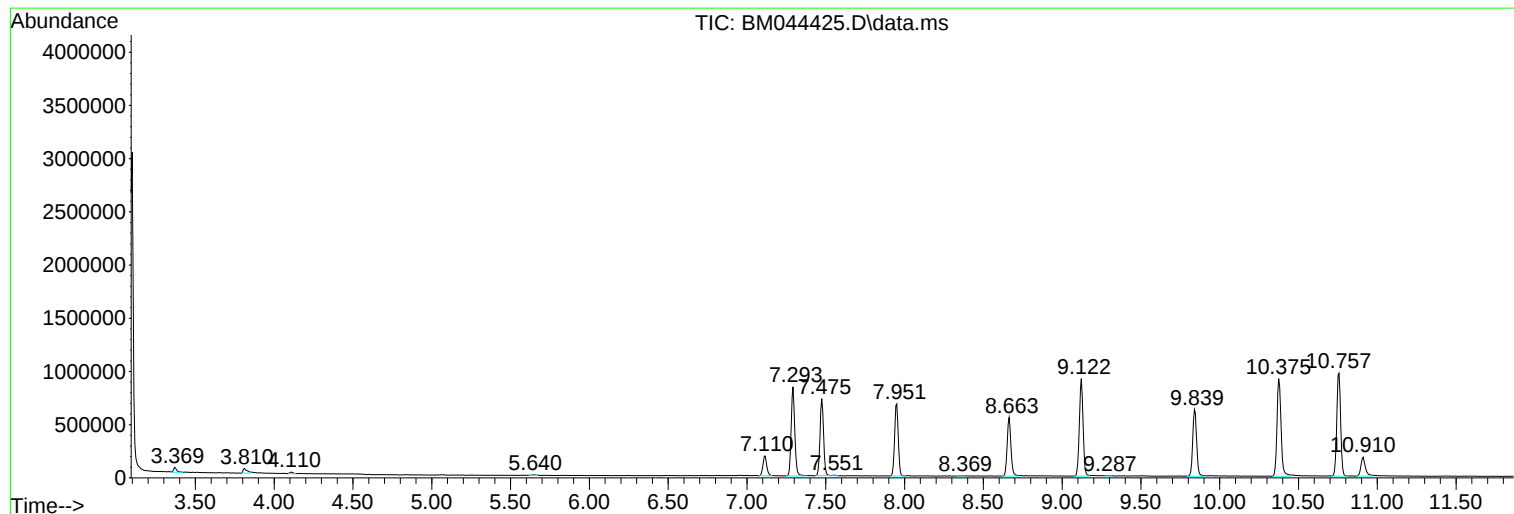

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044425.D
Acq On : 29 Feb 2024 04:29
Operator : MA/JU
Sample : P1535-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044425.D
Acq On : 29 Feb 2024 04:29
Operator : MA/JU
Sample : P1535-13
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AB9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc