

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044426.D
 Acq On : 29 Feb 2024 05:42
 Operator : MA/JU
 Sample : P1535-15
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	39	42	45	rBV2	34237	41135	0.66%	0.079%
2	3.369	45	48	54	rVB	49486	56244	0.91%	0.108%
3	3.804	119	122	132	rBV	58256	112426	1.82%	0.216%
4	4.110	170	174	179	rVB3	12747	18216	0.29%	0.035%
5	4.634	260	263	268	rVB7	10261	13572	0.22%	0.026%
6	7.116	677	685	694	rBV	211409	353853	5.71%	0.681%
7	7.292	708	715	726	rBV	948431	1502319	24.25%	2.891%
8	7.475	739	746	754	rBV	862925	1352293	21.83%	2.602%
9	7.557	759	760	764	rVB4	5322	6258	0.10%	0.012%
10	7.951	819	827	834	rBV	571967	904311	14.60%	1.740%
11	8.663	939	948	961	rBV	633912	1033671	16.69%	1.989%
12	9.122	1018	1026	1036	rBV	1035162	1721491	27.79%	3.312%
13	9.839	1138	1148	1158	rBV	777262	1338523	21.61%	2.576%
14	10.375	1231	1239	1256	rBV	1090248	1951595	31.51%	3.755%
15	10.533	1263	1266	1271	rVB8	5501	8306	0.13%	0.016%
16	10.757	1296	1304	1312	rBV	828106	1384316	22.35%	2.664%
17	10.910	1321	1330	1340	rBV	313080	611779	9.88%	1.177%
18	12.351	1570	1575	1583	rVB	22978	39471	0.64%	0.076%
19	13.498	1763	1770	1776	rBV	100269	164557	2.66%	0.317%
20	14.015	1851	1858	1873	rBV	2247688	3158083	50.99%	6.077%
21	14.286	1895	1904	1917	rBV	2600235	3934542	63.52%	7.571%
22	14.592	1949	1956	1965	rBV	1180451	1765332	28.50%	3.397%
23	14.815	1986	1994	2011	rBV4	47321	189532	3.06%	0.365%
24	15.021	2022	2029	2038	rVB4	6837	20355	0.33%	0.039%
25	15.392	2088	2092	2095	rBV	15540	19946	0.32%	0.038%
26	15.586	2118	2125	2139	rBV	3281625	4899429	79.10%	9.427%
27	15.704	2139	2145	2160	rVV	969720	1486085	23.99%	2.860%
28	15.815	2160	2164	2177	rVB5	22263	62016	1.00%	0.119%
29	16.368	2253	2258	2265	rVB9	12339	21711	0.35%	0.042%
30	17.021	2364	2369	2374	rVB9	9045	17213	0.28%	0.033%
31	17.115	2380	2385	2386	rBV5	4465	7680	0.12%	0.015%
32	17.339	2416	2423	2433	rBV	1404179	2012129	32.49%	3.872%
33	17.439	2433	2440	2458	rBV	3882223	5553020	89.65%	10.685%
34	17.639	2470	2474	2479	rVB5	6133	10409	0.17%	0.020%
35	18.015	2532	2538	2543	rVB9	12666	22902	0.37%	0.044%
36	18.245	2573	2577	2583	rBV3	46791	69037	1.11%	0.133%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044426.D
Acq On : 29 Feb 2024 05:42
Operator : MA/JU
Sample : P1535-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	18.456	2609	2613	2620	rBV3	22324	34368	0.55%	0.066%
38	19.103	2721	2723	2727	rVB5	8662	10344	0.17%	0.020%
39	19.297	2752	2756	2760	rBV2	46599	59681	0.96%	0.115%
40	19.368	2764	2768	2773	rBV2	41232	63921	1.03%	0.123%
41	19.527	2791	2795	2801	rBV3	40402	56640	0.91%	0.109%
42	19.686	2818	2822	2824	rBV2	26311	29322	0.47%	0.056%
43	19.733	2824	2830	2839	rVV	4689071	6193965	100.00%	11.918%
44	21.533	3131	3136	3146	rBV	1406326	1930366	31.17%	3.714%
45	23.803	3514	3522	3535	rBV2	2829989	5739680	92.67%	11.044%
46	23.956	3542	3548	3558	rVB	961826	1987889	32.09%	3.825%




Sum of corrected areas: 51969933

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044426.D
Acq On : 29 Feb 2024 05:42
Operator : MA/JU
Sample : P1535-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

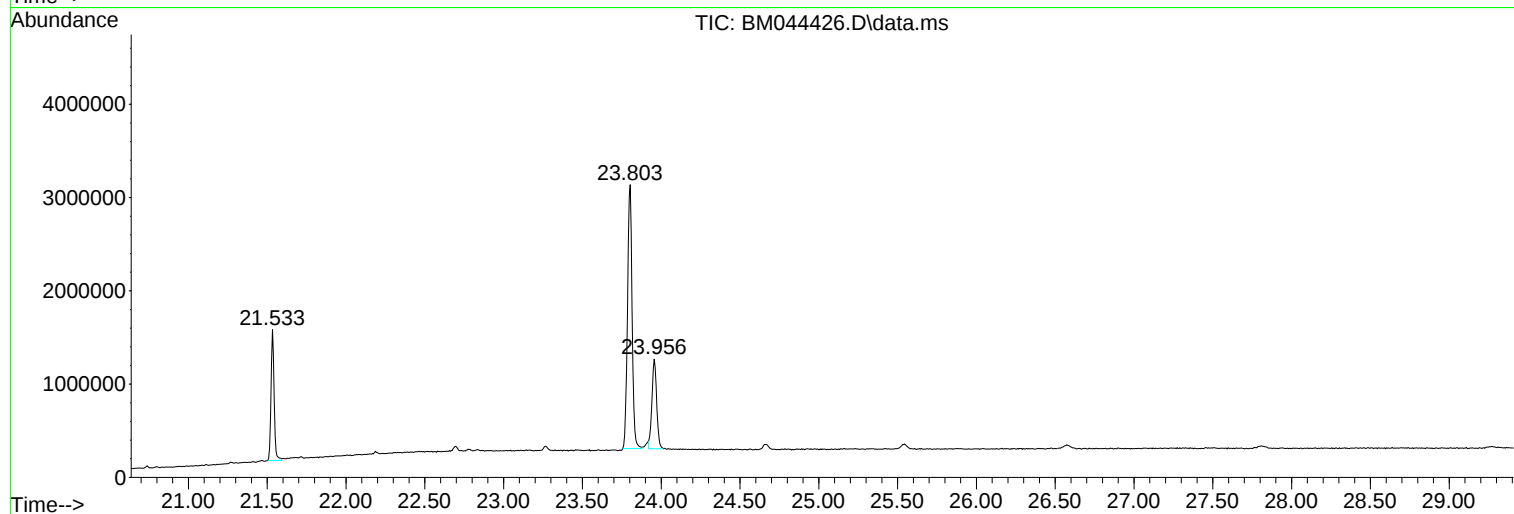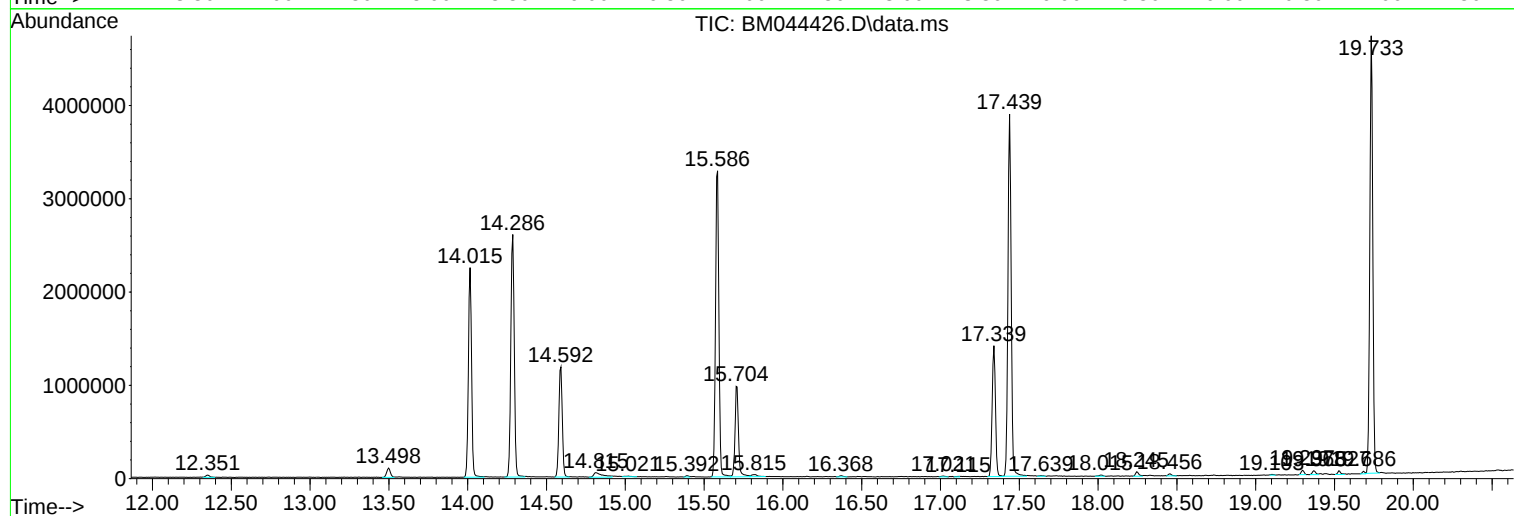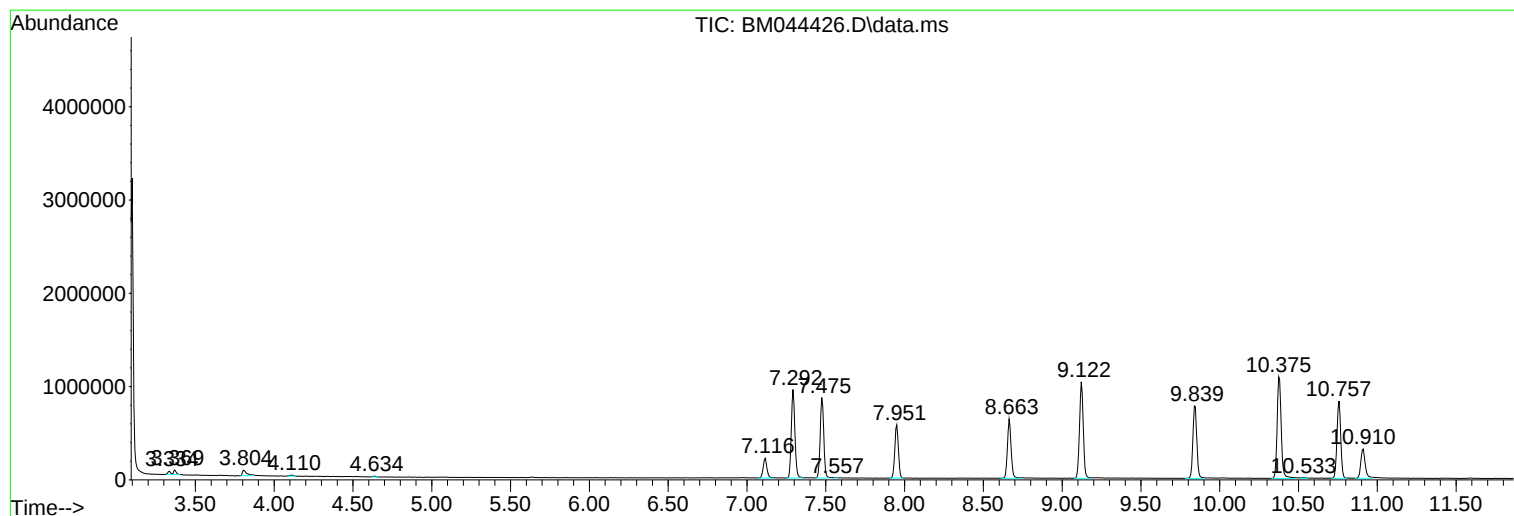

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044426.D
Acq On : 29 Feb 2024 05:42
Operator : MA/JU
Sample : P1535-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044426.D
Acq On : 29 Feb 2024 05:42
Operator : MA/JU
Sample : P1535-15
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc