

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044427.D
 Acq On : 29 Feb 2024 06:19
 Operator : MA/JU
 Sample : P1535-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	54	rVB	47849	57287	0.88%	0.106%
2	3.799	118	121	135	rBV	104571	199283	3.06%	0.370%
3	4.110	171	174	178	rVB2	15133	17767	0.27%	0.033%
4	4.634	259	263	270	rVB	50430	74586	1.15%	0.139%
5	7.116	678	685	694	rBV	206876	340668	5.24%	0.633%
6	7.292	709	715	726	rBV	925019	1456056	22.38%	2.707%
7	7.475	739	746	757	rBV	827535	1315750	20.22%	2.446%
8	7.563	758	761	765	rVB5	5255	7531	0.12%	0.014%
9	7.951	818	827	837	rBV	620594	1004642	15.44%	1.868%
10	8.663	940	948	960	rBV	603517	995304	15.30%	1.850%
11	9.122	1018	1026	1042	rBV	1034925	1702768	26.17%	3.165%
12	9.839	1140	1148	1159	rBV	770762	1308241	20.11%	2.432%
13	10.375	1231	1239	1256	rBV	1077669	1894842	29.12%	3.522%
14	10.757	1297	1304	1314	rBV	908848	1512483	23.24%	2.812%
15	10.904	1321	1329	1342	rBV	556636	1080392	16.60%	2.008%
16	12.345	1568	1574	1581	rVB	22465	39160	0.60%	0.073%
17	13.498	1765	1770	1778	rVB	20339	34584	0.53%	0.064%
18	14.016	1850	1858	1872	rBV	2235434	3117995	47.92%	5.796%
19	14.286	1896	1904	1918	rBV	2622118	3880556	59.64%	7.214%
20	14.592	1949	1956	1966	rBV	1313203	1936023	29.75%	3.599%
21	14.815	1985	1994	2011	rBV3	44501	177202	2.72%	0.329%
22	15.010	2023	2027	2029	rBV5	6071	9039	0.14%	0.017%
23	15.586	2118	2125	2139	rBV	3249993	4816385	74.02%	8.953%
24	15.710	2139	2146	2161	rVV	1031549	1518148	23.33%	2.822%
25	15.821	2162	2165	2171	rVB3	18622	30959	0.48%	0.058%
26	16.368	2254	2258	2265	rVB7	10799	17043	0.26%	0.032%
27	16.756	2318	2324	2328	rBV7	3996	6890	0.11%	0.013%
28	17.021	2364	2369	2372	rVB8	6884	8938	0.14%	0.017%
29	17.339	2416	2423	2433	rBV	1579027	2220471	34.12%	4.128%
30	17.439	2433	2440	2452	rBV	3875727	5606326	86.16%	10.422%
31	17.639	2471	2474	2480	rVB6	5723	10216	0.16%	0.019%
32	18.015	2534	2538	2544	rVB6	19536	30172	0.46%	0.056%
33	18.245	2573	2577	2584	rBV3	29744	49737	0.76%	0.092%
34	18.580	2632	2634	2638	rVB5	5146	6735	0.10%	0.013%
35	19.103	2720	2723	2727	rBV4	13745	16752	0.26%	0.031%
36	19.298	2751	2756	2761	rBV4	49413	68436	1.05%	0.127%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044427.D
Acq On : 29 Feb 2024 06:19
Operator : MA/JU
Sample : P1535-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.368	2763	2768	2773	rBV2	41118	64386	0.99%	0.120%
38	19.450	2778	2782	2784	rVB5	6352	9721	0.15%	0.018%
39	19.533	2792	2796	2799	rBV3	20674	25936	0.40%	0.048%
40	19.686	2818	2822	2824	rBV3	23584	27100	0.42%	0.050%
41	19.733	2824	2830	2839	rVV	4782531	6506985	100.00%	12.096%
42	21.533	3131	3136	3147	rBV	1538084	2106398	32.37%	3.916%
43	23.803	3514	3522	3535	rBV2	3064701	6255164	96.13%	11.628%
44	23.956	3542	3548	3561	rVB	1064197	2228760	34.25%	4.143%




Sum of corrected areas: 53793817

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044427.D
Acq On : 29 Feb 2024 06:19
Operator : MA/JU
Sample : P1535-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

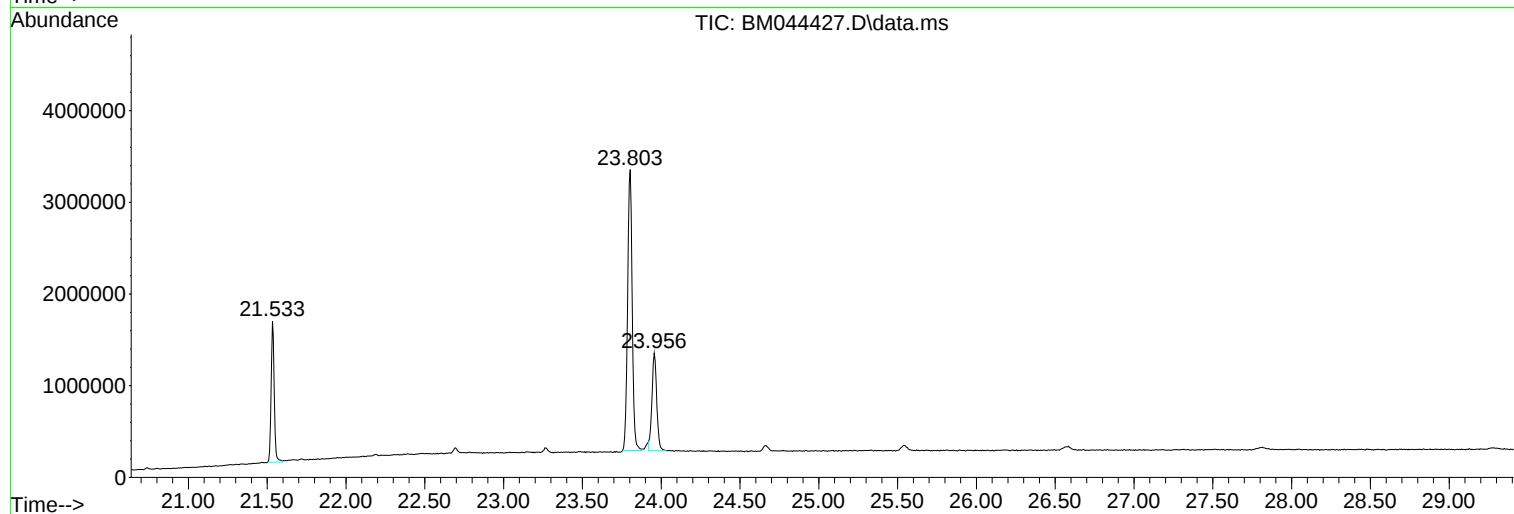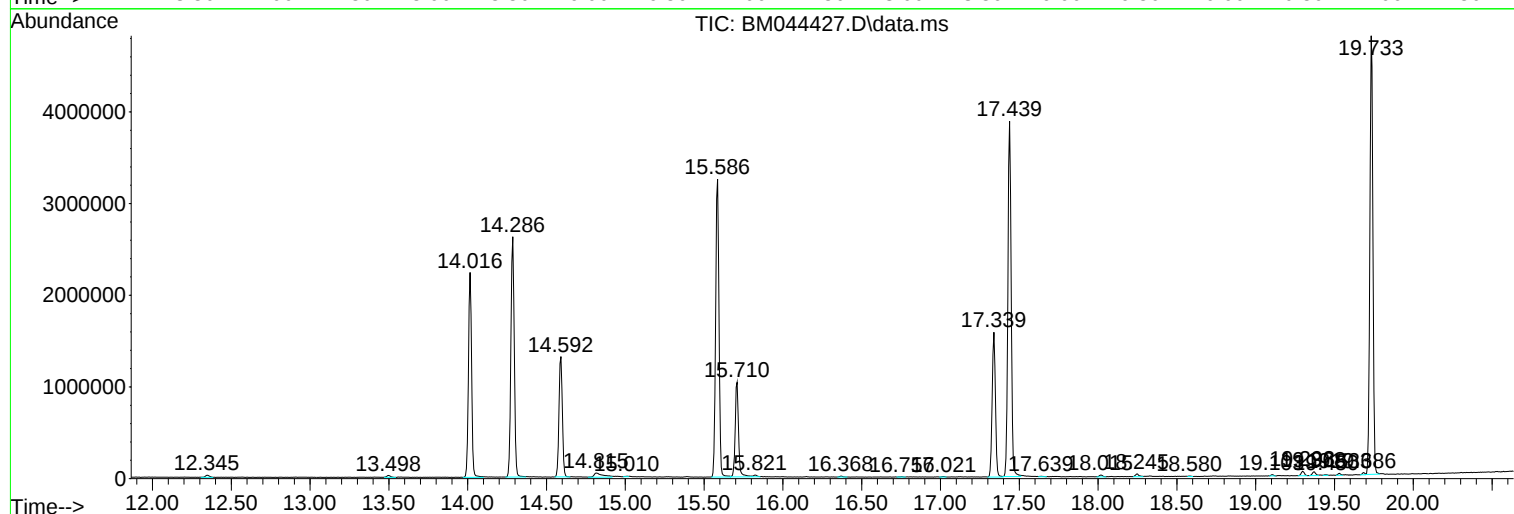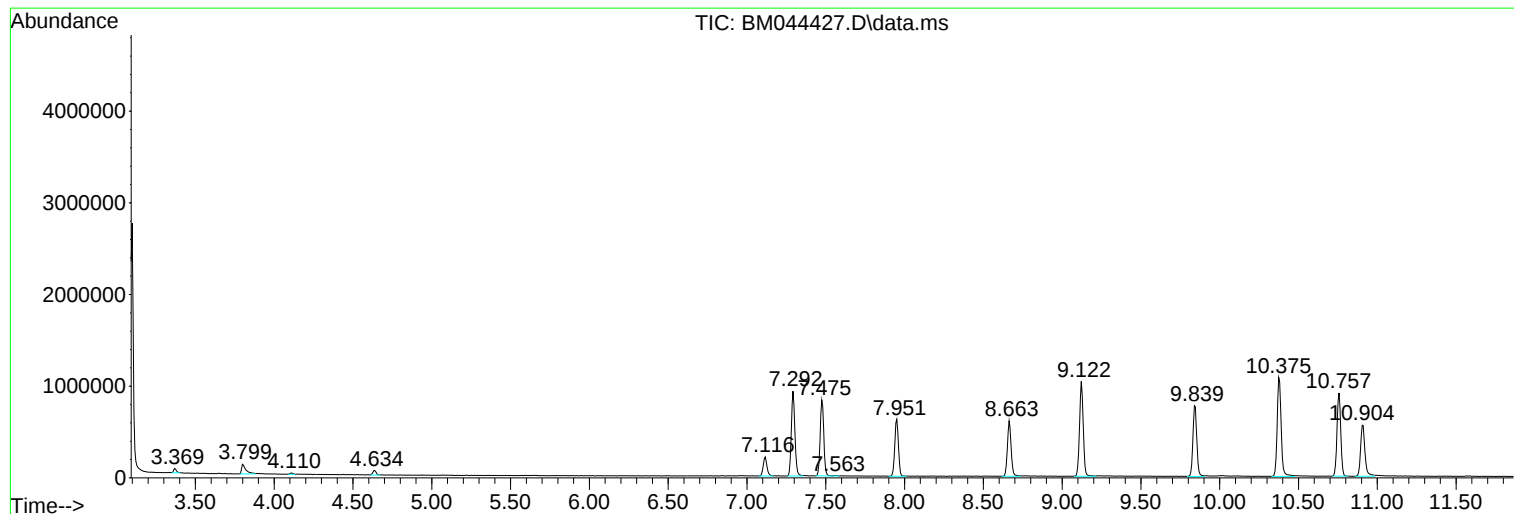

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044427.D
Acq On : 29 Feb 2024 06:19
Operator : MA/JU
Sample : P1535-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044427.D
Acq On : 29 Feb 2024 06:19
Operator : MA/JU
Sample : P1535-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc