

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044429.D
 Acq On : 29 Feb 2024 07:31
 Operator : MA/JU
 Sample : P1535-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AF8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.334	39	42	45	rBV3	24858	29105	0.45%	0.052%
2	3.369	45	48	57	rVB	55857	77992	1.21%	0.140%
3	3.799	117	121	136	rBV	184568	354600	5.48%	0.635%
4	4.110	171	174	181	rVB	16744	23679	0.37%	0.042%
5	4.634	258	263	271	rVB	100829	144707	2.24%	0.259%
6	7.116	679	685	697	rVB	234622	385811	5.96%	0.691%
7	7.293	709	715	731	rBV	1012445	1599500	24.73%	2.866%
8	7.475	739	746	756	rBV	925756	1469790	22.72%	2.633%
9	7.951	820	827	836	rVB	626464	997442	15.42%	1.787%
10	8.663	941	948	962	rBV	668142	1105794	17.09%	1.981%
11	9.122	1017	1026	1036	rBV	1097444	1835208	28.37%	3.288%
12	9.292	1051	1055	1061	rVB8	4345	6731	0.10%	0.012%
13	9.845	1142	1149	1158	rBV	866590	1432290	22.14%	2.566%
14	10.381	1232	1240	1253	rBV	1153283	2059787	31.84%	3.691%
15	10.757	1296	1304	1313	rBV	889087	1501861	23.22%	2.691%
16	10.910	1321	1330	1342	rBV	597995	1146915	17.73%	2.055%
17	12.351	1568	1575	1583	rVB2	23754	45165	0.70%	0.081%
18	13.498	1766	1770	1777	rBV2	18943	29018	0.45%	0.052%
19	14.016	1849	1858	1870	rBV	2367105	3333194	51.52%	5.972%
20	14.286	1896	1904	1916	rBV	2877824	4220787	65.25%	7.562%
21	14.592	1949	1956	1964	rBV	1286139	1908829	29.51%	3.420%
22	14.821	1988	1995	2012	rBV4	43283	183084	2.83%	0.328%
23	15.257	2066	2069	2073	rBV6	4087	7354	0.11%	0.013%
24	15.398	2088	2093	2096	rBV	14609	20835	0.32%	0.037%
25	15.586	2118	2125	2140	rBV	3660794	5272882	81.51%	9.447%
26	15.710	2140	2146	2158	rVV	1040078	1500035	23.19%	2.688%
27	15.821	2161	2165	2171	rVB3	16947	31899	0.49%	0.057%
28	16.151	2218	2221	2228	rBV8	4013	6518	0.10%	0.012%
29	16.368	2253	2258	2265	rVB6	11217	16194	0.25%	0.029%
30	17.021	2365	2369	2373	rVB6	5244	7898	0.12%	0.014%
31	17.339	2416	2423	2433	rBV	1543701	2171194	33.56%	3.890%
32	17.439	2433	2440	2454	rBV2	4013291	5837887	90.24%	10.460%
33	18.021	2535	2539	2544	rVB2	27976	36837	0.57%	0.066%
34	18.245	2572	2577	2583	rBV5	23290	42929	0.66%	0.077%
35	19.103	2721	2723	2727	rBV5	4848	7180	0.11%	0.013%
36	19.298	2751	2756	2762	rBV2	46812	68686	1.06%	0.123%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044429.D
Acq On : 29 Feb 2024 07:31
Operator : MA/JU
Sample : P1535-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.368	2763	2768	2773	rVV	42866	64772	1.00%	0.116%
38	19.445	2779	2781	2785	rVB4	8399	10785	0.17%	0.019%
39	19.533	2792	2796	2800	rBV4	16101	23318	0.36%	0.042%
40	19.686	2818	2822	2824	rBV3	25166	29179	0.45%	0.052%
41	19.733	2824	2830	2840	rVV	4737299	6469119	100.00%	11.591%
42	20.739	2998	3001	3004	rBV3	21823	28322	0.44%	0.051%
43	21.533	3131	3136	3143	rBV	1444854	2003803	30.97%	3.590%
44	23.803	3514	3522	3536	rBV2	3059803	6156814	95.17%	11.031%
45	23.956	3542	3548	3559	rVB	1009453	2107159	32.57%	3.775%




Sum of corrected areas: 55812888

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044429.D
Acq On : 29 Feb 2024 07:31
Operator : MA/JU
Sample : P1535-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

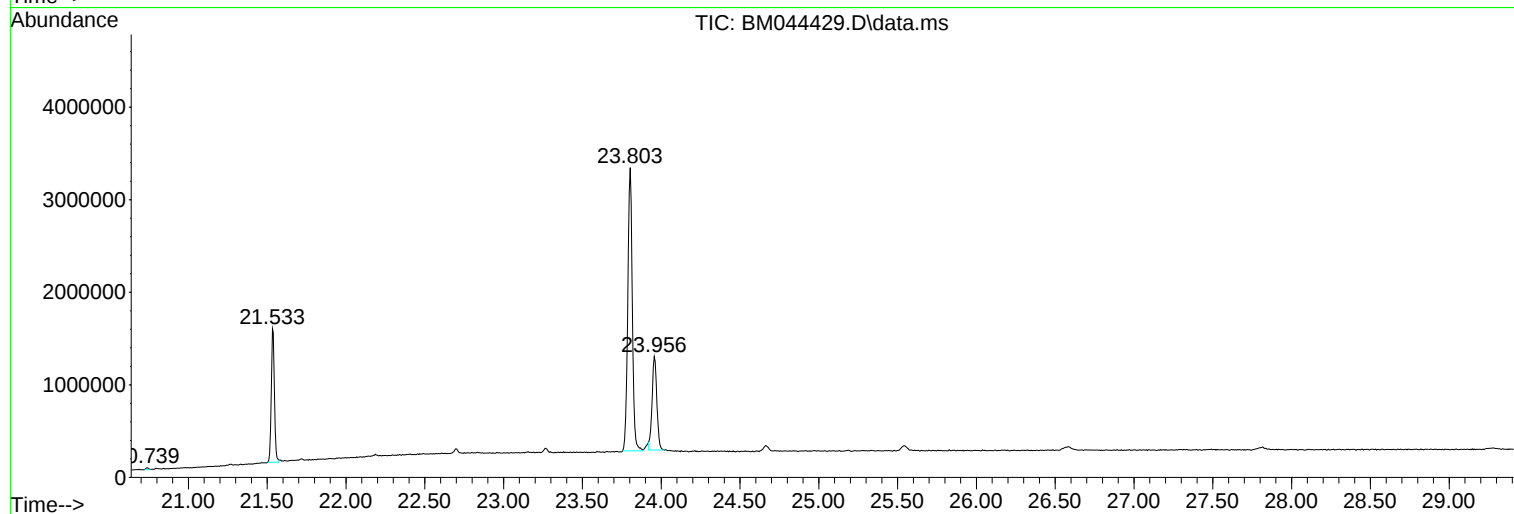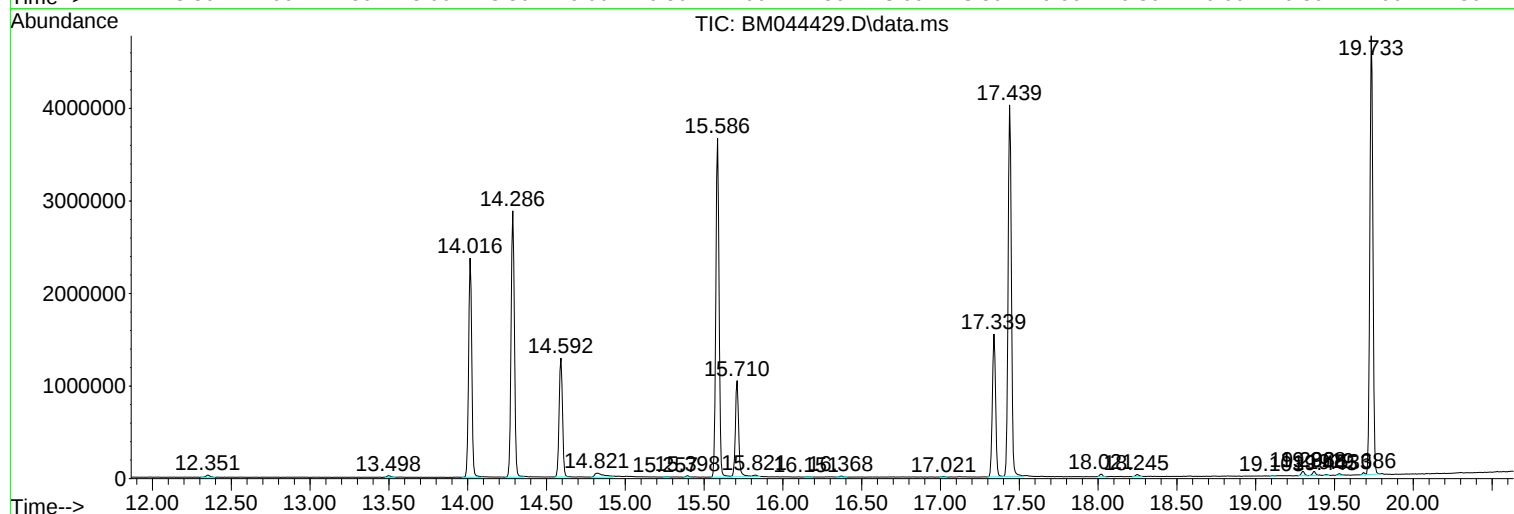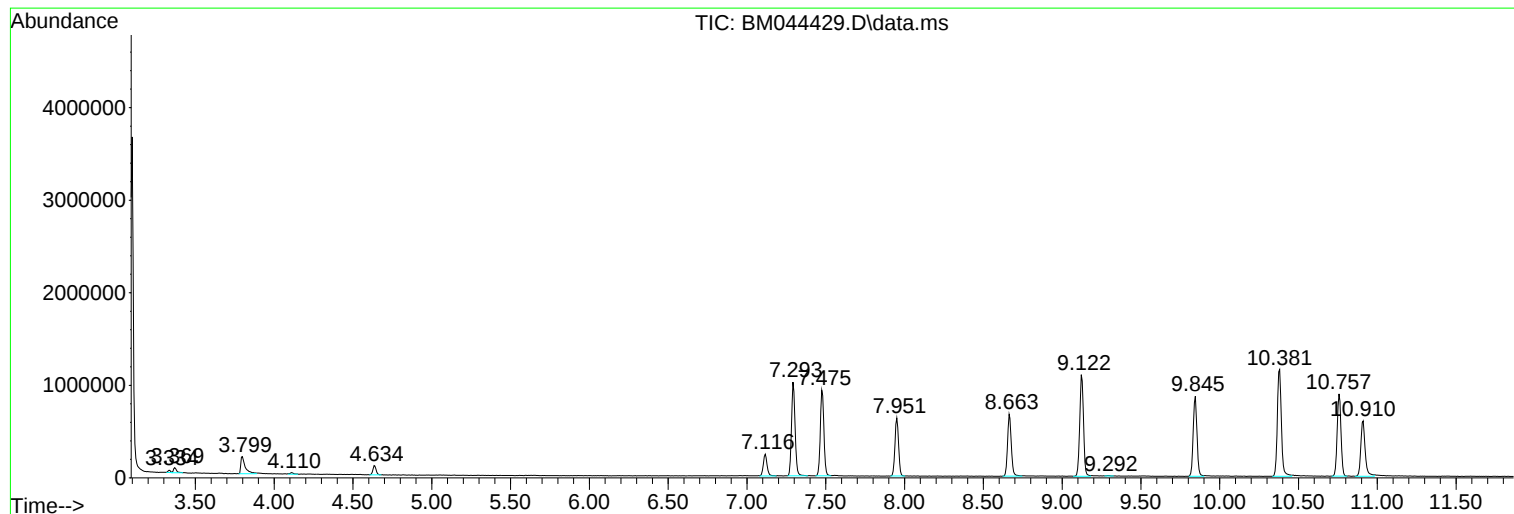

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044429.D
Acq On : 29 Feb 2024 07:31
Operator : MA/JU
Sample : P1535-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044429.D
Acq On : 29 Feb 2024 07:31
Operator : MA/JU
Sample : P1535-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AF8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
