

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044438.D
 Acq On : 29 Feb 2024 14:14
 Operator : MA/JU
 Sample : PB159263BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK263

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	45	48	57	rVB	73613	102727	2.39%	0.214%
2	3.787	116	119	143	rBV	763467	1306861	30.39%	2.718%
3	4.116	171	175	178	rVB3	9766	13815	0.32%	0.029%
4	7.122	679	686	698	rBV	867348	1382532	32.15%	2.876%
5	7.298	710	716	729	rVV	764159	1194432	27.78%	2.485%
6	7.481	740	747	760	rBV	889541	1407872	32.74%	2.929%
7	7.669	777	779	786	rVB6	2942	5808	0.14%	0.012%
8	7.957	821	828	835	rBV	759380	1196086	27.81%	2.488%
9	8.669	942	949	963	rBV	997453	1662798	38.67%	3.459%
10	9.128	1020	1027	1041	rBV	768344	1306259	30.38%	2.717%
11	9.851	1139	1150	1162	rBV	617267	1056050	24.56%	2.197%
12	10.386	1232	1241	1258	rBV	884922	1605937	37.35%	3.341%
13	10.763	1296	1305	1316	rBV	993312	1699064	39.51%	3.534%
14	10.916	1323	1331	1352	rBV	894630	1726623	40.15%	3.592%
15	11.469	1422	1425	1430	rVB7	2965	4790	0.11%	0.010%
16	11.998	1513	1515	1521	rVB5	2919	4444	0.10%	0.009%
17	12.357	1571	1576	1584	rBV2	16542	31898	0.74%	0.066%
18	13.504	1763	1771	1778	rBV4	14031	25800	0.60%	0.054%
19	14.021	1852	1859	1875	rBV	1633854	2297512	53.43%	4.779%
20	14.292	1897	1905	1919	rBV	1959037	2858221	66.47%	5.945%
21	14.598	1949	1957	1969	rBV	1438761	2129653	49.52%	4.430%
22	14.810	1987	1993	2021	rBV	332669	975087	22.68%	2.028%
23	15.592	2118	2126	2136	rBV	2366233	3490620	81.17%	7.261%
24	15.715	2141	2147	2162	rVV	609987	915636	21.29%	1.905%
25	15.833	2162	2167	2170	rVB5	12442	18227	0.42%	0.038%
26	16.374	2256	2259	2265	rVB5	8495	11363	0.26%	0.024%
27	17.127	2383	2387	2392	rBV7	5317	9953	0.23%	0.021%
28	17.345	2417	2424	2434	rBV	1733286	2463923	57.30%	5.125%
29	17.445	2434	2441	2456	rVV	2656681	3821664	88.87%	7.950%
30	17.727	2486	2489	2493	rBV6	3200	4798	0.11%	0.010%
31	18.256	2577	2579	2585	rVB6	3045	5292	0.12%	0.011%
32	18.398	2599	2603	2607	rBV6	2109	4473	0.10%	0.009%
33	19.303	2753	2757	2764	rVB4	30092	43934	1.02%	0.091%
34	19.374	2764	2769	2774	rBV	28957	41586	0.97%	0.087%
35	19.739	2825	2831	2844	rBV	3239562	4300187	100.00%	8.945%
36	21.539	3132	3137	3150	rBV	1799213	2395950	55.72%	4.984%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044438.D
Acq On : 29 Feb 2024 14:14
Operator : MA/JU
Sample : PB159263BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK263

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	23.809	3515	3523	3535	rBV	1892969	4036810	93.88%	8.397%
38	23.962	3542	3549	3562	rVB	1161013	2515085	58.49%	5.232%




Sum of corrected areas: 48073770

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044438.D
Acq On : 29 Feb 2024 14:14
Operator : MA/JU
Sample : PB159263BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK263

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

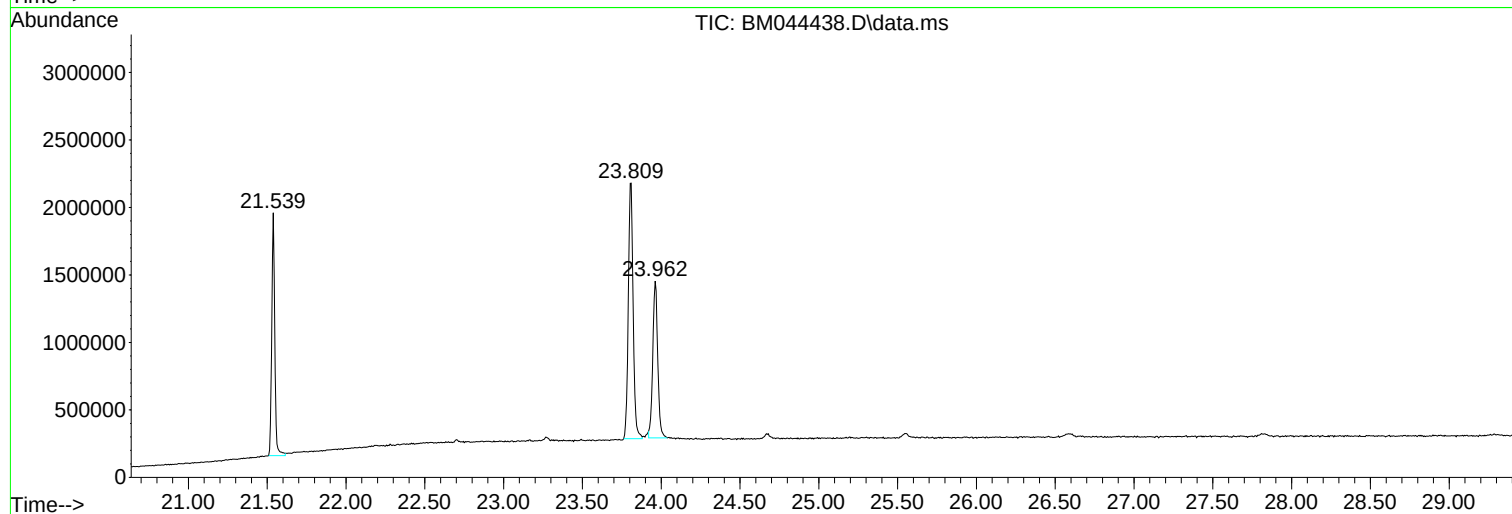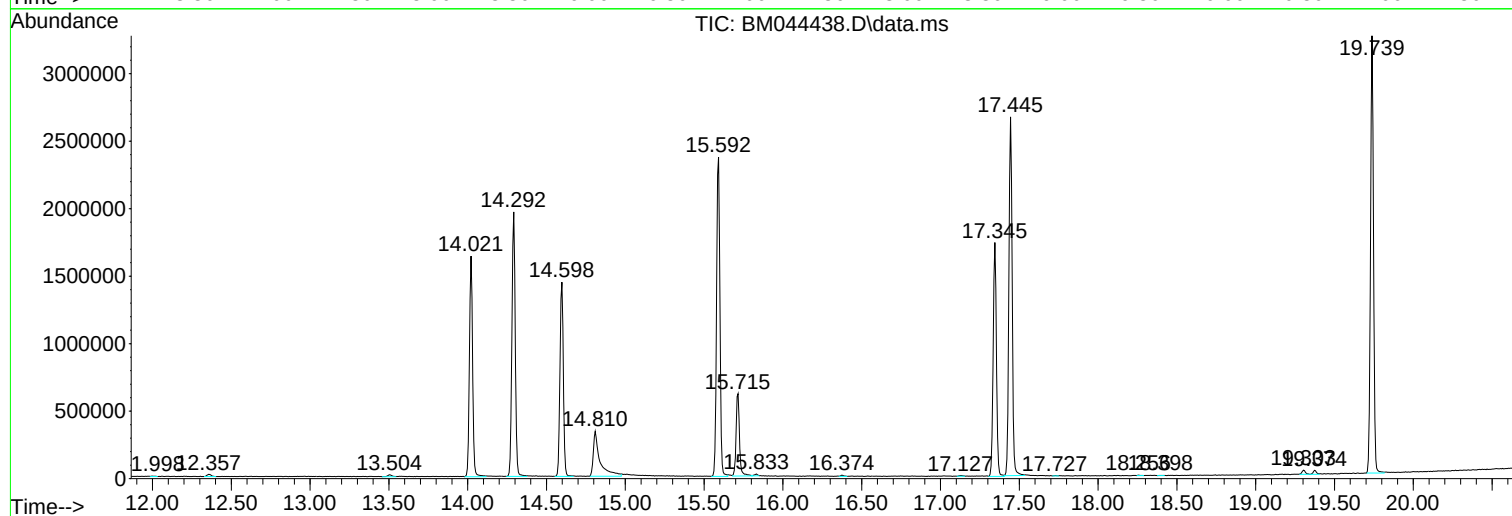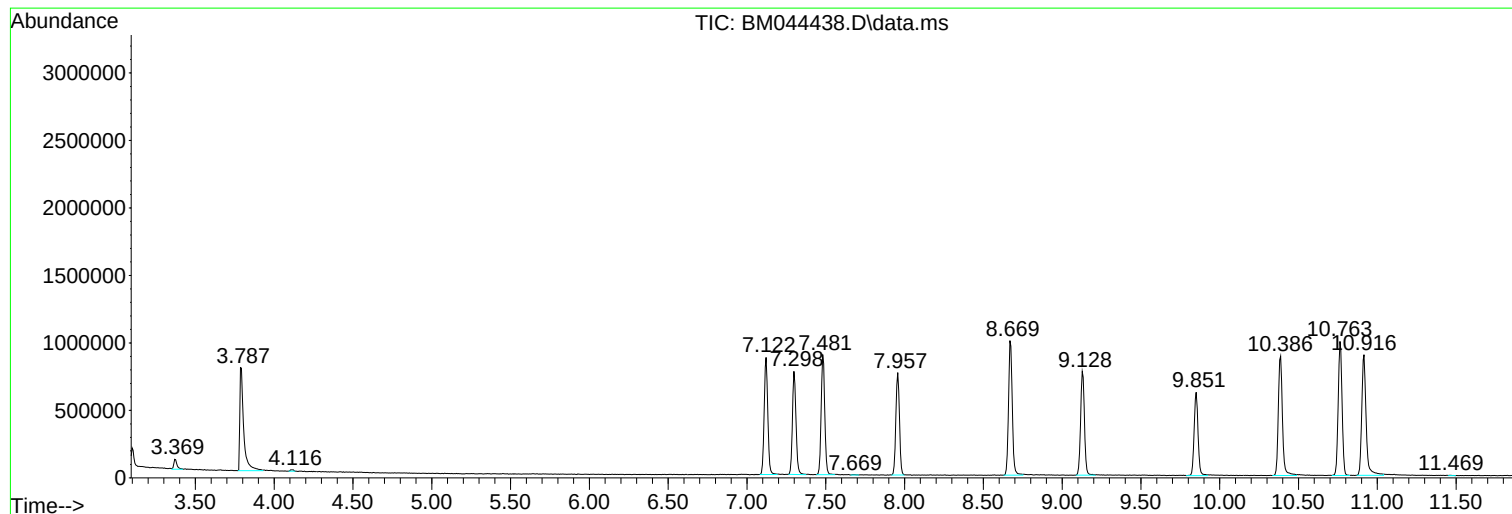

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044438.D
Acq On : 29 Feb 2024 14:14
Operator : MA/JU
Sample : PB159263BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK263

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044438.D
Acq On : 29 Feb 2024 14:14
Operator : MA/JU
Sample : PB159263BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK263

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------