

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044447.D
 Acq On : 29 Feb 2024 19:44
 Operator : MA/JU
 Sample : P1501-17
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E10A4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	55	rVB	51090	63783	1.11%	0.121%
2	3.799	118	121	138	rBV	299392	527481	9.15%	1.003%
3	4.116	171	175	179	rBV	28571	37616	0.65%	0.072%
4	4.646	259	265	271	rBV	215423	299961	5.20%	0.570%
5	5.604	424	428	433	rBV	25976	41078	0.71%	0.078%
6	7.128	681	687	696	rVB	187838	311805	5.41%	0.593%
7	7.304	711	717	730	rVB	826310	1302713	22.60%	2.477%
8	7.487	741	748	760	rBV	738117	1172704	20.34%	2.230%
9	7.581	760	764	767	rVB6	4567	6809	0.12%	0.013%
10	7.963	821	829	839	rBV	767292	1192446	20.69%	2.268%
11	8.675	942	950	958	rBV	531720	900566	15.62%	1.713%
12	9.134	1021	1028	1043	rBV	875129	1512057	26.23%	2.875%
13	9.534	1090	1096	1099	rBV4	6384	10796	0.19%	0.021%
14	9.857	1143	1151	1161	rBV	692267	1169846	20.29%	2.225%
15	10.392	1233	1242	1254	rBV	955127	1670257	28.97%	3.176%
16	10.769	1298	1306	1316	rVB	1022678	1745786	30.28%	3.320%
17	10.922	1324	1332	1352	rBV	901872	1700152	29.49%	3.233%
18	11.604	1444	1448	1454	rBV7	5319	10095	0.18%	0.019%
19	12.363	1572	1577	1581	rBV2	19977	30523	0.53%	0.058%
20	13.433	1755	1759	1765	rBV7	4808	9434	0.16%	0.018%
21	13.510	1767	1772	1778	rVB	35236	59182	1.03%	0.113%
22	14.027	1852	1860	1872	rBV	2006166	2817086	48.87%	5.357%
23	14.298	1898	1906	1916	rBV	2415231	3495615	60.64%	6.647%
24	14.604	1951	1958	1965	rBV	1525070	2220557	38.52%	4.223%
25	14.657	1965	1967	1972	rVB6	4928	7094	0.12%	0.013%
26	14.827	1990	1996	2008	rBV3	45232	151794	2.63%	0.289%
27	15.016	2024	2028	2037	rVB3	4808	13111	0.23%	0.025%
28	15.598	2119	2127	2141	rBV	3024260	4450159	77.20%	8.463%
29	15.721	2141	2148	2162	rVV	910371	1368458	23.74%	2.602%
30	15.833	2162	2167	2177	rVB5	16419	38217	0.66%	0.073%
31	16.380	2256	2260	2265	rBV5	11788	17107	0.30%	0.033%
32	17.027	2367	2370	2373	rVB5	4725	6287	0.11%	0.012%
33	17.139	2383	2389	2391	rBV6	4188	6561	0.11%	0.012%
34	17.351	2418	2425	2435	rBV	1746099	2489949	43.19%	4.735%
35	17.451	2435	2442	2460	rVV	3643612	5191141	90.05%	9.872%
36	18.039	2537	2542	2548	rBV9	5383	11472	0.20%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044447.D
Acq On : 29 Feb 2024 19:44
Operator : MA/JU
Sample : P1501-17
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	18.257	2574	2579	2586	rBV2	63206	92504	1.60%	0.176%
38	18.339	2591	2593	2597	rVB5	5048	5919	0.10%	0.011%
39	18.698	2650	2654	2657	rVB5	4763	6734	0.12%	0.013%
40	18.939	2691	2695	2699	rBV7	3725	8695	0.15%	0.017%
41	19.309	2754	2758	2765	rBV2	39388	58247	1.01%	0.111%
42	19.380	2766	2770	2774	rBV	39244	53781	0.93%	0.102%
43	19.451	2780	2782	2787	rVB6	8370	10807	0.19%	0.021%
44	19.539	2794	2797	2804	rBV4	35657	46403	0.80%	0.088%
45	19.692	2820	2823	2826	rBV5	18009	21066	0.37%	0.040%
46	19.745	2826	2832	2840	rVV	4247685	5764728	100.00%	10.962%
47	21.539	3132	3137	3150	rBV	1719146	2436580	42.27%	4.633%
48	23.815	3516	3524	3538	rBV	2736372	5501877	95.44%	10.463%
49	23.974	3544	3551	3561	rVB	1206534	2519559	43.71%	4.791%




Sum of corrected areas: 52586598

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044447.D
Acq On : 29 Feb 2024 19:44
Operator : MA/JU
Sample : P1501-17
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

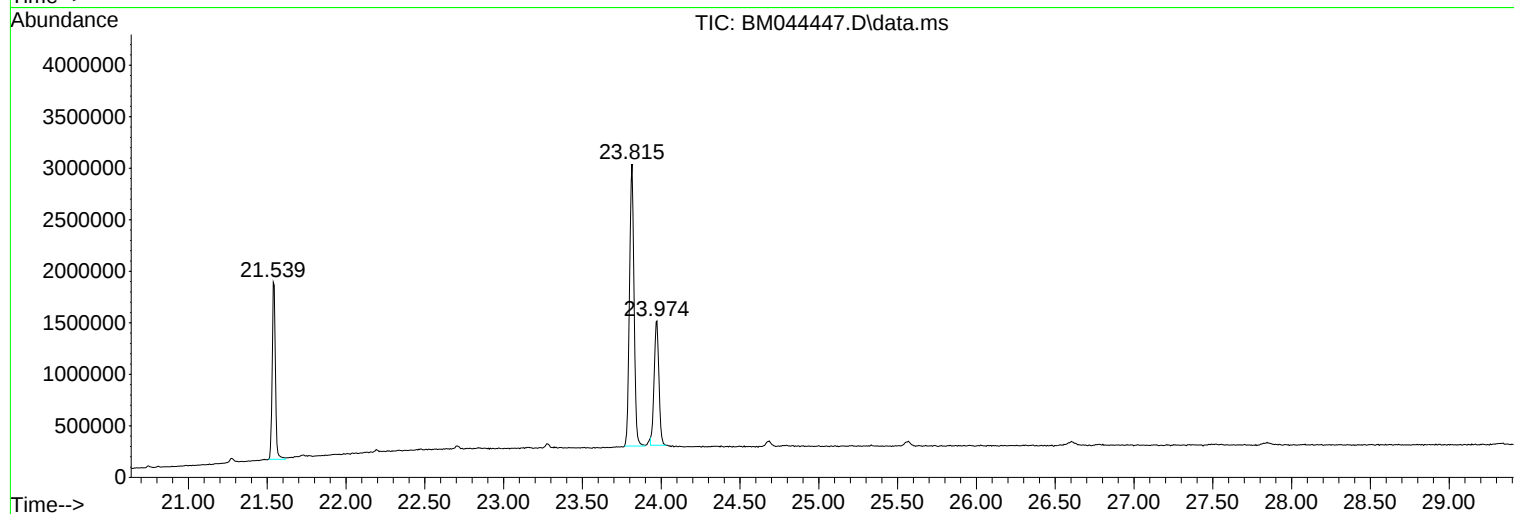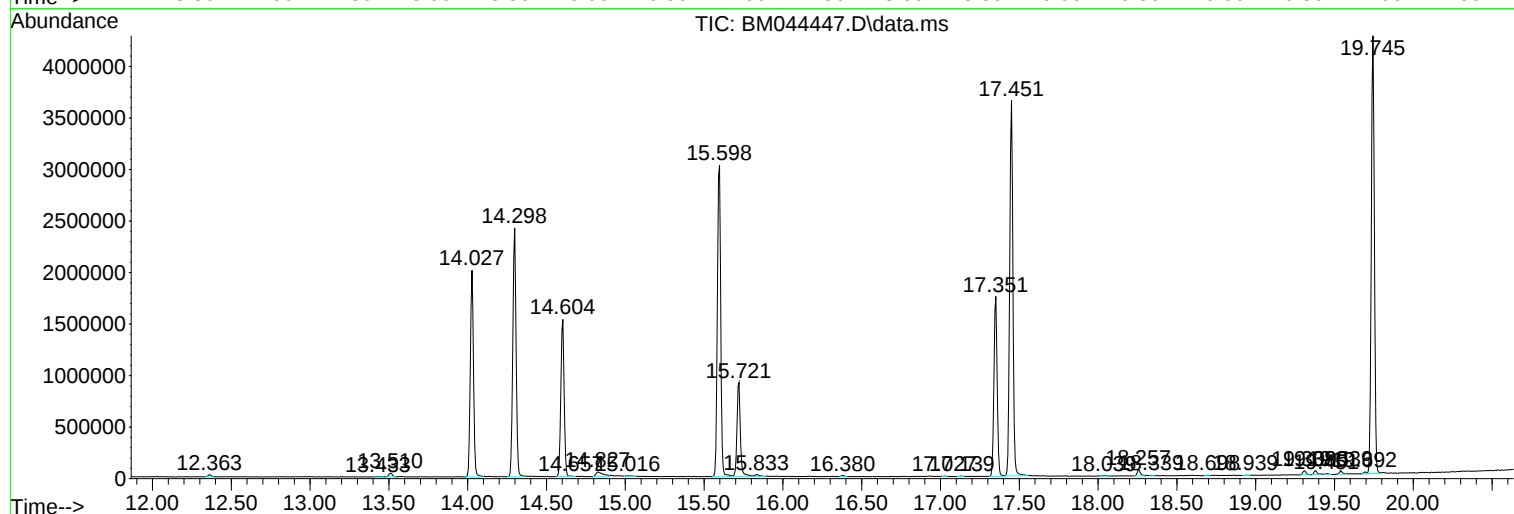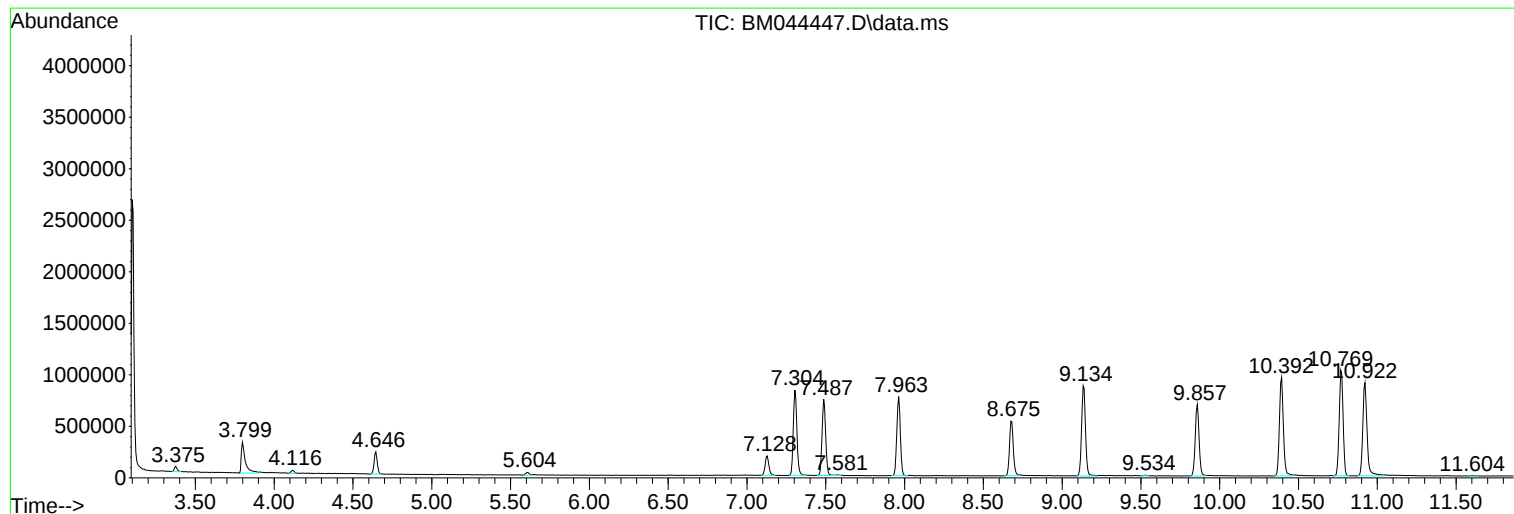

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044447.D
Acq On : 29 Feb 2024 19:44
Operator : MA/JU
Sample : P1501-17
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044447.D
Acq On : 29 Feb 2024 19:44
Operator : MA/JU
Sample : P1501-17
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------