

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044449.D
 Acq On : 29 Feb 2024 20:57
 Operator : MA/JU
 Sample : P1501-19
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E10B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	45	49	58	rVB	45810	63240	1.10%	0.124%
2	3.799	118	121	134	rBV	329159	556630	9.70%	1.093%
3	4.116	172	175	181	rVB	25688	34461	0.60%	0.068%
4	5.610	424	429	434	rVB	24748	36825	0.64%	0.072%
5	7.128	681	687	697	rVB	193484	315176	5.49%	0.619%
6	7.310	711	718	730	rBV	809615	1322872	23.06%	2.597%
7	7.492	741	749	757	rBV	740412	1189890	20.74%	2.336%
8	7.963	822	829	838	rVV	682968	1090041	19.00%	2.140%
9	8.681	940	951	963	rBV	550842	921364	16.06%	1.808%
10	9.139	1021	1029	1038	rBV	895759	1498116	26.12%	2.941%
11	9.857	1143	1151	1160	rBV	686308	1166934	20.34%	2.290%
12	10.392	1235	1242	1264	rBV	967115	1713241	29.87%	3.363%
13	10.775	1299	1307	1322	rVB	944970	1589405	27.71%	3.120%
14	10.922	1324	1332	1353	rBV	983125	1846196	32.18%	3.624%
15	12.369	1572	1578	1582	rBV	19299	31225	0.54%	0.061%
16	13.457	1760	1763	1767	rBV3	5993	8377	0.15%	0.016%
17	13.516	1767	1773	1781	rVB2	21924	36467	0.64%	0.072%
18	14.027	1854	1860	1872	rBV	1926022	2812627	49.03%	5.521%
19	14.298	1898	1906	1916	rBV	2343780	3453504	60.20%	6.779%
20	14.604	1951	1958	1967	rBV	1399705	2036349	35.50%	3.997%
21	14.833	1992	1997	2010	rBV5	36225	137190	2.39%	0.269%
22	15.015	2025	2028	2033	rVB6	4465	5934	0.10%	0.012%
23	15.598	2120	2127	2134	rBV	3109444	4408331	76.85%	8.653%
24	15.721	2142	2148	2164	rBV	870412	1240976	21.63%	2.436%
25	15.833	2164	2167	2176	rVB4	17433	28970	0.51%	0.057%
26	16.162	2220	2223	2227	rVB6	3924	6093	0.11%	0.012%
27	16.386	2257	2261	2266	rVB7	10423	15892	0.28%	0.031%
28	17.027	2366	2370	2377	rVB9	5985	10172	0.18%	0.020%
29	17.139	2382	2389	2392	rBV5	4324	7506	0.13%	0.015%
30	17.351	2418	2425	2435	rBV	1629333	2306287	40.20%	4.527%
31	17.451	2435	2442	2458	rVV	3626008	5137000	89.55%	10.083%
32	17.556	2458	2460	2466	rVB6	12965	20043	0.35%	0.039%
33	18.262	2575	2580	2584	rBV5	13680	23078	0.40%	0.045%
34	18.750	2660	2663	2667	rBV6	4398	8291	0.14%	0.016%
35	19.309	2754	2758	2764	rVB2	39296	56638	0.99%	0.111%
36	19.380	2764	2770	2775	rBV	36176	59624	1.04%	0.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044449.D
Acq On : 29 Feb 2024 20:57
Operator : MA/JU
Sample : P1501-19
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10B8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.545	2795	2798	2802	rBV6	7884	8127	0.14%	0.016%
38	19.697	2821	2824	2826	rBV3	13042	14477	0.25%	0.028%
39	19.745	2826	2832	2842	rVV	4408198	5736542	100.00%	11.260%
40	21.544	3132	3138	3148	rBV	1593372	2219538	38.69%	4.357%
41	23.815	3517	3524	3539	rBV2	2600030	5385040	93.87%	10.570%
42	23.974	3544	3551	3568	rVB	1080953	2388638	41.64%	4.688%




Sum of corrected areas: 50947327

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044449.D
Acq On : 29 Feb 2024 20:57
Operator : MA/JU
Sample : P1501-19
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10B8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

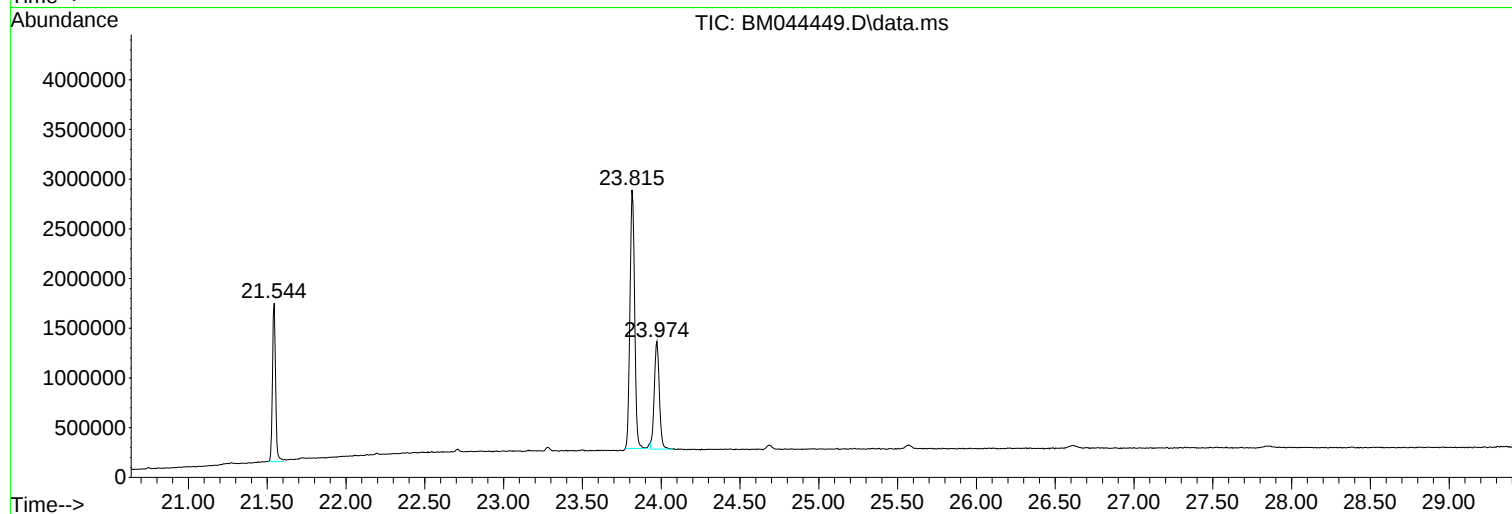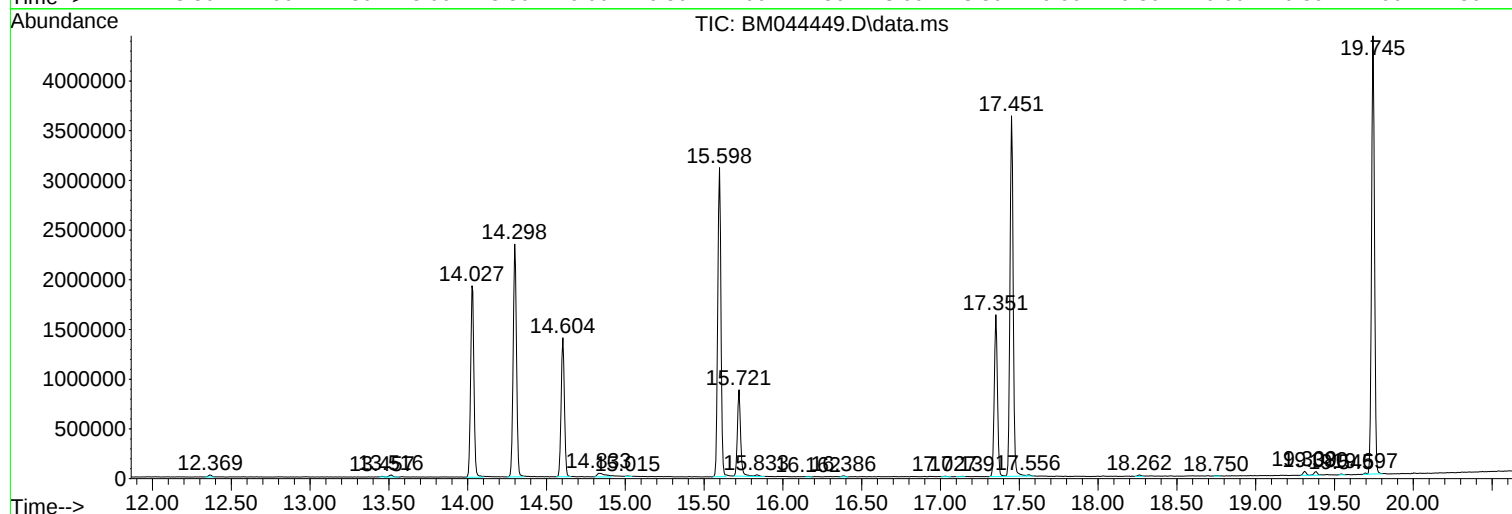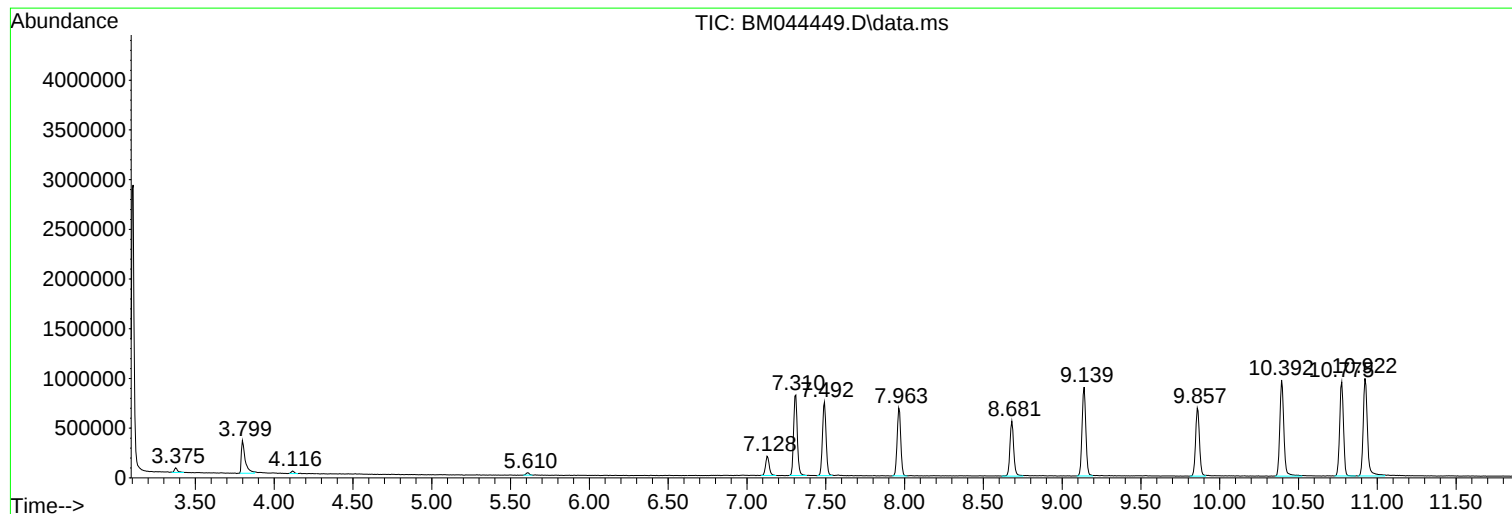

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044449.D
Acq On : 29 Feb 2024 20:57
Operator : MA/JU
Sample : P1501-19
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10B8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044449.D
Acq On : 29 Feb 2024 20:57
Operator : MA/JU
Sample : P1501-19
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10B8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------