

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044450.D
 Acq On : 29 Feb 2024 21:34
 Operator : MA/JU
 Sample : P1501-20
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E10B9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	46	49	57	rVB	55384	76296	1.35%	0.148%
2	3.799	118	121	148	rBV	357175	660399	11.72%	1.279%
3	4.116	172	175	181	rVB	16574	24213	0.43%	0.047%
4	5.610	424	429	434	rBV	31411	45937	0.82%	0.089%
5	7.134	681	688	697	rBV	212887	354560	6.29%	0.687%
6	7.310	711	718	735	rBV	970004	1546533	27.44%	2.994%
7	7.492	742	749	759	rBV	874580	1369026	24.29%	2.651%
8	7.581	761	764	768	rVB6	5429	7511	0.13%	0.015%
9	7.969	823	830	840	rVB	695607	1119083	19.86%	2.167%
10	8.681	943	951	963	rBV	598936	995102	17.66%	1.927%
11	9.139	1022	1029	1045	rVB	1015375	1671123	29.65%	3.236%
12	9.528	1094	1095	1099	rVB4	5185	6203	0.11%	0.012%
13	9.863	1143	1152	1163	rBV	752841	1293011	22.95%	2.504%
14	10.398	1235	1243	1258	rBV	1017768	1825114	32.39%	3.534%
15	10.775	1300	1307	1315	rBV	925025	1534586	27.23%	2.971%
16	10.928	1325	1333	1357	rBV	1014815	1911807	33.93%	3.702%
17	12.369	1572	1578	1585	rVB2	20066	35200	0.62%	0.068%
18	12.880	1662	1665	1672	rVB5	10732	16263	0.29%	0.031%
19	13.516	1768	1773	1780	rVB3	19891	31388	0.56%	0.061%
20	14.033	1853	1861	1877	rBV	2004148	2784172	49.41%	5.391%
21	14.304	1899	1907	1921	rBV	2363171	3600086	63.89%	6.971%
22	14.604	1951	1958	1965	rBV	1248415	1879462	33.35%	3.639%
23	14.839	1989	1998	2007	rBV4	34241	112999	2.01%	0.219%
24	15.598	2120	2127	2142	rBV	2949721	4345307	77.11%	8.413%
25	15.721	2142	2148	2163	rVV	840442	1246631	22.12%	2.414%
26	15.839	2164	2168	2174	rVB3	15901	25601	0.45%	0.050%
27	16.162	2221	2223	2230	rVB8	4281	8028	0.14%	0.016%
28	16.386	2255	2261	2265	rBV5	10805	15215	0.27%	0.029%
29	16.762	2321	2325	2332	rBV9	5926	9289	0.16%	0.018%
30	17.039	2365	2372	2374	rBV7	5396	9521	0.17%	0.018%
31	17.357	2419	2426	2436	rBV	1442151	2132267	37.84%	4.129%
32	17.457	2436	2443	2455	rVV	3373650	4982958	88.43%	9.648%
33	17.557	2458	2460	2467	rVB7	14273	25712	0.46%	0.050%
34	18.139	2555	2559	2562	rBV6	7359	8727	0.15%	0.017%
35	18.262	2575	2580	2589	rBV2	65341	98816	1.75%	0.191%
36	18.845	2676	2679	2682	rBV5	5460	7766	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044450.D
Acq On : 29 Feb 2024 21:34
Operator : MA/JU
Sample : P1501-20
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10B9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.315	2754	2759	2765	rBV2	37636	60711	1.08%	0.118%
38	19.386	2767	2771	2775	rVV	33031	45207	0.80%	0.088%
39	19.456	2781	2783	2787	rVB5	6135	6290	0.11%	0.012%
40	19.545	2794	2798	2804	rBV3	45199	60828	1.08%	0.118%
41	19.698	2821	2824	2826	rBV3	13200	13121	0.23%	0.025%
42	19.750	2826	2833	2841	rVV	4143327	5635229	100.00%	10.911%
43	21.544	3133	3138	3148	rBV	1474927	2089764	37.08%	4.046%
44	22.850	3357	3360	3368	rVB	107196	153938	2.73%	0.298%
45	23.821	3517	3525	3540	rBV2	2657090	5473268	97.13%	10.597%
46	23.980	3545	3552	3564	rVB	1068578	2293139	40.69%	4.440%




Sum of corrected areas: 51647407

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044450.D
Acq On : 29 Feb 2024 21:34
Operator : MA/JU
Sample : P1501-20
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10B9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

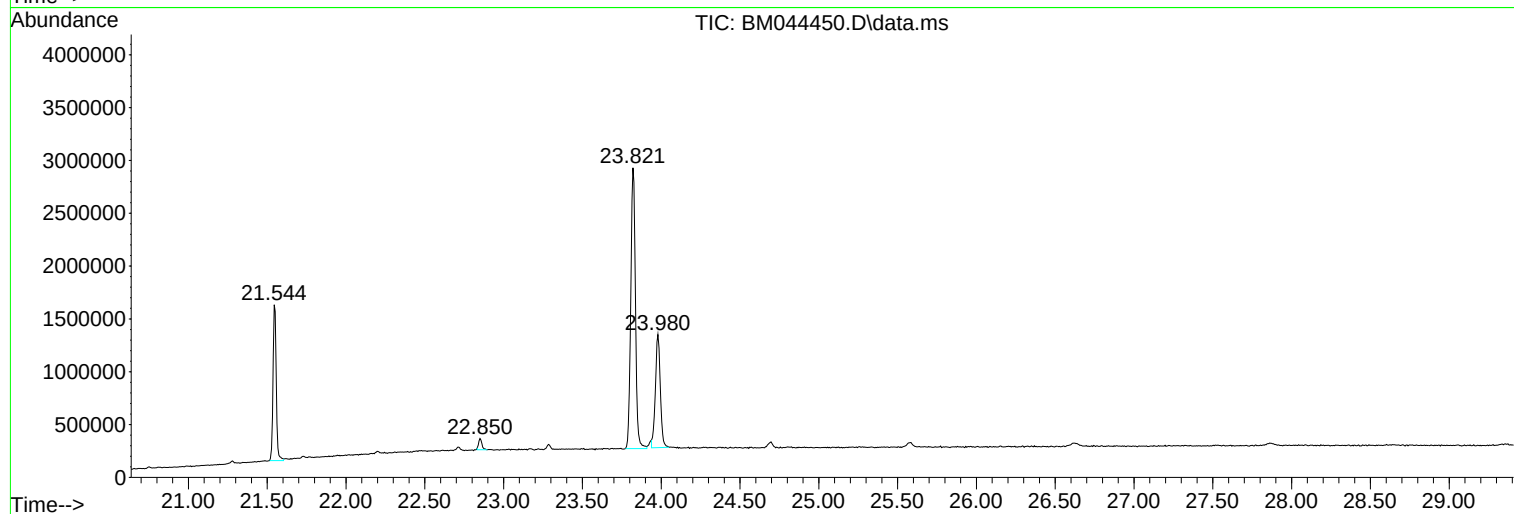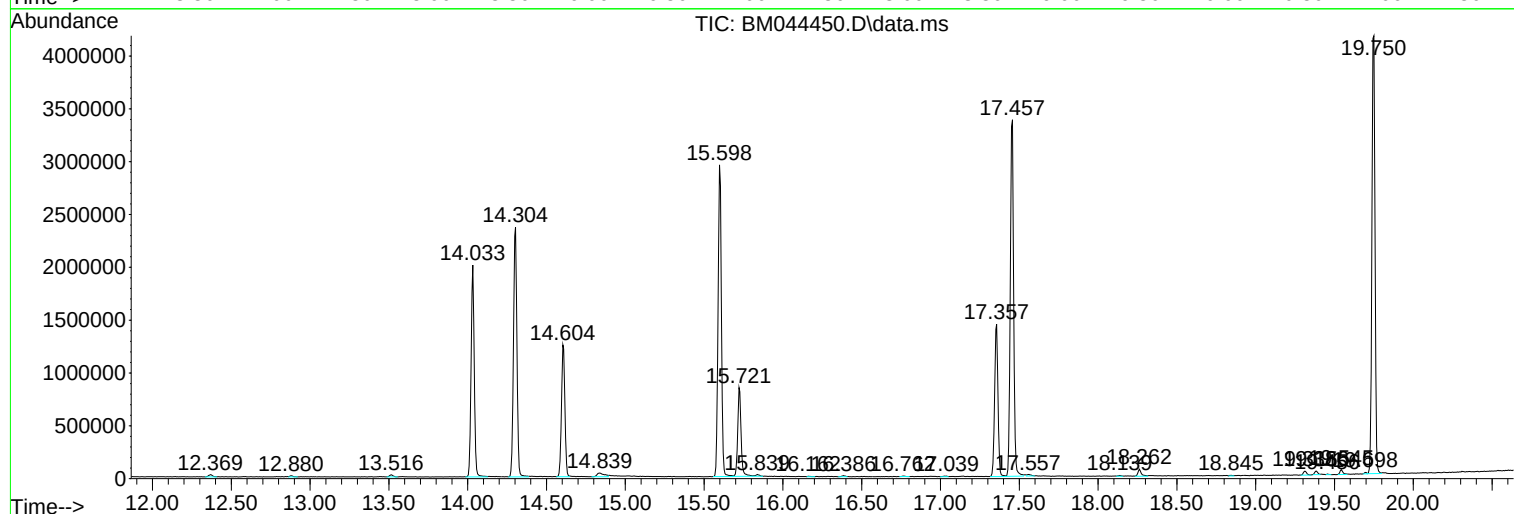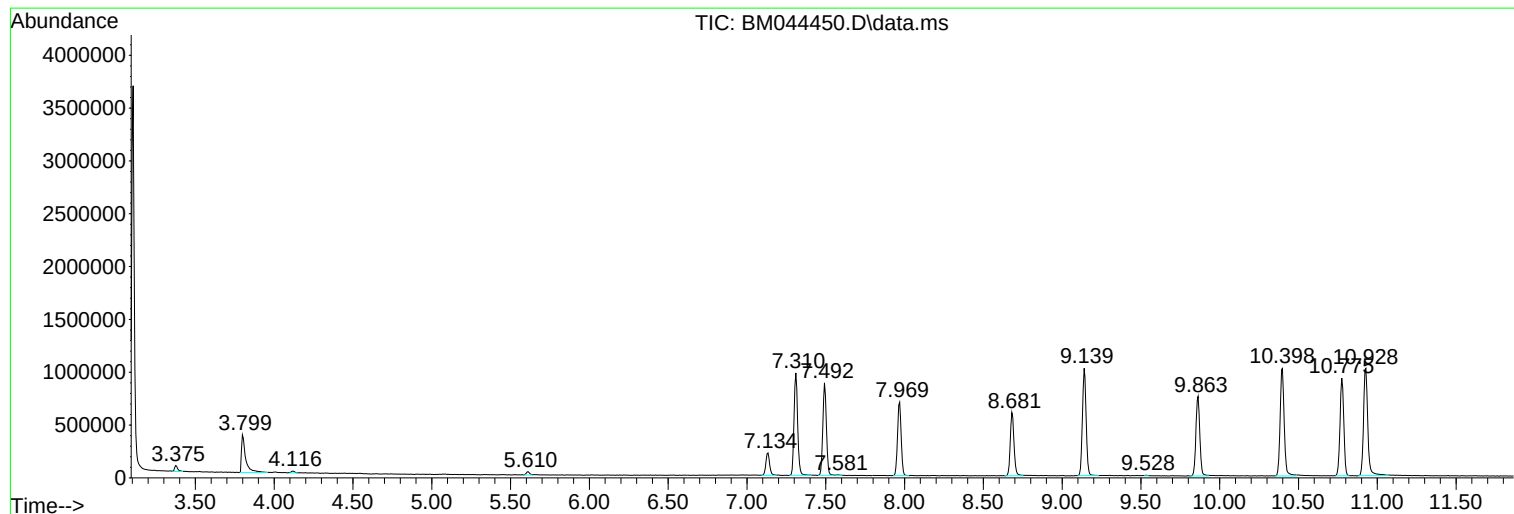

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044450.D
Acq On : 29 Feb 2024 21:34
Operator : MA/JU
Sample : P1501-20
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10B9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044450.D
Acq On : 29 Feb 2024 21:34
Operator : MA/JU
Sample : P1501-20
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10B9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------