

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044451.D
 Acq On : 29 Feb 2024 22:10
 Operator : MA/JU
 Sample : P1501-21
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E10C0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	46	49	55	rVB	50035	62739	1.04%	0.114%
2	3.805	119	122	137	rBV	241625	432566	7.18%	0.783%
3	4.116	172	175	184	rVB	21899	30420	0.51%	0.055%
4	4.646	260	265	273	rVB	213716	301524	5.01%	0.545%
5	5.228	360	364	368	rVB7	4904	6955	0.12%	0.013%
6	5.610	425	429	435	rBV	28599	42568	0.71%	0.077%
7	7.134	680	688	697	rBV	202530	341557	5.67%	0.618%
8	7.310	712	718	731	rBV	871883	1388033	23.05%	2.511%
9	7.493	743	749	758	rBV	802022	1261035	20.94%	2.281%
10	7.969	823	830	838	rBV	828995	1287627	21.38%	2.329%
11	8.045	839	843	846	rVB6	4652	6129	0.10%	0.011%
12	8.681	945	951	967	rBV	566814	964703	16.02%	1.745%
13	9.139	1020	1029	1041	rBV	933491	1587992	26.37%	2.873%
14	9.534	1095	1096	1101	rVB5	7636	8200	0.14%	0.015%
15	9.863	1144	1152	1167	rBV	734606	1243446	20.65%	2.250%
16	10.398	1235	1243	1258	rBV	1025250	1793975	29.79%	3.246%
17	10.492	1258	1259	1264	rVB5	5500	6178	0.10%	0.011%
18	10.775	1300	1307	1316	rBV	1107710	1876151	31.16%	3.394%
19	10.928	1323	1333	1356	rBV	887900	1727406	28.68%	3.125%
20	12.369	1572	1578	1585	rVB	20454	34561	0.57%	0.063%
21	13.516	1768	1773	1780	rVB	26602	43581	0.72%	0.079%
22	14.033	1854	1861	1869	rBV	2065214	2846319	47.27%	5.149%
23	14.304	1900	1907	1920	rBV	2404009	3610904	59.96%	6.533%
24	14.610	1949	1959	1967	rBV	1597323	2393836	39.75%	4.331%
25	14.739	1978	1981	1985	rVB6	4484	6348	0.11%	0.011%
26	14.833	1990	1997	2009	rBV2	51679	170878	2.84%	0.309%
27	15.598	2118	2127	2141	rBV	3121394	4619319	76.71%	8.357%
28	15.721	2142	2148	2165	rVV	940611	1402612	23.29%	2.537%
29	15.839	2165	2168	2173	rVB6	14184	20548	0.34%	0.037%
30	16.380	2256	2260	2267	rVB8	10987	21098	0.35%	0.038%
31	16.498	2277	2280	2284	rVB5	4787	6886	0.11%	0.012%
32	17.039	2367	2372	2374	rVB6	6162	7485	0.12%	0.014%
33	17.357	2419	2426	2436	rBV	1902515	2720138	45.17%	4.921%
34	17.457	2436	2443	2457	rVV	3672858	5361556	89.03%	9.700%
35	18.039	2537	2542	2545	rBV7	7415	11618	0.19%	0.021%
36	18.262	2576	2580	2585	rBV	52508	73965	1.23%	0.134%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044451.D
Acq On : 29 Feb 2024 22:10
Operator : MA/JU
Sample : P1501-21
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10C0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	18.698	2649	2654	2657	rBV7	3962	7549	0.13%	0.014%
38	18.751	2660	2663	2667	rBV5	5134	7431	0.12%	0.013%
39	19.315	2754	2759	2763	rBV	43830	59728	0.99%	0.108%
40	19.386	2766	2771	2776	rBV	36064	59867	0.99%	0.108%
41	19.545	2795	2798	2805	rBV7	27598	35078	0.58%	0.063%
42	19.704	2821	2825	2826	rBV3	17228	19413	0.32%	0.035%
43	19.751	2826	2833	2841	rVV	4583542	6021987	100.00%	10.894%
44	21.545	3133	3138	3149	rBV	1976222	2666361	44.28%	4.824%
45	23.821	3517	3525	3538	rBV2	2824558	5837197	96.93%	10.560%
46	23.980	3545	3552	3564	rVB	1329027	2840269	47.16%	5.138%




Sum of corrected areas: 55275736

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044451.D
Acq On : 29 Feb 2024 22:10
Operator : MA/JU
Sample : P1501-21
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

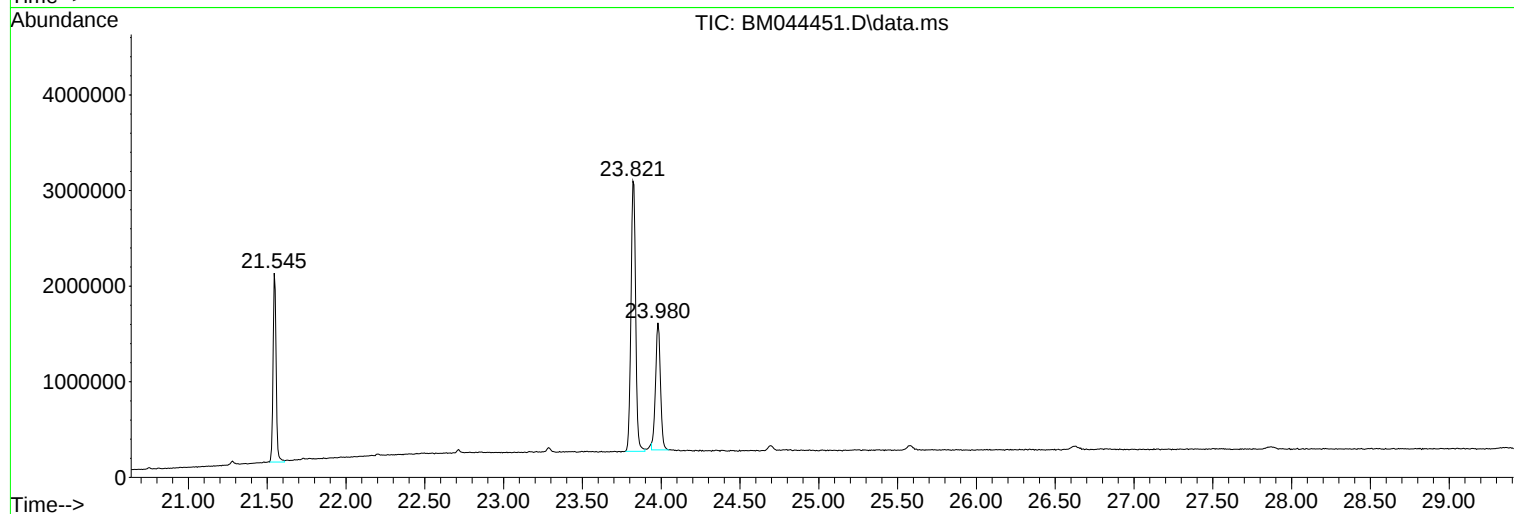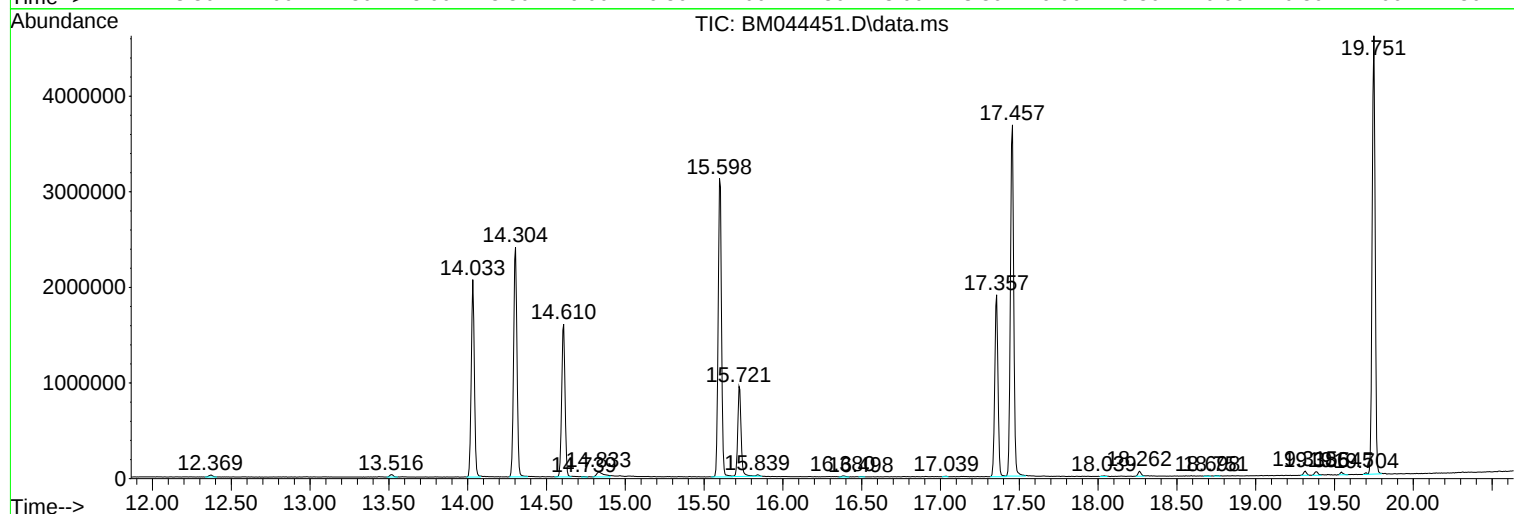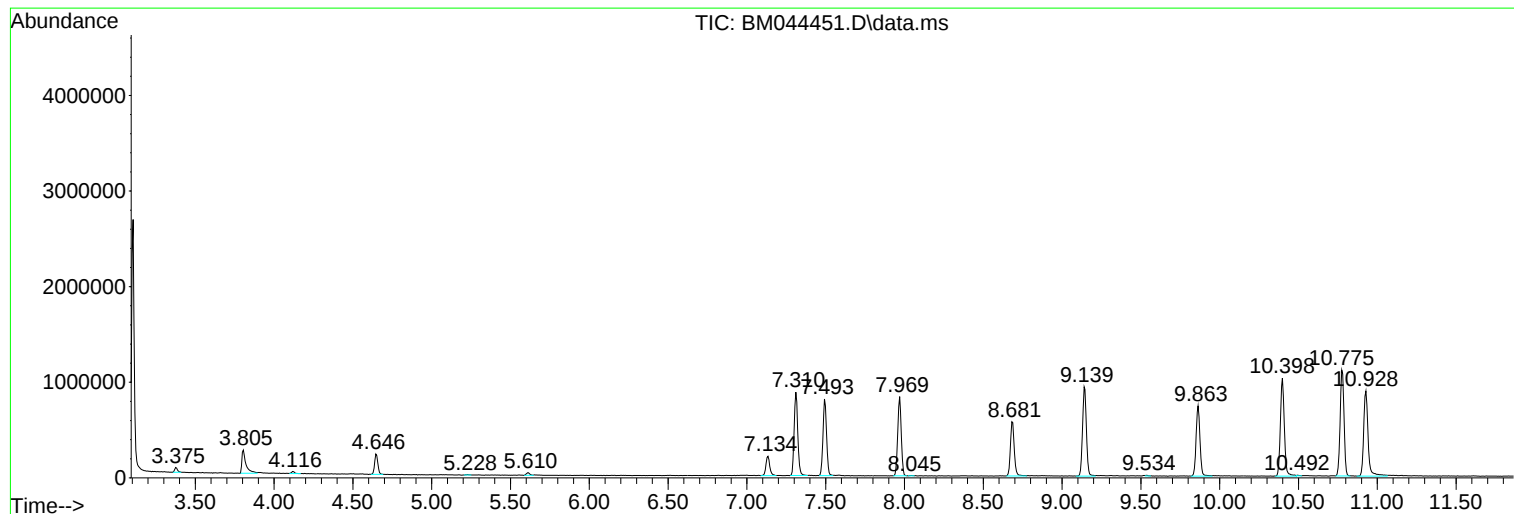

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044451.D
Acq On : 29 Feb 2024 22:10
Operator : MA/JU
Sample : P1501-21
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044451.D
Acq On : 29 Feb 2024 22:10
Operator : MA/JU
Sample : P1501-21
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10C0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------