

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044452.D
 Acq On : 29 Feb 2024 22:47
 Operator : MA/JU
 Sample : P1501-02
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E10A0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.375	46	49	55	rVB	53273	62042	0.99%	0.106%
2	3.799	118	121	137	rBV	298138	535066	8.51%	0.915%
3	4.122	172	176	183	rVB	22167	32146	0.51%	0.055%
4	5.616	425	430	433	rVB7	5950	9310	0.15%	0.016%
5	7.134	682	688	697	rVB	236019	377099	6.00%	0.645%
6	7.310	712	718	731	rBV	968252	1529630	24.32%	2.615%
7	7.493	742	749	760	rBV	879795	1387879	22.07%	2.373%
8	7.969	823	830	838	rBV	838530	1325785	21.08%	2.267%
9	8.687	945	952	961	rBV	623568	1055212	16.78%	1.804%
10	9.145	1019	1030	1043	rBV	1008613	1751261	27.85%	2.994%
11	9.251	1045	1048	1052	rVV6	4810	9202	0.15%	0.016%
12	9.298	1055	1056	1064	rVB8	3447	7429	0.12%	0.013%
13	9.534	1092	1096	1099	rBV3	6465	9196	0.15%	0.016%
14	9.863	1145	1152	1165	rBV	804057	1357211	21.58%	2.321%
15	10.398	1235	1243	1257	rBV	1127727	1949737	31.01%	3.334%
16	10.781	1301	1308	1316	rVB	1150846	1960335	31.17%	3.352%
17	10.928	1324	1333	1347	rBV	1064202	1920565	30.54%	3.284%
18	11.610	1445	1449	1454	rVB6	7362	11847	0.19%	0.020%
19	12.369	1571	1578	1585	rBV2	23877	40445	0.64%	0.069%
20	13.439	1757	1760	1765	rBV5	6044	9137	0.15%	0.016%
21	13.516	1768	1773	1778	rVB	19771	33134	0.53%	0.057%
22	14.033	1853	1861	1876	rBV	2179999	3037139	48.30%	5.193%
23	14.304	1899	1907	1919	rBV	2658650	3905739	62.11%	6.678%
24	14.610	1952	1959	1966	rBV	1714996	2535653	40.32%	4.336%
25	14.827	1990	1996	2008	rBV2	53647	177333	2.82%	0.303%
26	15.598	2120	2127	2142	rBV	3322291	4976096	79.13%	8.508%
27	15.727	2142	2149	2161	rVV	990731	1461290	23.24%	2.499%
28	15.839	2164	2168	2173	rVB4	15152	26934	0.43%	0.046%
29	16.386	2256	2261	2265	rVB5	11164	16412	0.26%	0.028%
30	17.033	2366	2371	2376	rBV8	6993	11931	0.19%	0.020%
31	17.357	2419	2426	2436	rBV	2026950	2872519	45.68%	4.912%
32	17.457	2436	2443	2459	rVV	3965654	5710734	90.81%	9.764%
33	17.663	2473	2478	2482	rVB6	6329	9203	0.15%	0.016%
34	18.039	2536	2542	2545	rBV6	5598	10412	0.17%	0.018%
35	18.262	2575	2580	2586	rBV	81852	111362	1.77%	0.190%
36	18.745	2660	2662	2667	rVB6	5801	6317	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044452.D
Acq On : 29 Feb 2024 22:47
Operator : MA/JU
Sample : P1501-02
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.315	2754	2759	2763	rBV2	45798	68480	1.09%	0.117%
38	19.386	2767	2771	2776	rVV	39641	59112	0.94%	0.101%
39	19.462	2780	2784	2786	rBV4	8102	11235	0.18%	0.019%
40	19.545	2794	2798	2805	rBV4	42733	64311	1.02%	0.110%
41	19.698	2820	2824	2827	rBV4	23466	30071	0.48%	0.051%
42	19.751	2827	2833	2842	rVV	4507603	6288453	100.00%	10.752%
43	20.751	3001	3003	3005	rVB2	19185	15267	0.24%	0.026%
44	21.280	3090	3093	3098	rVB6	34769	48454	0.77%	0.083%
45	21.545	3133	3138	3148	rBV	2053417	2733943	43.48%	4.675%
46	23.821	3517	3525	3538	rBV2	2929035	6026181	95.83%	10.304%
47	23.980	3545	3552	3562	rVB	1389010	2897071	46.07%	4.954%




Sum of corrected areas: 58485320

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044452.D
Acq On : 29 Feb 2024 22:47
Operator : MA/JU
Sample : P1501-02
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

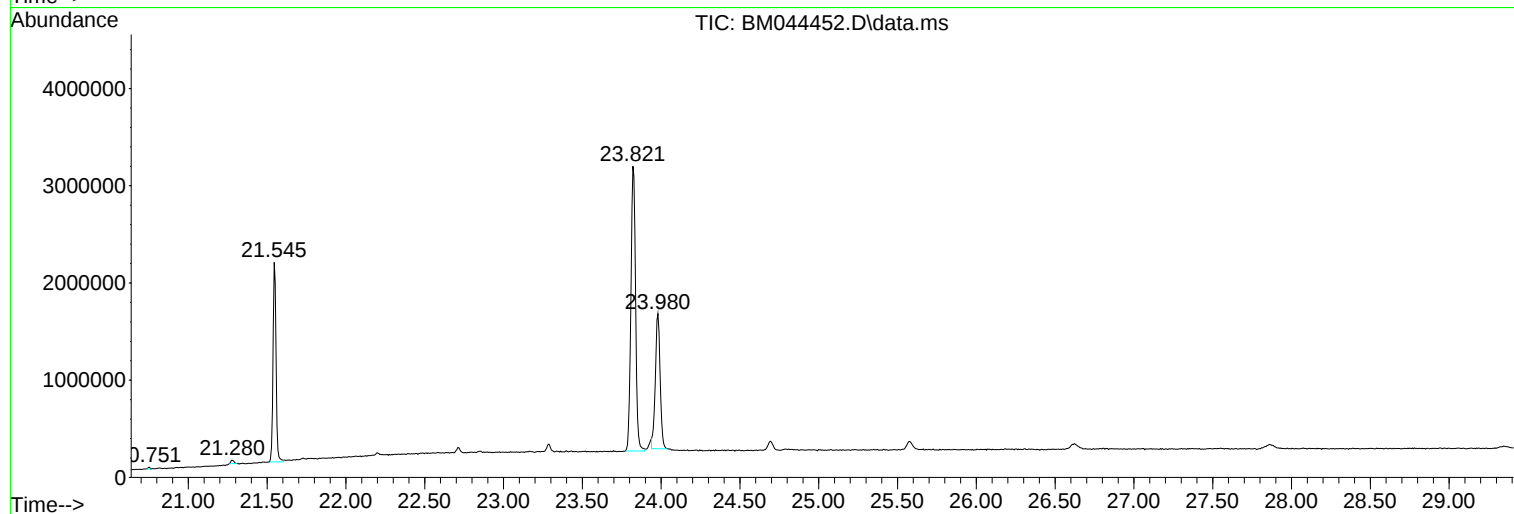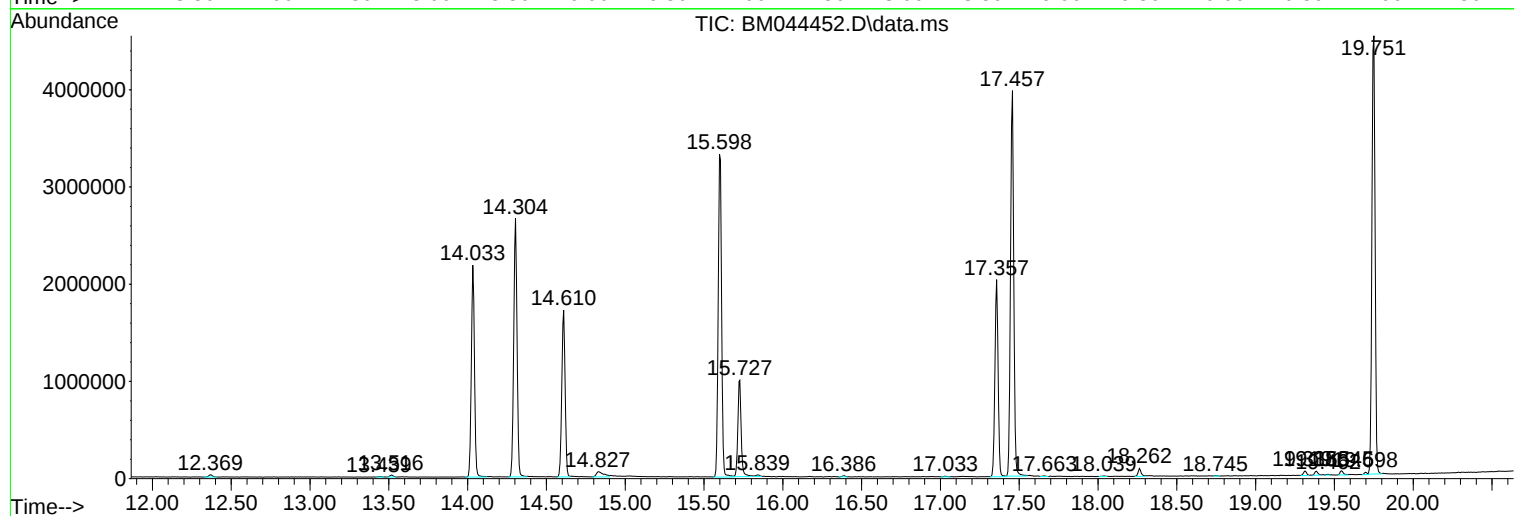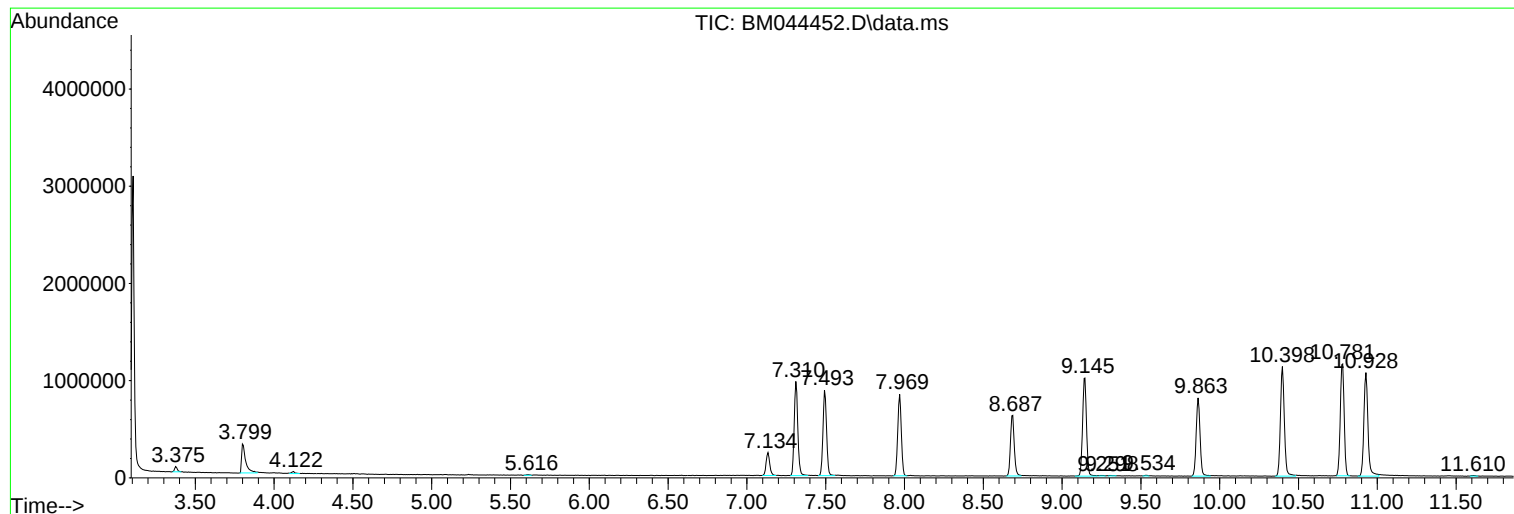

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044452.D
Acq On : 29 Feb 2024 22:47
Operator : MA/JU
Sample : P1501-02
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044452.D
Acq On : 29 Feb 2024 22:47
Operator : MA/JU
Sample : P1501-02
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc