

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044457.D
 Acq On : 01 Mar 2024 02:26
 Operator : MA/JU
 Sample : PB159242BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.163	9	13	26	rVB	528549	626973	12.98%	1.114%
2	3.387	47	51	60	rVB	78250	103787	2.15%	0.184%
3	3.804	119	122	147	rBV	884844	1448746	29.99%	2.575%
4	4.134	173	178	185	rVB3	37690	64791	1.34%	0.115%
5	4.310	206	208	212	rVB5	7875	8909	0.18%	0.016%
6	4.369	215	218	223	rVB3	15044	19299	0.40%	0.034%
7	4.522	241	244	249	rVB6	13078	19440	0.40%	0.035%
8	4.657	263	267	271	rBV5	7686	9943	0.21%	0.018%
9	4.704	271	275	281	rVB	52642	74048	1.53%	0.132%
10	4.763	281	285	292	rVB3	15688	26463	0.55%	0.047%
11	5.869	470	473	479	rVB7	6507	9932	0.21%	0.018%
12	6.304	543	547	552	rVV7	7272	13308	0.28%	0.024%
13	7.157	685	692	701	rBV	975825	1535109	31.77%	2.728%
14	7.334	716	722	733	rBV	803849	1290038	26.70%	2.293%
15	7.516	747	753	766	rVB	971250	1533776	31.75%	2.726%
16	7.704	781	785	792	rVB9	8049	17755	0.37%	0.032%
17	7.992	827	834	842	rVB	869136	1360697	28.16%	2.418%
18	8.169	858	864	868	rBV8	4346	8225	0.17%	0.015%
19	8.239	871	876	881	rVB8	6262	11480	0.24%	0.020%
20	8.710	948	956	969	rBV	1140484	1887166	39.06%	3.354%
21	9.169	1026	1034	1047	rBV	892003	1470924	30.45%	2.614%
22	9.339	1060	1063	1069	rVB7	4074	5317	0.11%	0.009%
23	9.886	1147	1156	1167	rBV	690737	1194613	24.73%	2.123%
24	10.422	1240	1247	1270	rBV	1056884	1888645	39.09%	3.357%
25	10.675	1285	1290	1296	rVB9	6226	10452	0.22%	0.019%
26	10.804	1303	1312	1321	rBV	1203943	2015875	41.72%	3.583%
27	10.951	1329	1337	1354	rBV	1020185	1979941	40.98%	3.519%
28	11.457	1419	1423	1426	rBV5	4514	8360	0.17%	0.015%
29	11.575	1438	1443	1447	rBV7	5687	11400	0.24%	0.020%
30	11.651	1452	1456	1460	rVV7	3091	5445	0.11%	0.010%
31	12.398	1577	1583	1588	rBV2	18948	30376	0.63%	0.054%
32	13.545	1773	1778	1783	rBV2	19027	30430	0.63%	0.054%
33	14.057	1859	1865	1880	rBV	1964219	2693244	55.74%	4.787%
34	14.163	1880	1883	1888	rVB5	3093	4975	0.10%	0.009%
35	14.327	1904	1911	1923	rBV	2209749	3331308	68.95%	5.921%
36	14.627	1956	1962	1976	rBV	1707053	2591067	53.63%	4.605%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044457.D
 Acq On : 01 Mar 2024 02:26
 Operator : MA/JU
 Sample : PB159242BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK242

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	14.839	1991	1998	2022	rBV	431547	1130458	23.40%	2.009%
38	15.621	2124	2131	2146	rBV	2875321	4113040	85.13%	7.310%
39	15.745	2146	2152	2168	rVV	768153	1093086	22.62%	1.943%
40	15.863	2168	2172	2176	rVB4	14633	21629	0.45%	0.038%
41	16.186	2224	2227	2231	rBV6	3917	6250	0.13%	0.011%
42	16.410	2260	2265	2270	rBV6	9566	12722	0.26%	0.023%
43	17.051	2371	2374	2382	rBV7	4811	9049	0.19%	0.016%
44	17.168	2390	2394	2396	rVB4	5283	6012	0.12%	0.011%
45	17.374	2422	2429	2440	rBV	2058431	2922257	60.48%	5.194%
46	17.474	2440	2446	2459	rBV2	3096367	4354952	90.14%	7.740%
47	19.333	2755	2762	2768	rBV4	36045	53929	1.12%	0.096%
48	19.403	2768	2774	2780	rBV	33998	49982	1.03%	0.089%
49	19.568	2799	2802	2805	rBV5	4990	7209	0.15%	0.013%
50	19.768	2829	2836	2845	rBV	3566274	4831384	100.00%	8.587%
51	21.562	3136	3141	3155	rBV	2012043	2768633	57.31%	4.921%
52	23.850	3522	3530	3544	rBV2	2186403	4596863	95.15%	8.170%
53	24.009	3550	3557	3571	rVB	1362447	2947138	61.00%	5.238%




Sum of corrected areas: 56266850

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044457.D
Acq On : 01 Mar 2024 02:26
Operator : MA/JU
Sample : PB159242BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK242

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

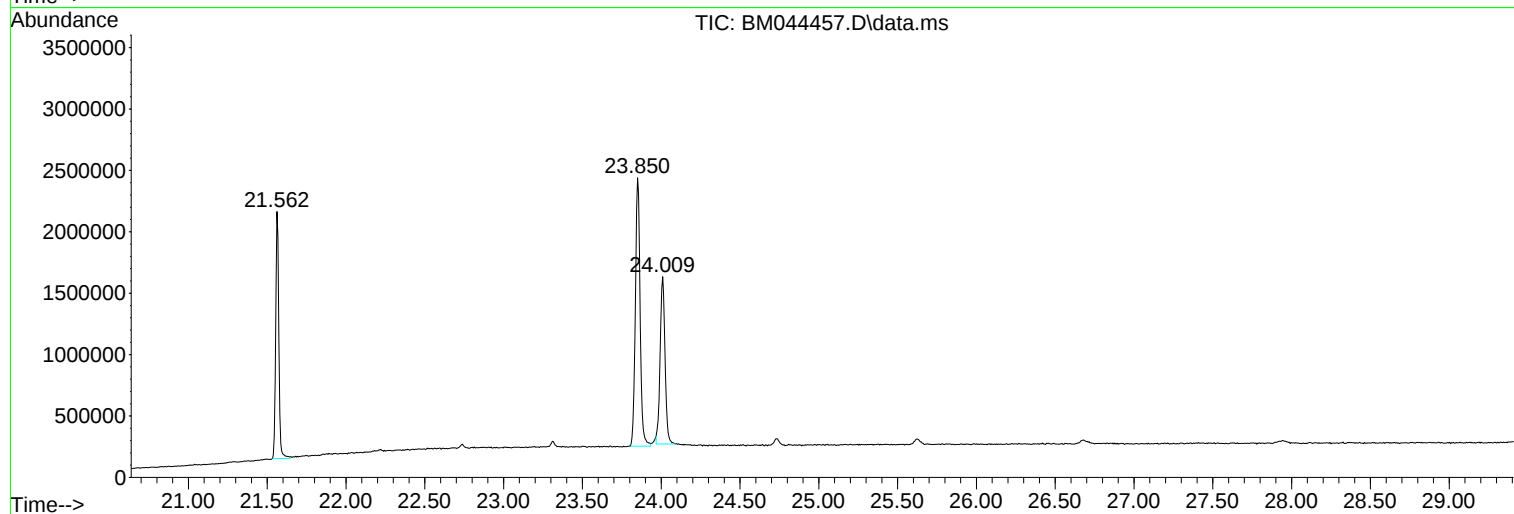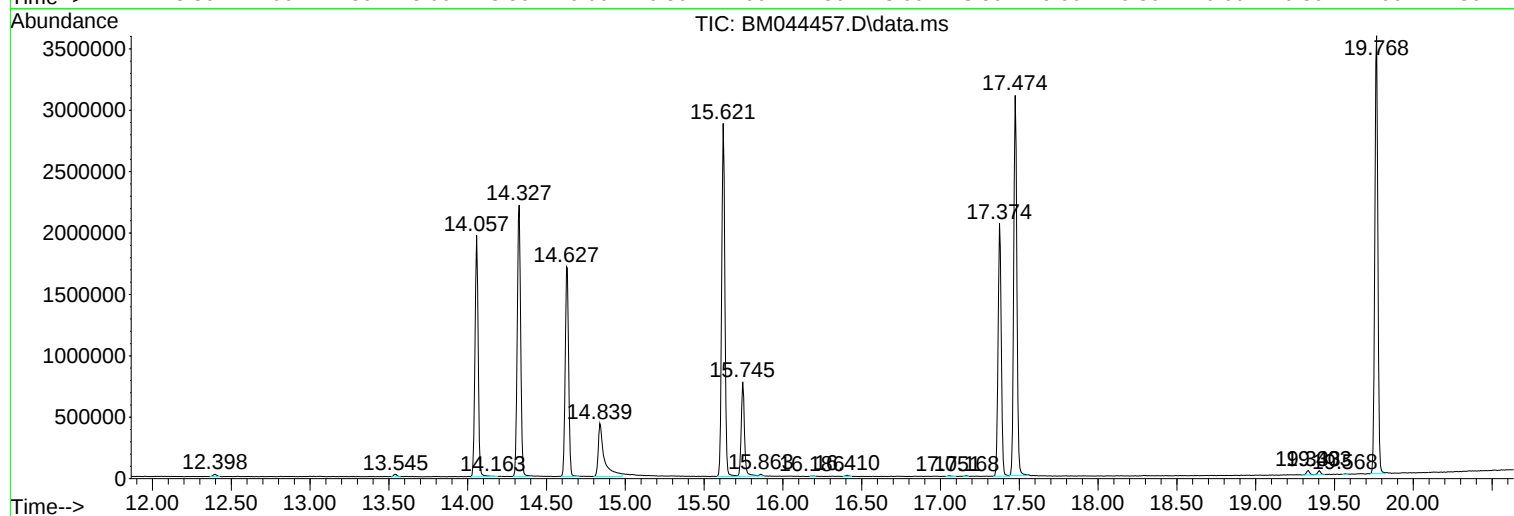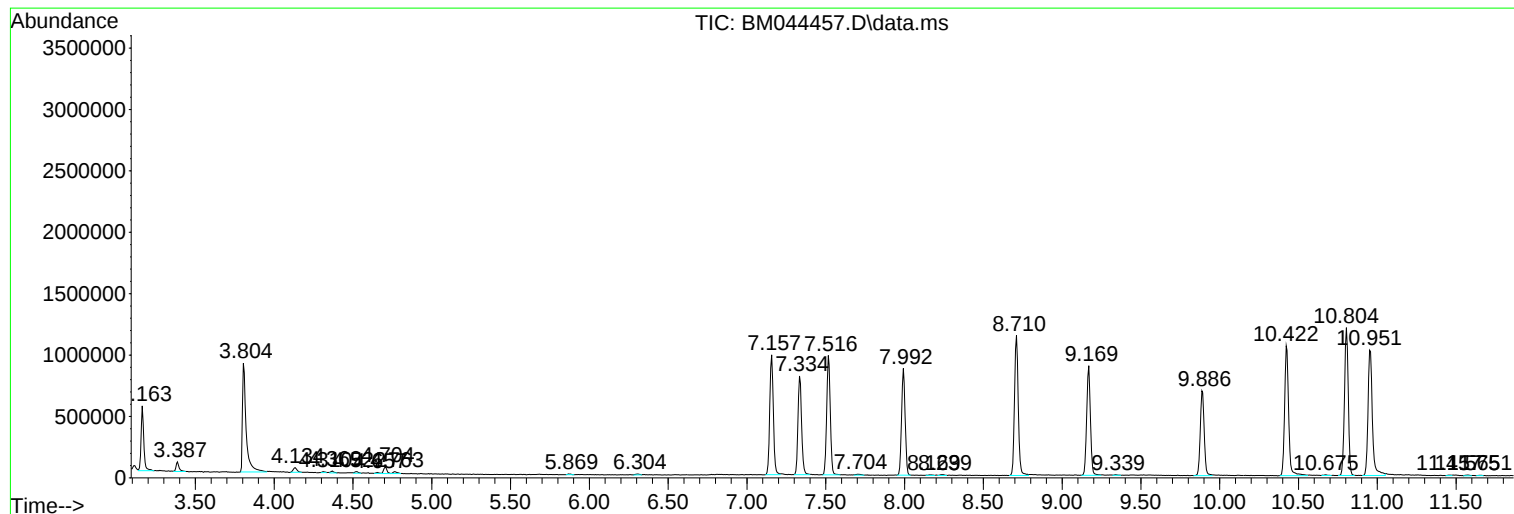

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044457.D
Acq On : 01 Mar 2024 02:26
Operator : MA/JU
Sample : PB159242BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK242










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Furan, tetrahydro-2-(methox... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.163	9.22 ng/ul	626973	1,4-Dichlorobenzene-d4	7.992

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Furan, tetrahydro-2-(methoxymeth...	116	C6H12O2	019354-27-9	72
2			3-Buten-2-ol, 2-methyl-	86	C5H10O	000115-18-4	72
3			Pentane, 2,2'-oxybis-	158	C10H22O	056762-00-6	64
4			3-Buten-2-ol, 2-methyl-	86	C5H10O	000115-18-4	59
5			3-Buten-2-ol, 2-methyl-	86	C5H10O	000115-18-4	50

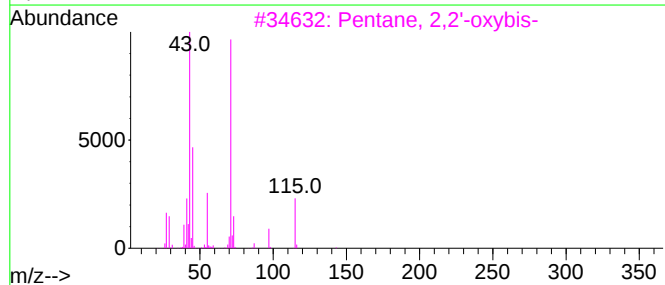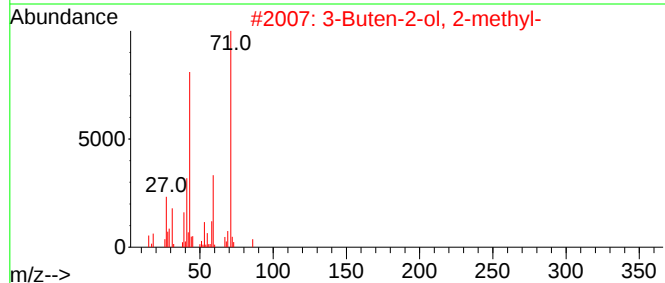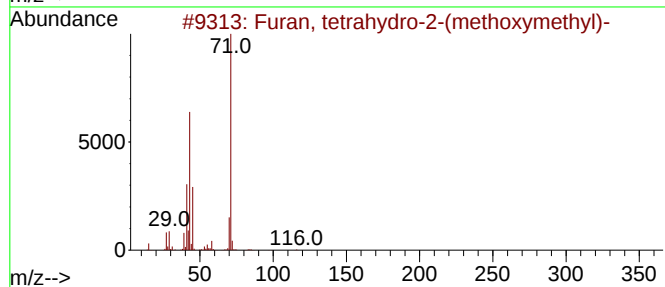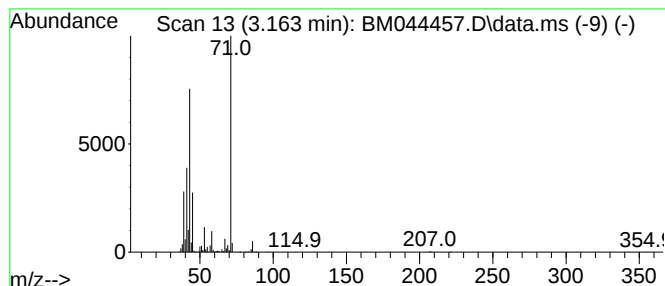

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044457.D
Acq On : 01 Mar 2024 02:26
Operator : MA/JU
Sample : PB159242BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK242

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Furan, tetrahyd...	3.163	9.2	ng/u1	626973	1	7.992	1360700	20.0