

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
 Data File : BM044460.D
 Acq On : 01 Mar 2024 04:15
 Operator : MA/JU
 Sample : P1501-01
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1098

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	48	51	61	rVB	56703	79806	1.25%	0.139%
2	3.817	121	124	142	rBV	228143	415684	6.50%	0.723%
3	4.134	175	178	185	rVB	39018	54654	0.85%	0.095%
4	7.157	685	692	703	rVB	209802	351573	5.49%	0.612%
5	7.334	714	722	737	rBV	914443	1491720	23.31%	2.595%
6	7.516	745	753	763	rBV	804974	1322003	20.66%	2.300%
7	7.993	828	834	843	rBV	786025	1236282	19.32%	2.150%
8	8.710	949	956	969	rBV	619989	1008199	15.76%	1.754%
9	9.169	1027	1034	1043	rBV	1020853	1704193	26.64%	2.964%
10	9.275	1050	1052	1056	rVB6	5984	8034	0.13%	0.014%
11	9.563	1095	1101	1108	rVB3	11288	24677	0.39%	0.043%
12	9.893	1149	1157	1172	rBV	799435	1340938	20.96%	2.332%
13	10.428	1240	1248	1262	rBV	1070224	1905017	29.77%	3.314%
14	10.804	1305	1312	1321	rBV	1087011	1839426	28.75%	3.200%
15	10.957	1328	1338	1357	rBV	897718	1714398	26.79%	2.982%
16	11.640	1448	1454	1458	rBV8	3195	6569	0.10%	0.011%
17	12.398	1578	1583	1591	rVB2	22887	39371	0.62%	0.068%
18	13.469	1761	1765	1770	rVB6	6305	8319	0.13%	0.014%
19	13.545	1773	1778	1783	rBV	19580	33848	0.53%	0.059%
20	14.057	1859	1865	1879	rBV	2212294	3136271	49.02%	5.455%
21	14.328	1904	1911	1924	rBV	2681809	3975850	62.14%	6.916%
22	14.633	1955	1963	1970	rBV	1624855	2386103	37.29%	4.150%
23	14.857	1995	2001	2013	rBV2	51754	173292	2.71%	0.301%
24	15.057	2030	2035	2037	rBV6	8037	13783	0.22%	0.024%
25	15.622	2124	2131	2146	rBV	3320004	4981341	77.86%	8.665%
26	15.745	2146	2152	2168	rVV	1030197	1511590	23.63%	2.629%
27	15.863	2168	2172	2178	rVB3	16099	28287	0.44%	0.049%
28	16.410	2261	2265	2271	rVB6	10473	16404	0.26%	0.029%
29	16.798	2324	2331	2335	rBV9	3847	8060	0.13%	0.014%
30	17.057	2372	2375	2379	rVB6	6863	8624	0.13%	0.015%
31	17.163	2391	2393	2398	rVB6	5374	8167	0.13%	0.014%
32	17.380	2423	2430	2440	rBV	1815071	2683700	41.94%	4.668%
33	17.480	2440	2447	2465	rVV	3864250	5774110	90.25%	10.044%
34	17.680	2478	2481	2486	rVB4	4231	6446	0.10%	0.011%
35	18.063	2542	2546	2550	rVB7	5250	8057	0.13%	0.014%
36	18.286	2579	2584	2591	rBV	121075	175126	2.74%	0.305%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044460.D
Acq On : 01 Mar 2024 04:15
Operator : MA/JU
Sample : P1501-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1098

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	18.721	2654	2658	2661	rVB6	8285	11695	0.18%	0.020%
38	18.768	2661	2666	2670	rBV7	6396	11623	0.18%	0.020%
39	19.333	2757	2762	2766	rBV2	45881	65930	1.03%	0.115%
40	19.404	2770	2774	2779	rBV	41653	60883	0.95%	0.106%
41	19.480	2785	2787	2792	rVB6	9036	9070	0.14%	0.016%
42	19.563	2797	2801	2808	rBV3	75944	105832	1.65%	0.184%
43	19.721	2824	2828	2830	rBV2	25182	30584	0.48%	0.053%
44	19.768	2830	2836	2844	rVV	4812460	6398206	100.00%	11.129%
45	21.298	3092	3096	3103	rBV5	51364	95531	1.49%	0.166%
46	21.562	3136	3141	3153	rBV2	1838885	2567613	40.13%	4.466%
47	23.856	3523	3531	3545	rBV2	2859703	5960495	93.16%	10.368%
48	24.009	3550	3557	3568	rVB	1262165	2693297	42.09%	4.685%




Sum of corrected areas: 57490681

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044460.D
Acq On : 01 Mar 2024 04:15
Operator : MA/JU
Sample : P1501-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

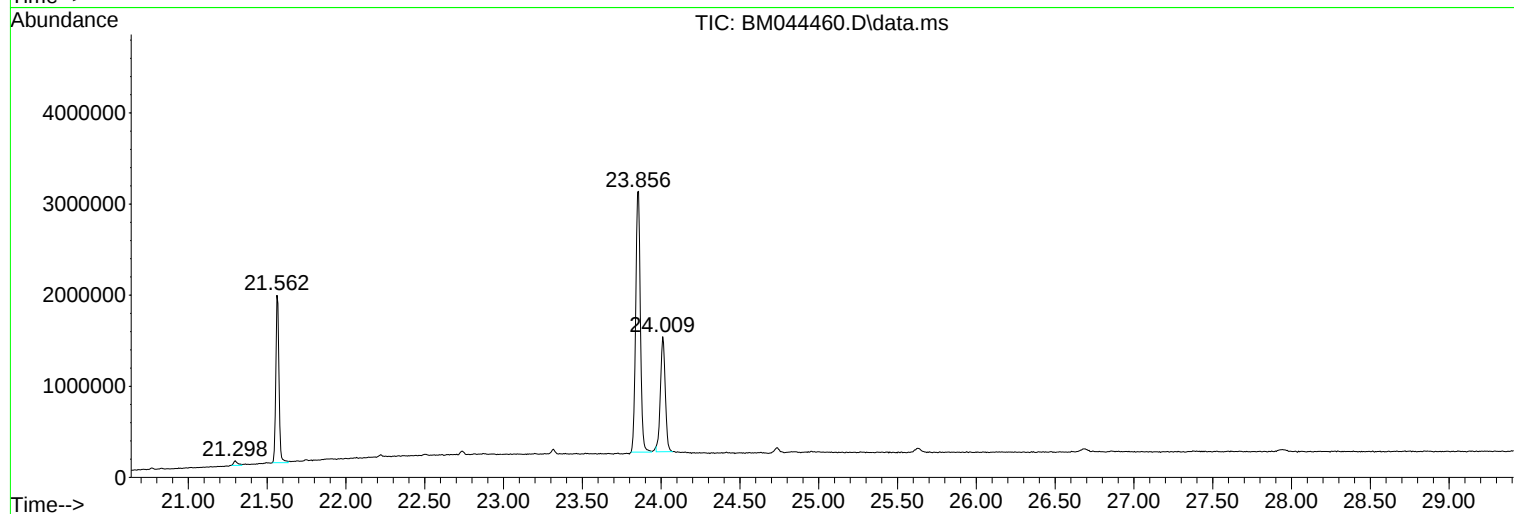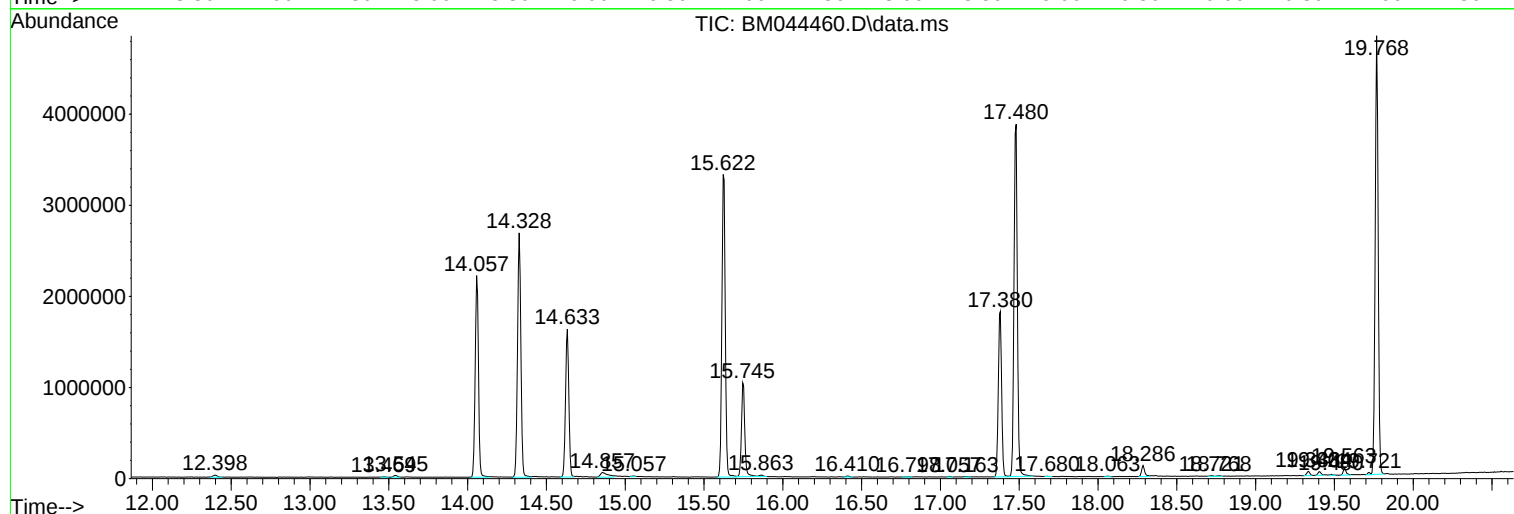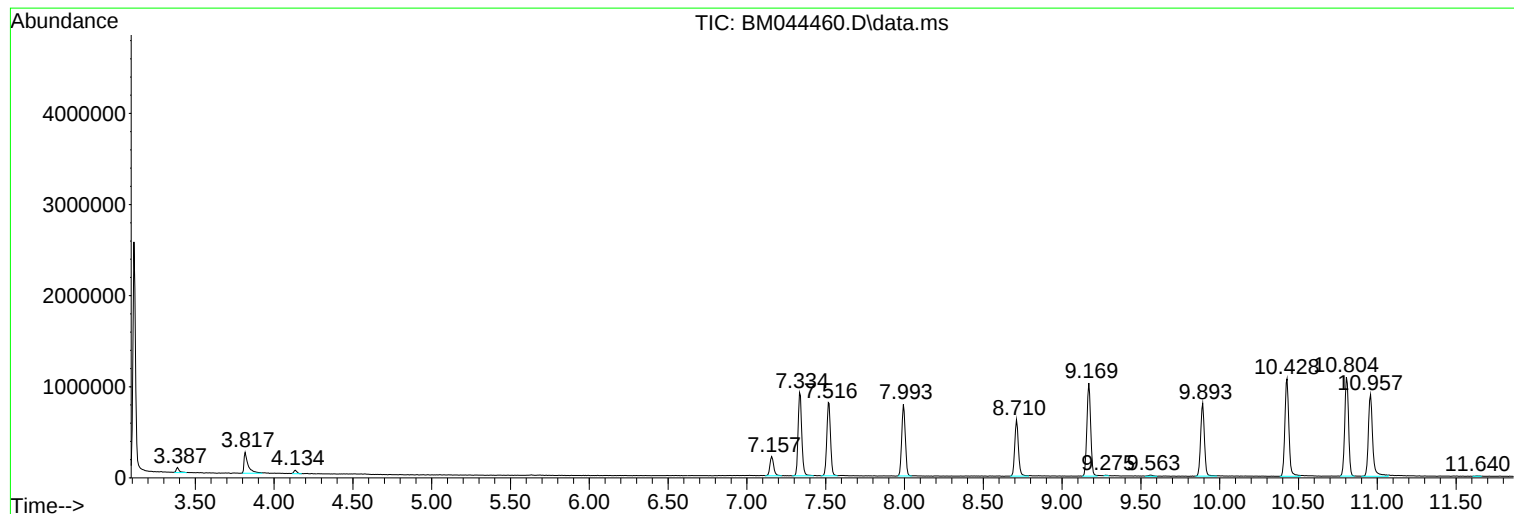

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044460.D
Acq On : 01 Mar 2024 04:15
Operator : MA/JU
Sample : P1501-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022824\
Data File : BM044460.D
Acq On : 01 Mar 2024 04:15
Operator : MA/JU
Sample : P1501-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1098

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc