
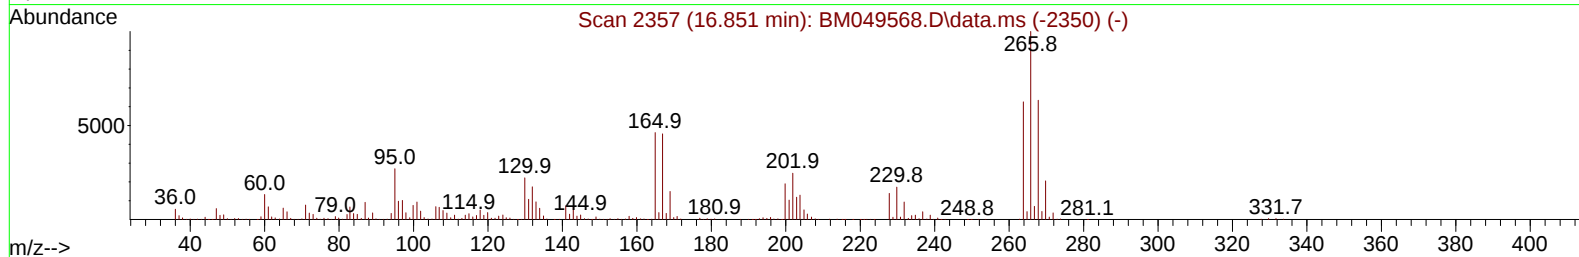
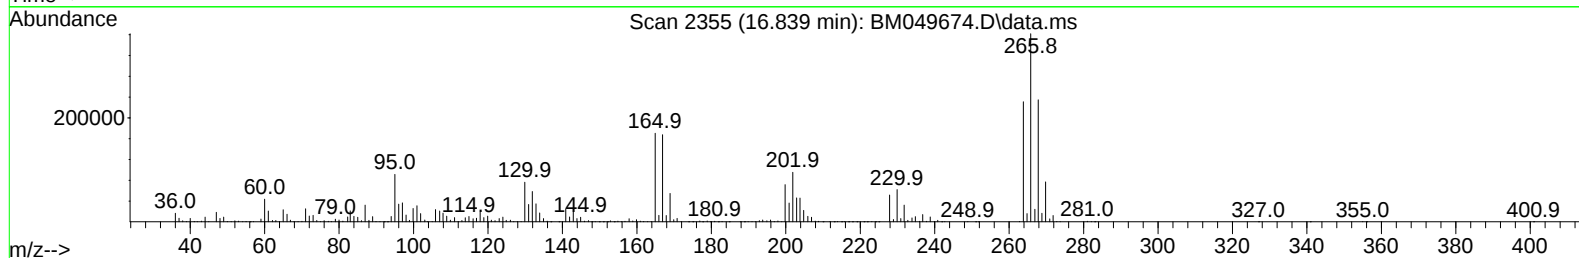


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049674.D
Acq On : 28 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 18:13:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

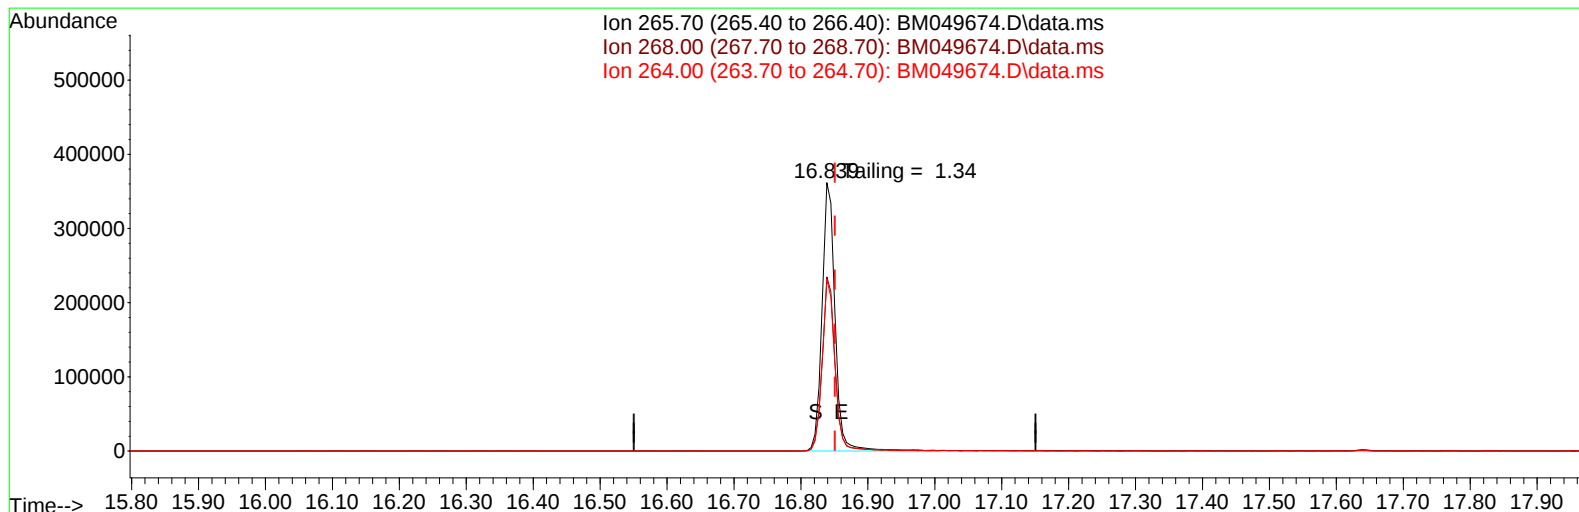

TIC: BM049674.D\data.ms

(70) Pentachlorophenol (C)




16.839min (-0.012) 32194.44 ng

response 486633

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.87
264.00	62.50	63.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049674.D
Acq On : 28 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 18:13:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

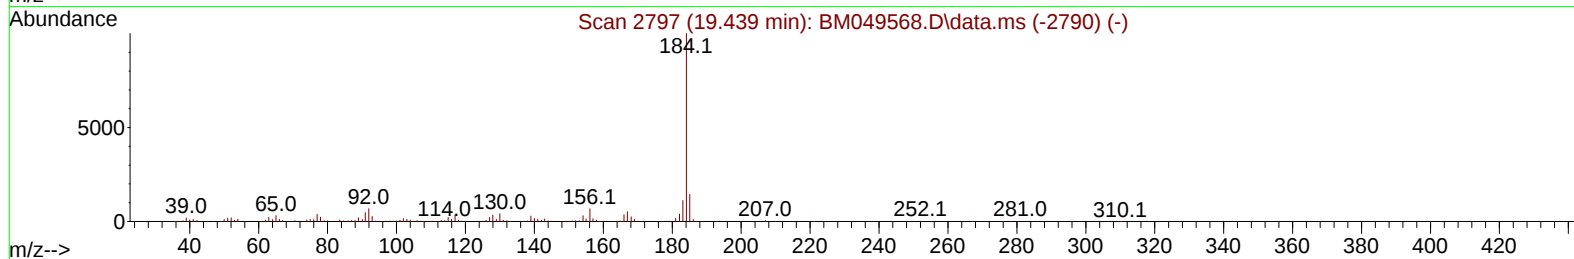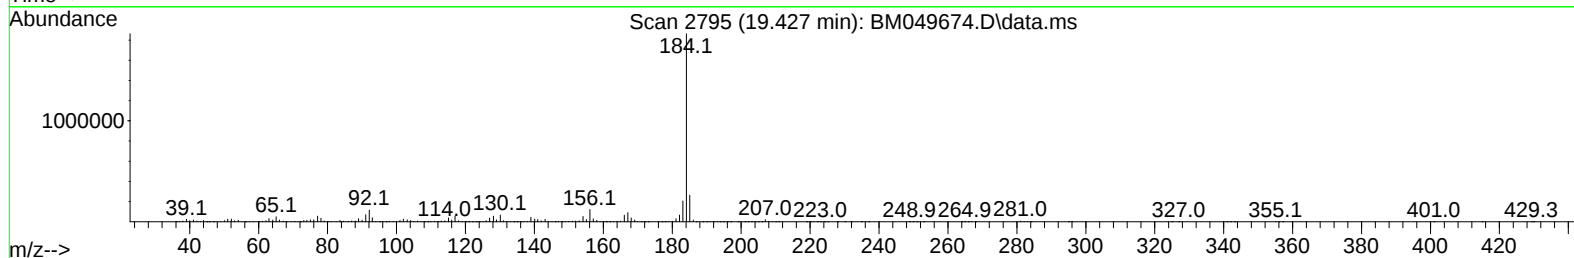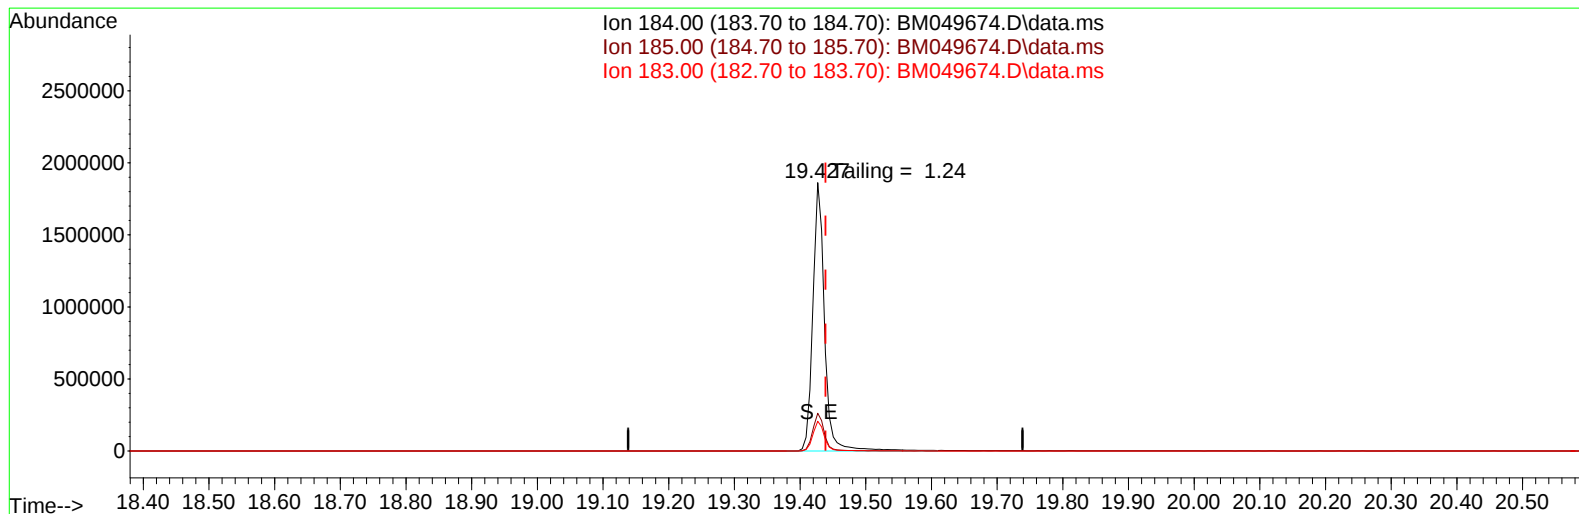

TIC: BM049674.D\data.ms

(77) Benzidine**19.427min (-0.012) 109569.14 ng****response 2304454**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.11
183.00	11.10	11.11
0.00	0.00	0.00