

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049676.D
Acq On : 28 Feb 2025 13:15
Operator : RC/JU
Sample : PB166930BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB166930BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM049676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	402	409	422	rBV	8347231	11279555	58.04%	12.761%
2	6.987	671	680	694	rBV	7053471	10961326	56.40%	12.401%
3	7.804	812	819	828	rVB	1331078	2040327	10.50%	2.308%
4	8.963	1006	1016	1023	rBV	4281759	6572410	33.82%	7.435%
5	10.604	1287	1295	1303	rBV	1499869	2444270	12.58%	2.765%
6	13.069	1707	1714	1727	rBV	11067807	15420472	79.35%	17.445%
7	14.445	1940	1948	1960	rBV	2018945	2844165	14.63%	3.218%
8	15.933	2193	2201	2219	rBV	7741894	9624177	49.52%	10.888%
9	17.186	2406	2414	2422	rBV	2218842	2897168	14.91%	3.278%
10	19.815	2855	2861	2872	rBV	18005047	19434132	100.00%	21.986%
11	21.427	3129	3135	3142	rBV	1776284	2509201	12.91%	2.839%
12	24.444	3640	3648	3657	rBV	979628	2365213	12.17%	2.676%




Sum of corrected areas: 88392416

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049676.D
Acq On : 28 Feb 2025 13:15
Operator : RC/JU
Sample : PB166930BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB166930BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

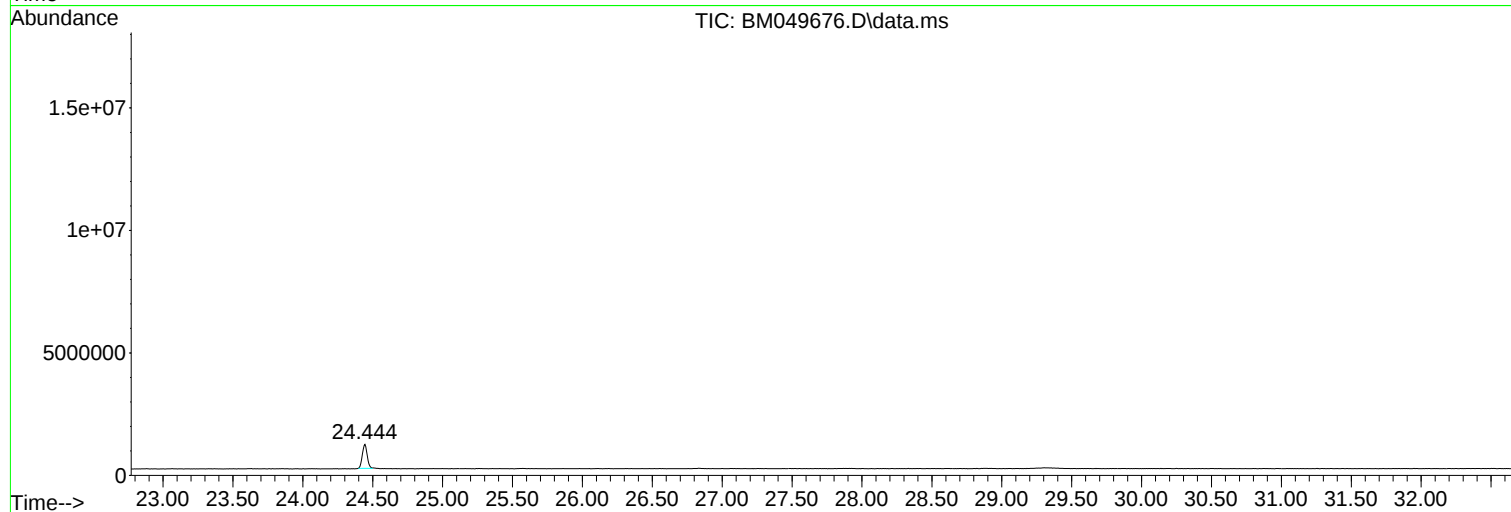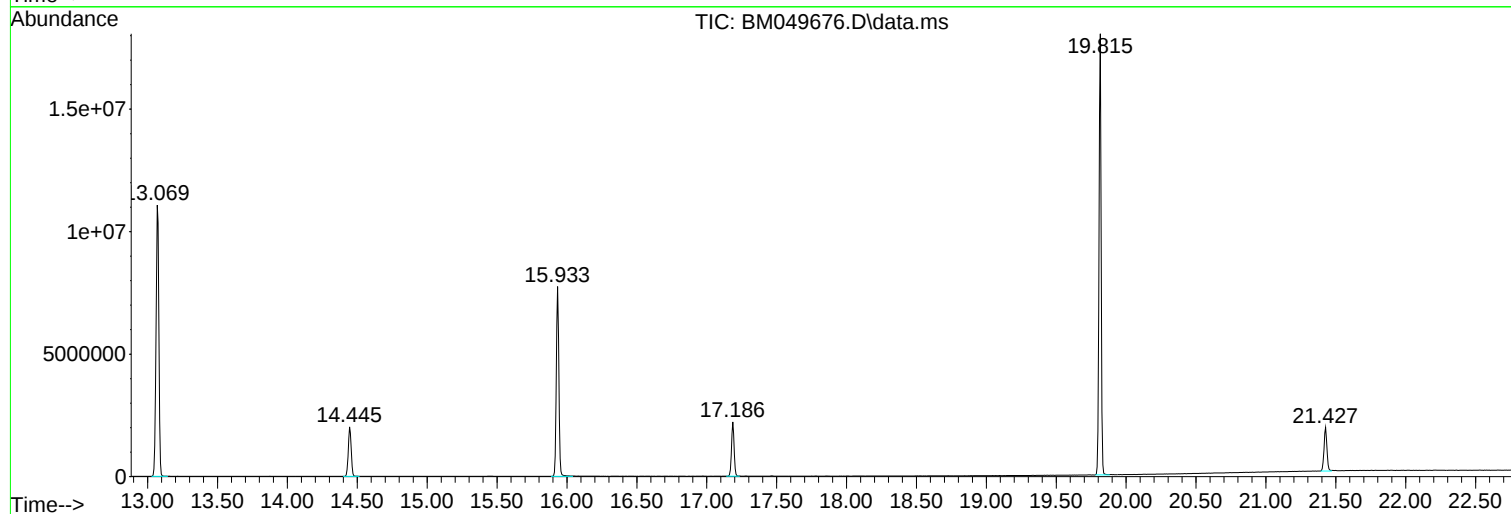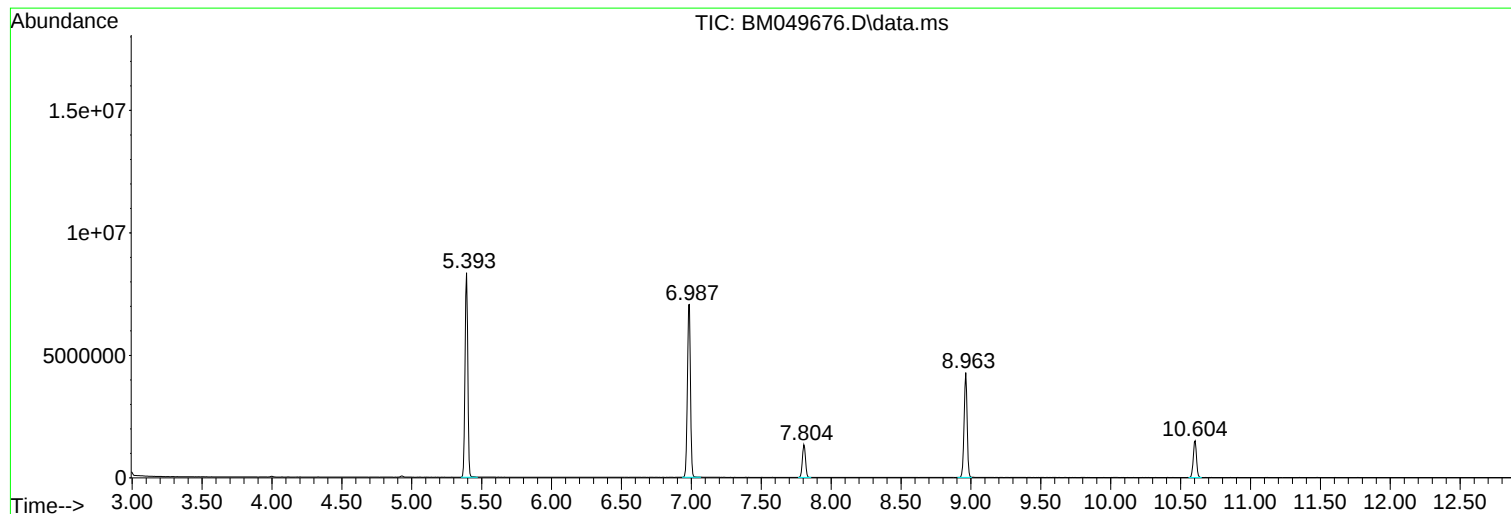

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049676.D
Acq On : 28 Feb 2025 13:15
Operator : RC/JU
Sample : PB166930BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB166930BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049676.D
Acq On : 28 Feb 2025 13:15
Operator : RC/JU
Sample : PB166930BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB166930BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------