

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
 Data File : BM049680.D
 Acq On : 28 Feb 2025 15:52
 Operator : RC/JU
 Sample : PB166933BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB166933BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM049680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	401	408	421	rBV	4369658	5838798	36.75%	9.568%
2	6.975	668	678	695	rBV	3792504	5641356	35.51%	9.245%
3	7.805	812	819	829	rVB	1017078	1529788	9.63%	2.507%
4	8.957	1006	1015	1025	rBV	3416343	5291754	33.31%	8.672%
5	10.599	1287	1294	1302	rBV	1119477	1794254	11.29%	2.940%
6	13.069	1706	1714	1727	rBV	8678728	12248200	77.09%	20.072%
7	14.439	1941	1947	1957	rBV	1407971	2080825	13.10%	3.410%
8	15.928	2194	2200	2219	rBV	3530820	4526172	28.49%	7.417%
9	17.180	2407	2413	2426	rBV2	1548377	2130705	13.41%	3.492%
10	19.810	2854	2860	2872	rBV	14181538	15887271	100.00%	26.035%
11	21.415	3128	3133	3140	rBV	1380063	1988540	12.52%	3.259%
12	24.433	3638	3646	3657	rBV	869934	2065156	13.00%	3.384%




Sum of corrected areas: 61022819

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049680.D
Acq On : 28 Feb 2025 15:52
Operator : RC/JU
Sample : PB166933BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB166933BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

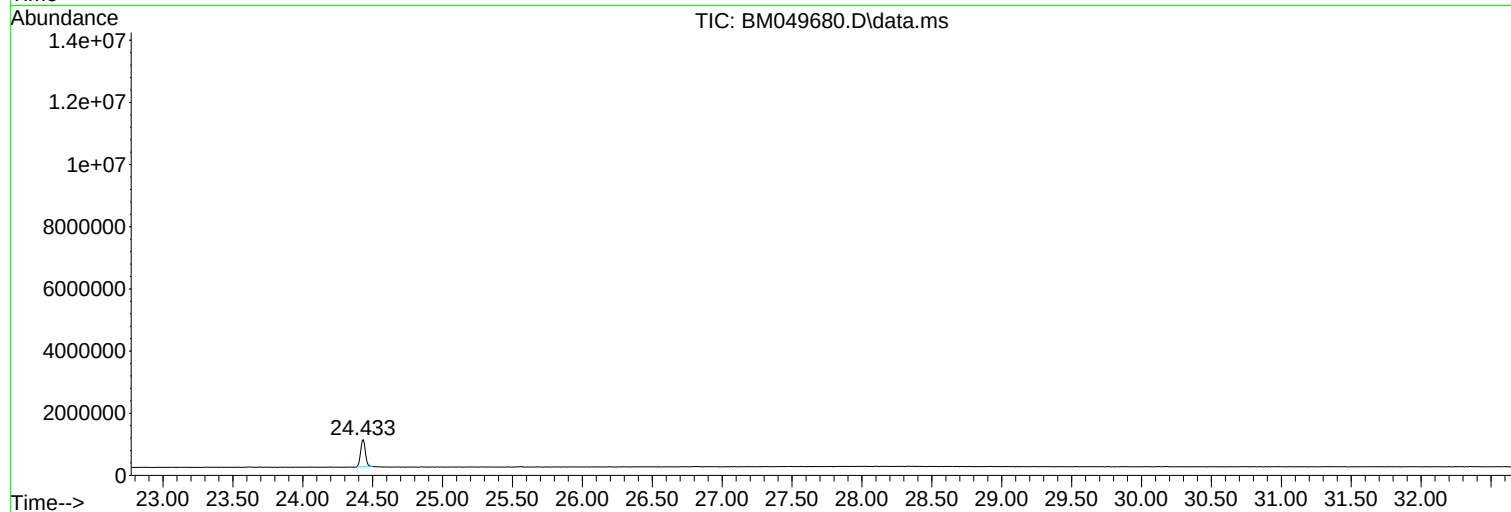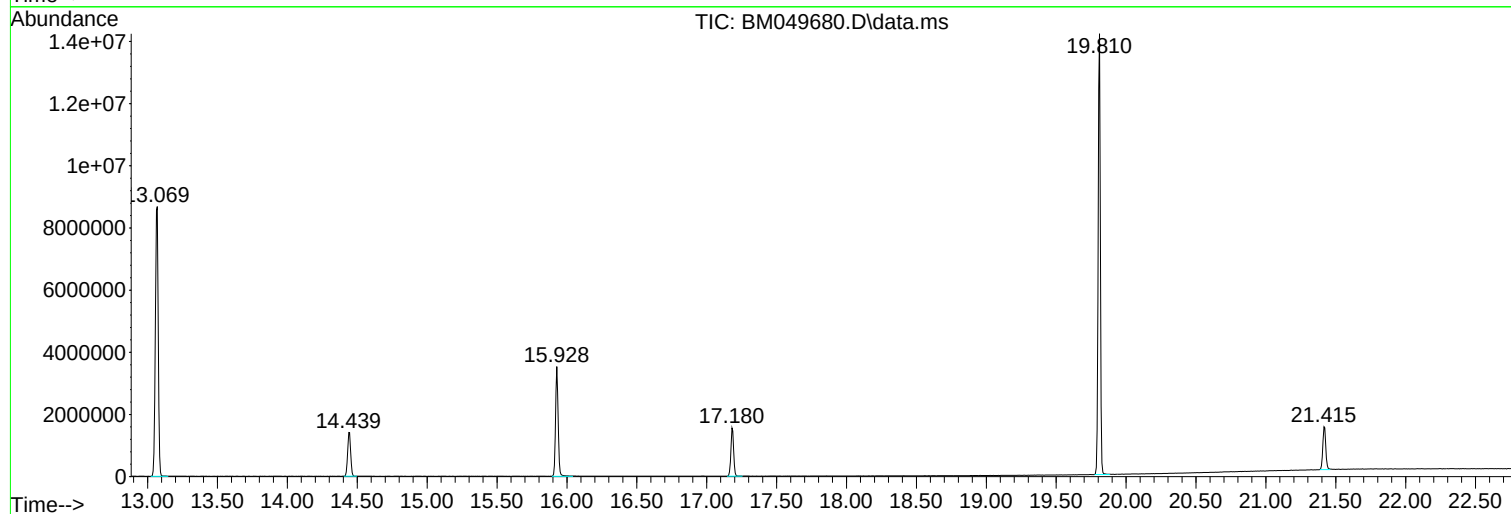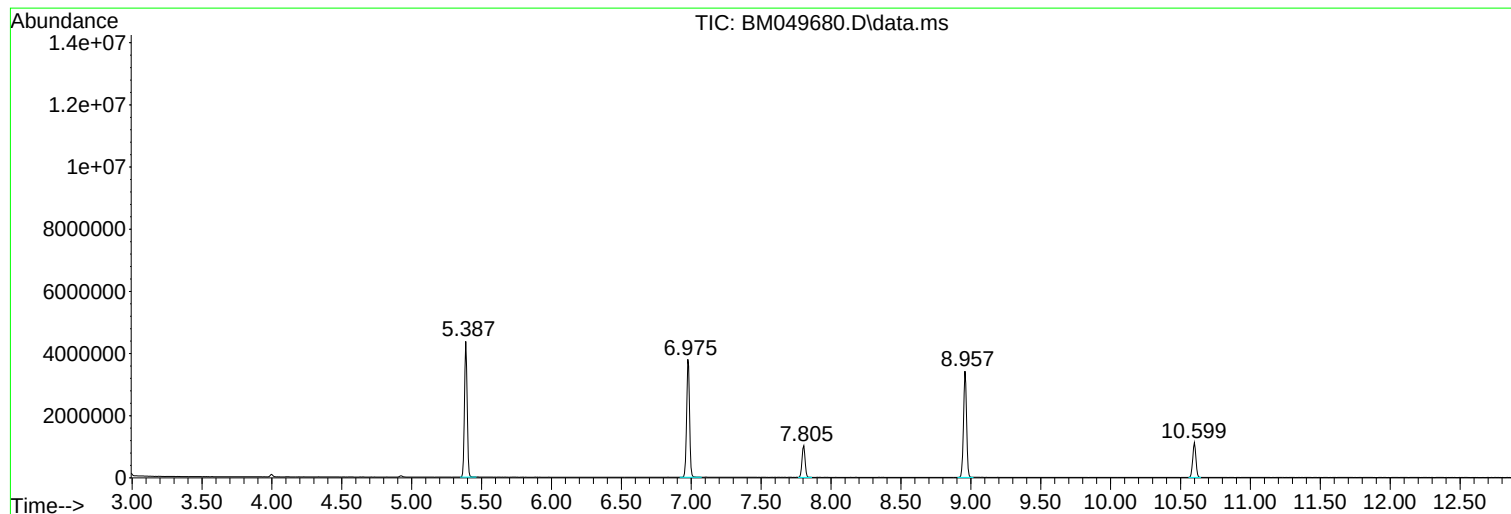

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049680.D
Acq On : 28 Feb 2025 15:52
Operator : RC/JU
Sample : PB166933BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB166933BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049680.D
Acq On : 28 Feb 2025 15:52
Operator : RC/JU
Sample : PB166933BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB166933BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------