


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049674.D
Acq On : 28 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 04:55:28 2025

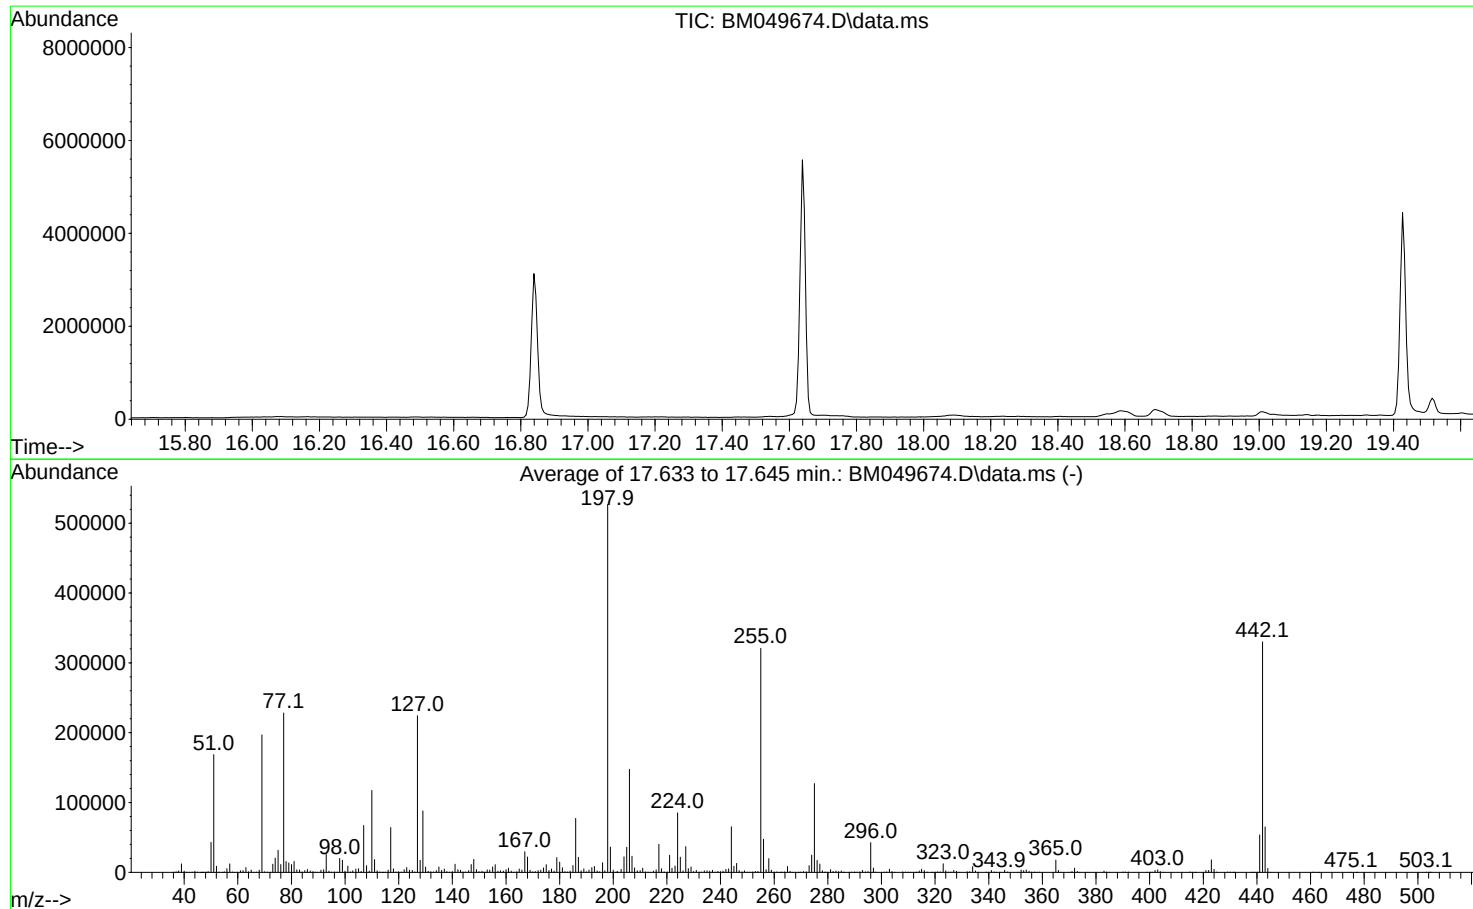

AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	168688	PASS
68	69	0.00	2	1.7	3318	PASS
69	198	0.00	100	37.4	196930	PASS
70	69	0.00	2	0.5	997	PASS
127	198	10	80	42.6	224235	PASS
197	198	0.00	2	0.4	2225	PASS
198	198	100	100	100.0	526805	PASS
199	198	5	9	6.9	36216	PASS
275	198	10	60	24.1	127184	PASS
365	198	1	100	3.3	17645	PASS
441	198	0.01	100	10.2	53744	PASS
442	442	50	100	100.0	330283	PASS
443	442	15	24	19.7	65032	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/28/2025	BNA_M	<u>BM049674.D</u>
Compound Name	Response	Retention Time
DDT	1525583	20.668
DDD	20140	20.227
DDE	6448	19.721
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26588	1552171	1.71

Instrument :
BNA_M
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049674.D
Acq On : 28 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 28 18:13:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

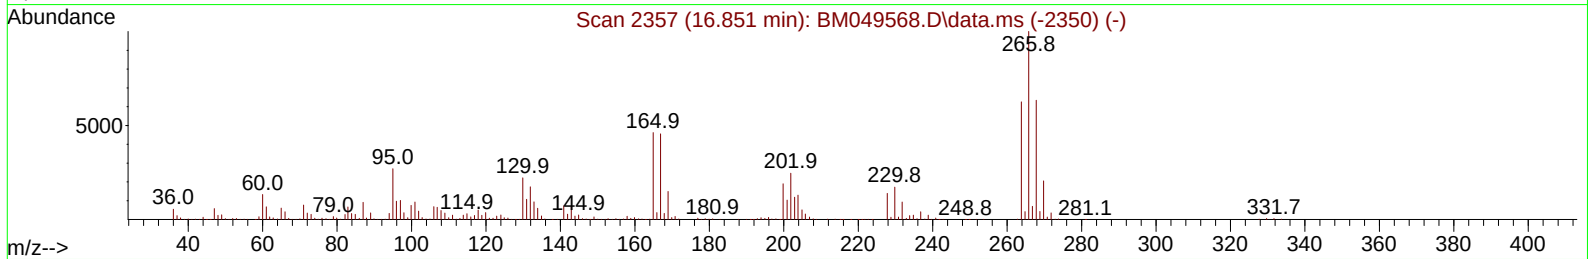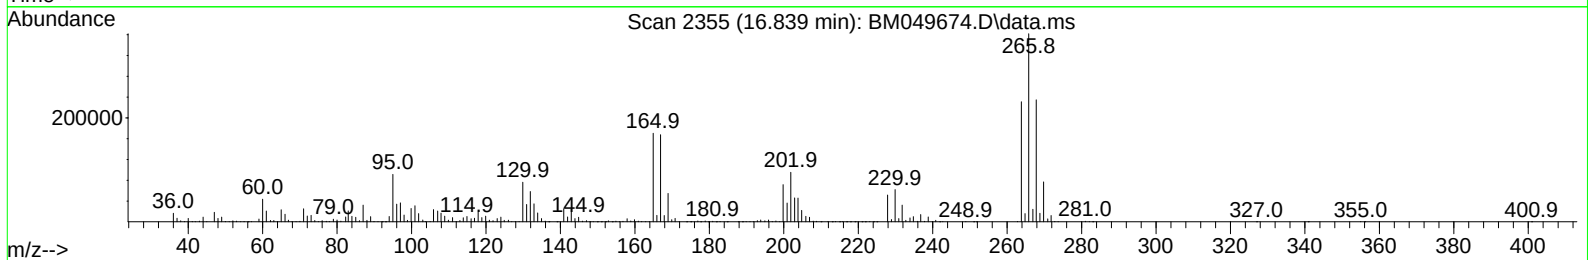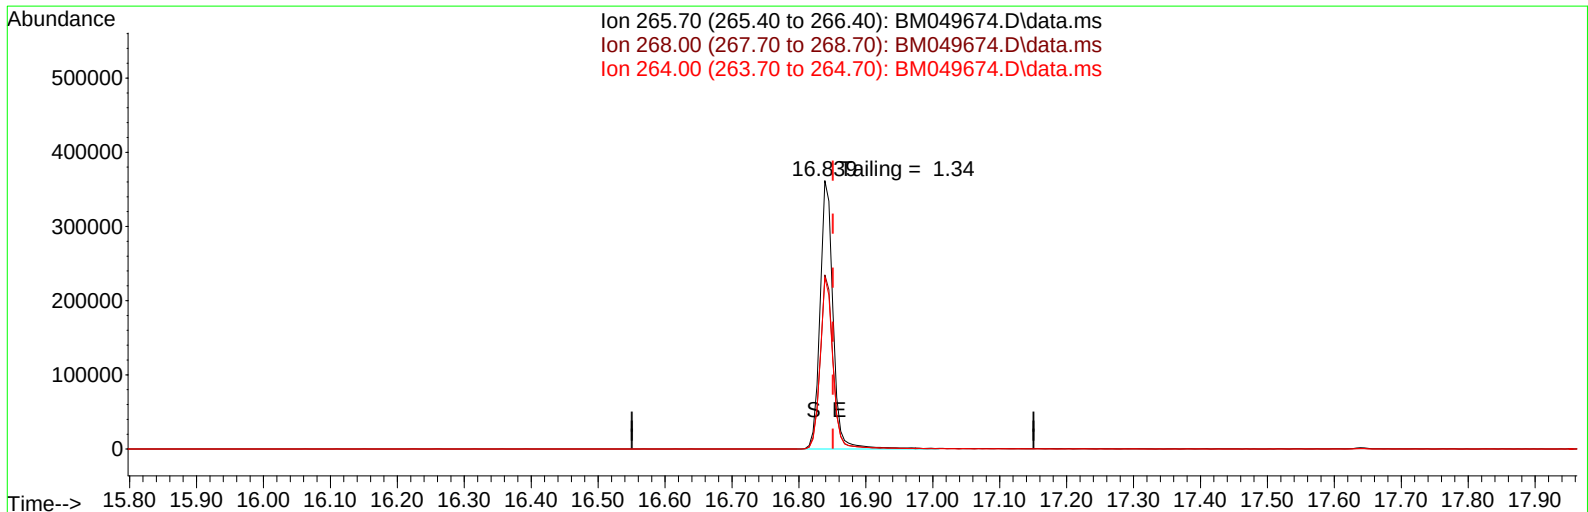

TIC: BM049674.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.012) 32194.44 ng




response 486633

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.87
264.00	62.50	63.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022825\
Data File : BM049674.D
Acq On : 28 Feb 2025 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 28 18:13:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 04:55:28 2025
Response via : Initial Calibration

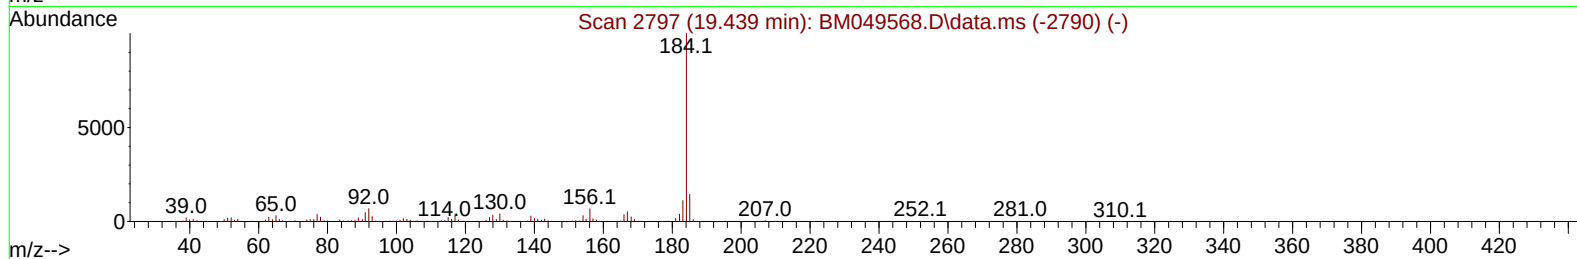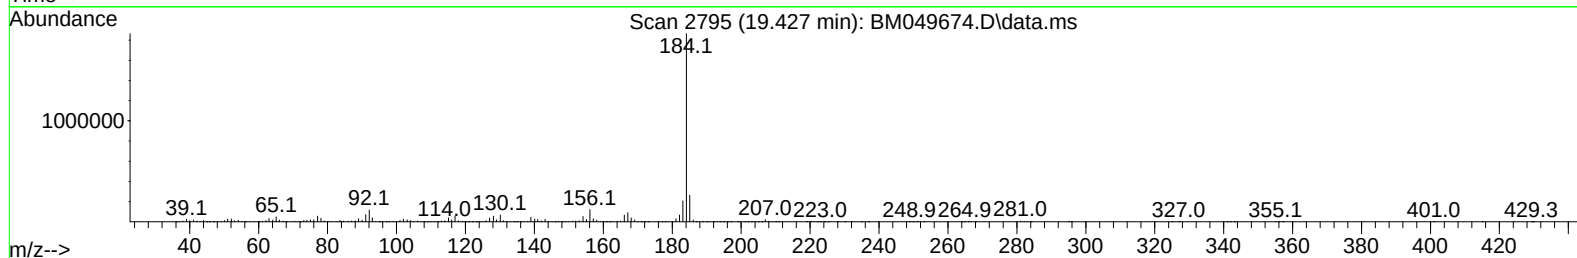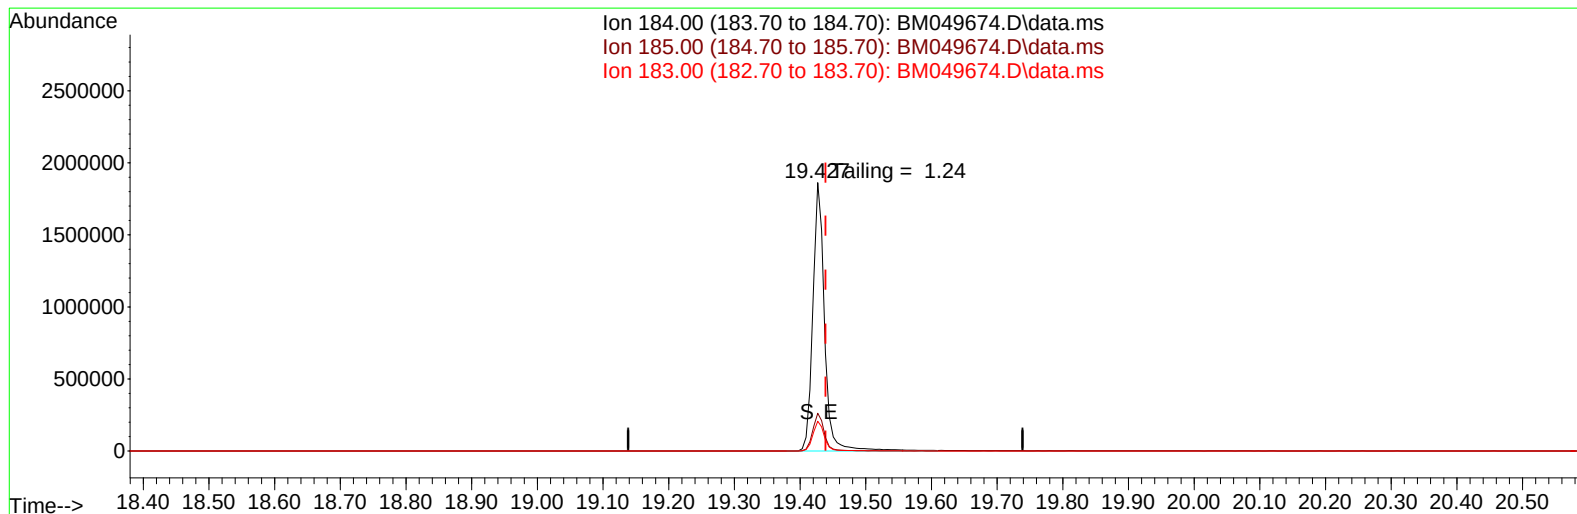

TIC: BM049674.D\data.ms

(77) Benzidine

19.427min (-0.012) 109569.14 ng

response 2304454

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.11
183.00	11.10	11.11
0.00	0.00	0.00