
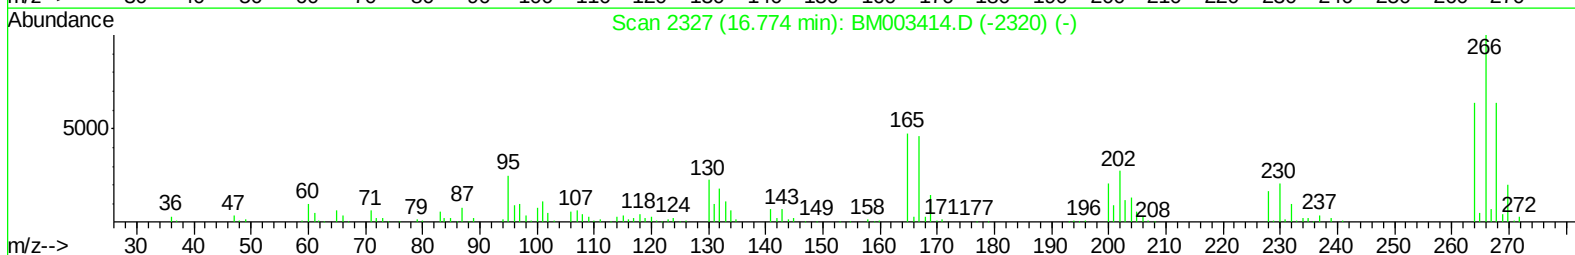
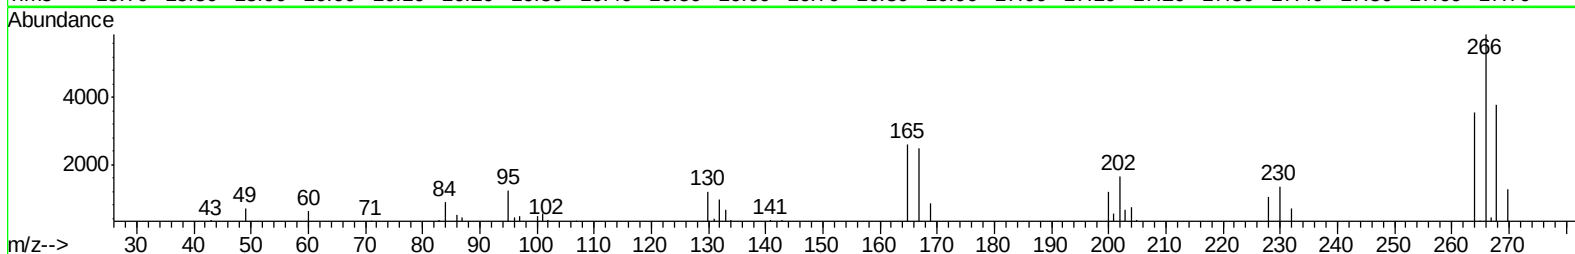


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022916\
Data File : BM004474.D
Acq On : 29 Feb 2016 16:56
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 01 08:07:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

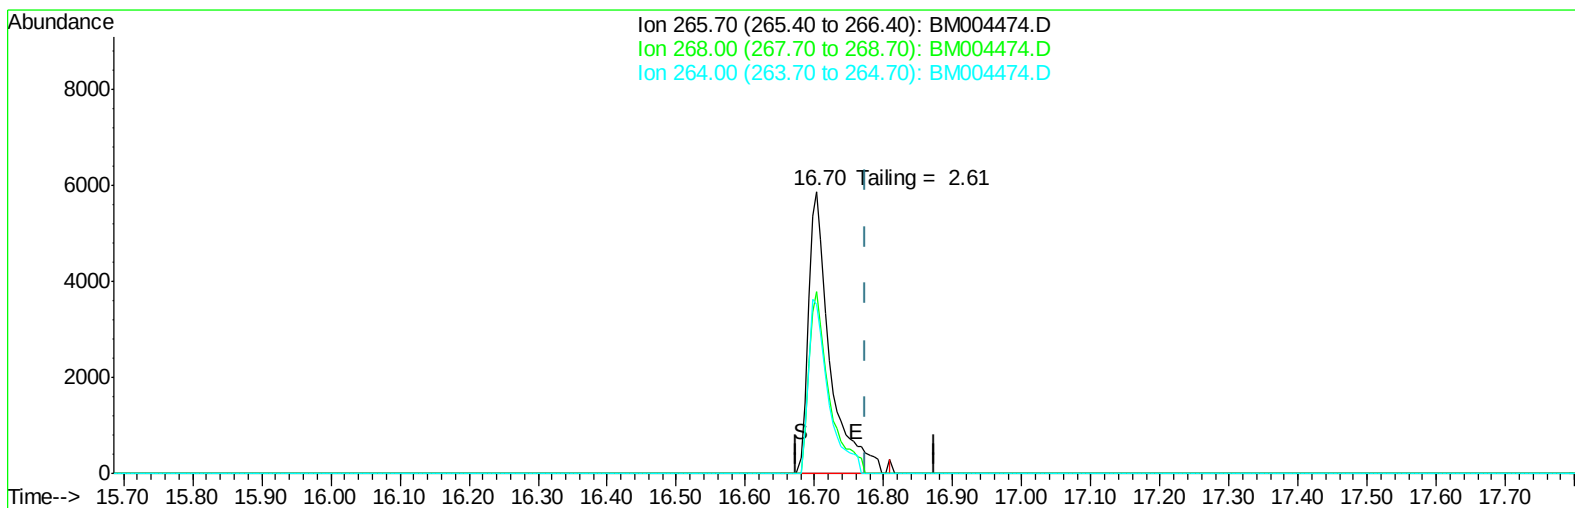

TIC: BM004474.D

(69) Pentachlorophenol (C)

16.703min (-0.071) 0.00ng




response 12104

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.61
264.00	61.20	60.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022916\
Data File : BM004474.D
Acq On : 29 Feb 2016 16:56
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 01 08:07:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

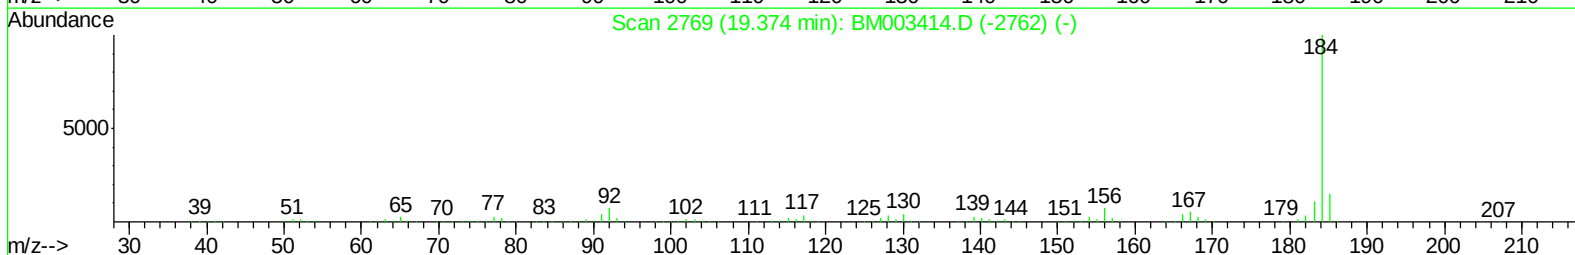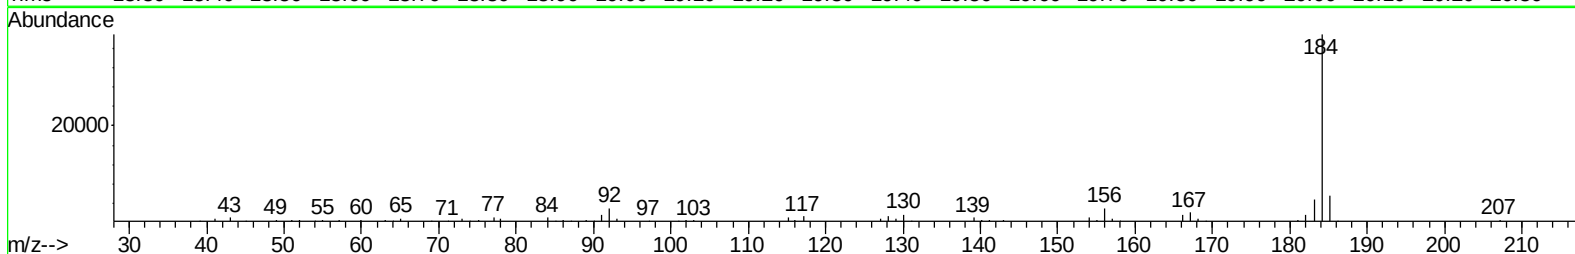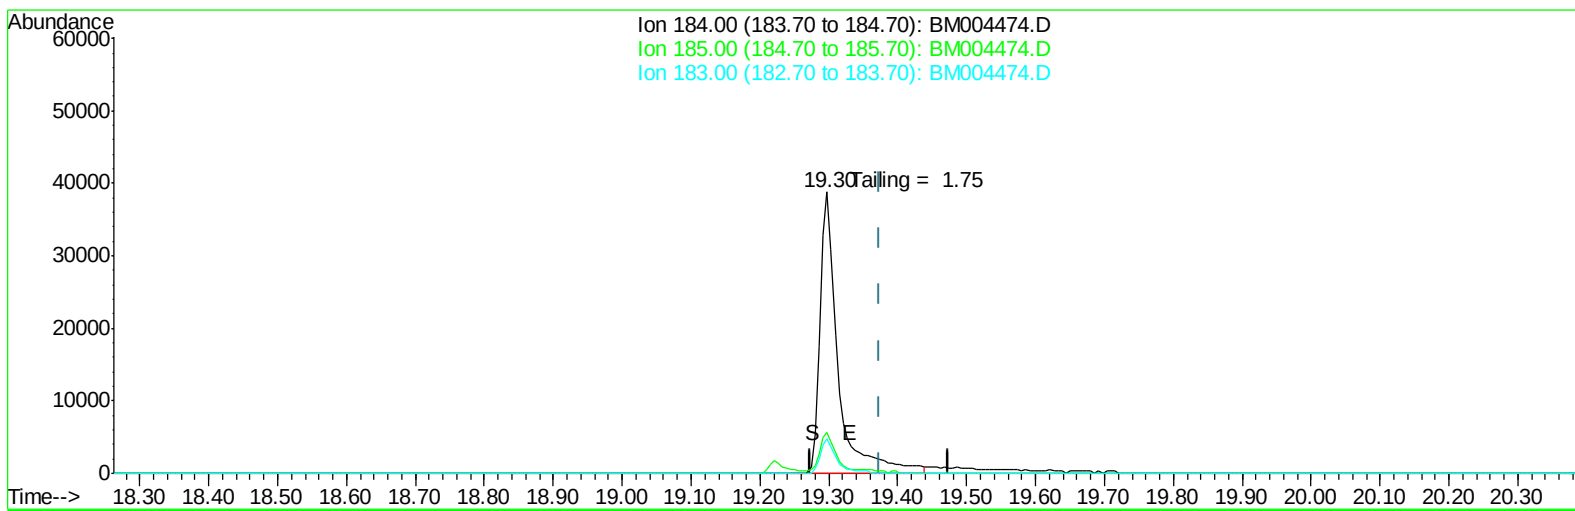

TIC: BM004474.D

(76) Benzidine

19.297min (-0.077) 405.12ng




response 67877

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.63
183.00	11.10	12.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022916\
Data File : BM004491.D
Acq On : 01 Mar 2016 04:59
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 01 08:08:37 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

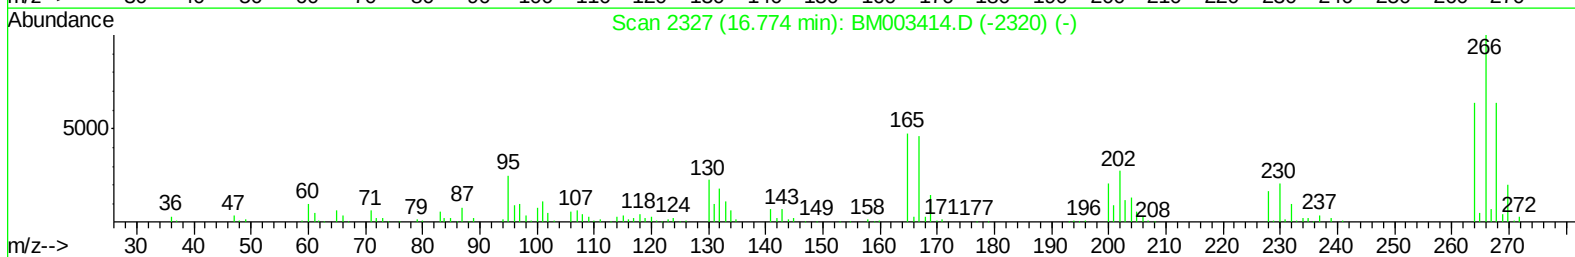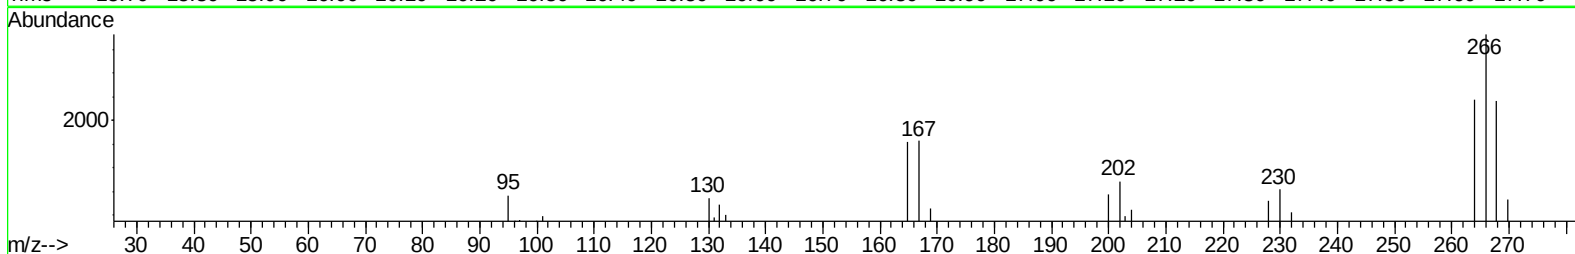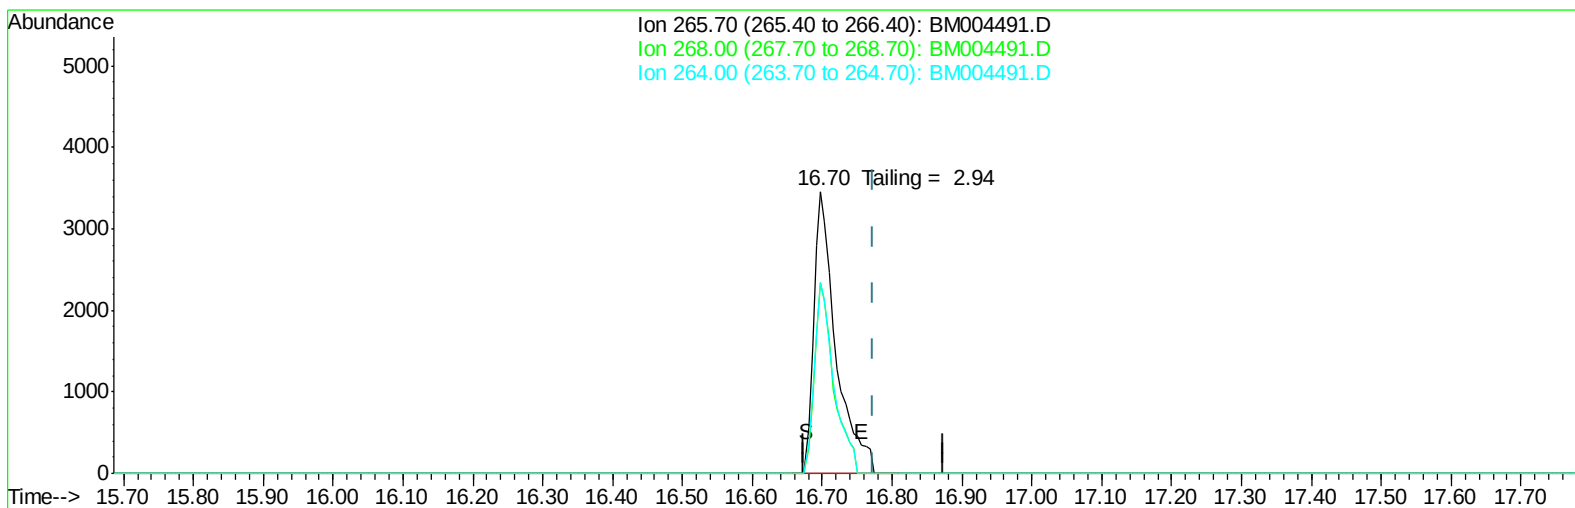

TIC: BM004491.D

(69) Pentachlorophenol (C)

16.698min (-0.076) 0.00ng




response 6795

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	67.67
264.00	61.20	67.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022916\
Data File : BM004491.D
Acq On : 01 Mar 2016 04:59
Operator : SJ/UM
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 01 08:08:37 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

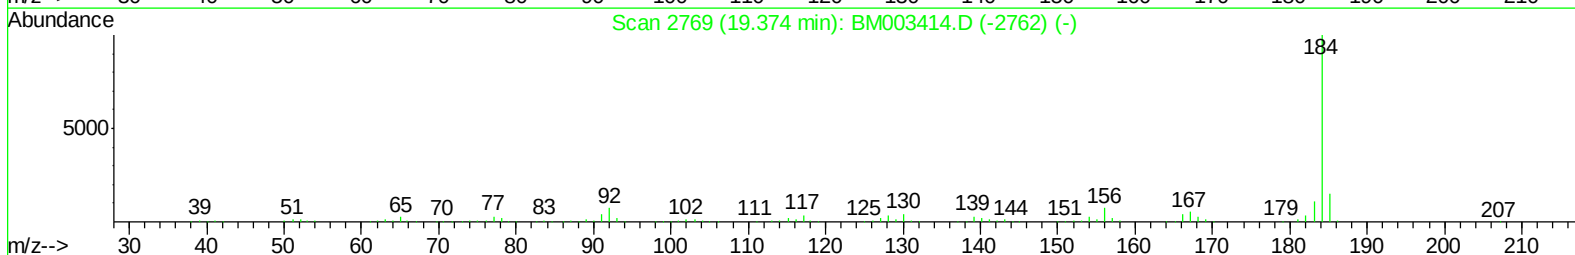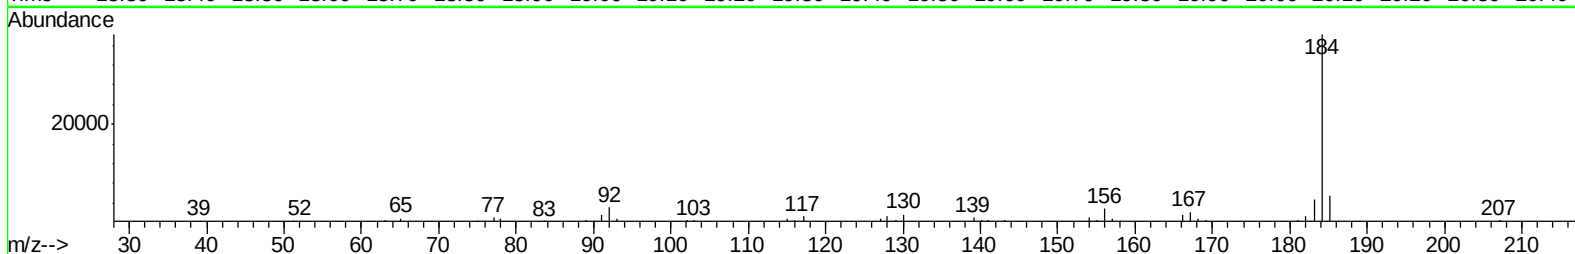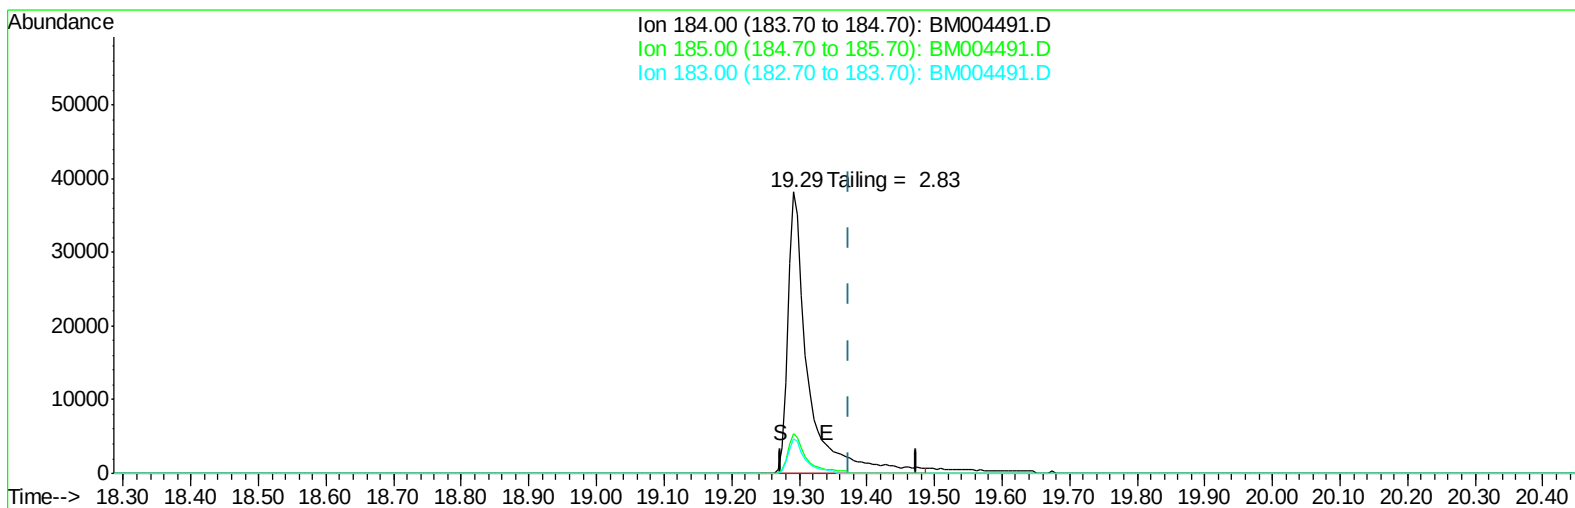

TIC: BM004491.D

(76) Benzidine

19.292min (-0.082) 0.00ng

response 55164

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.08
183.00	11.10	12.10
0.00	0.00	0.00