


Data Path : S:\HPCHEM1\BNA_M\DATA\BM022916\
 Data File : BM004474.D
 Acq On : 29 Feb 2016 16:56
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM022916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 01 00:52:28 2016

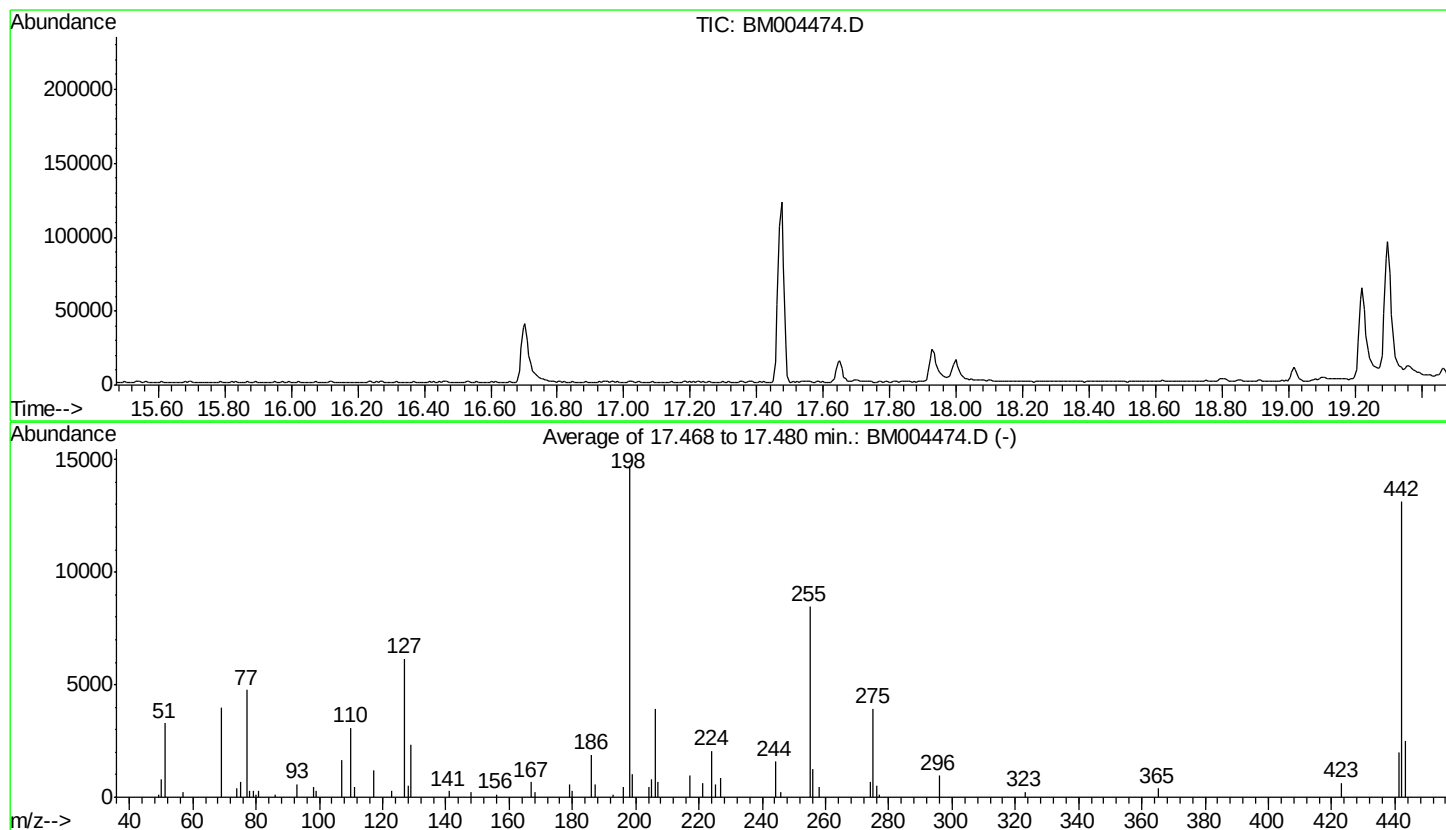

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.2	3277	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.0	3984	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.9	6168	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14735	PASS
199	198	5	9	6.9	1024	PASS
275	198	10	60	26.8	3953	PASS
365	198	1	100	2.7	397	PASS
441	442	0.01	24	15.4	2021	PASS
442	198	50	100	89.1	13124	PASS
443	442	15	24	19.2	2517	PASS