


Data Path : S:\HPCHEM1\BNA_M\DATA\BM022916\
 Data File : BM004491.D
 Acq On : 01 Mar 2016 04:59
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM022916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 01 00:52:28 2016

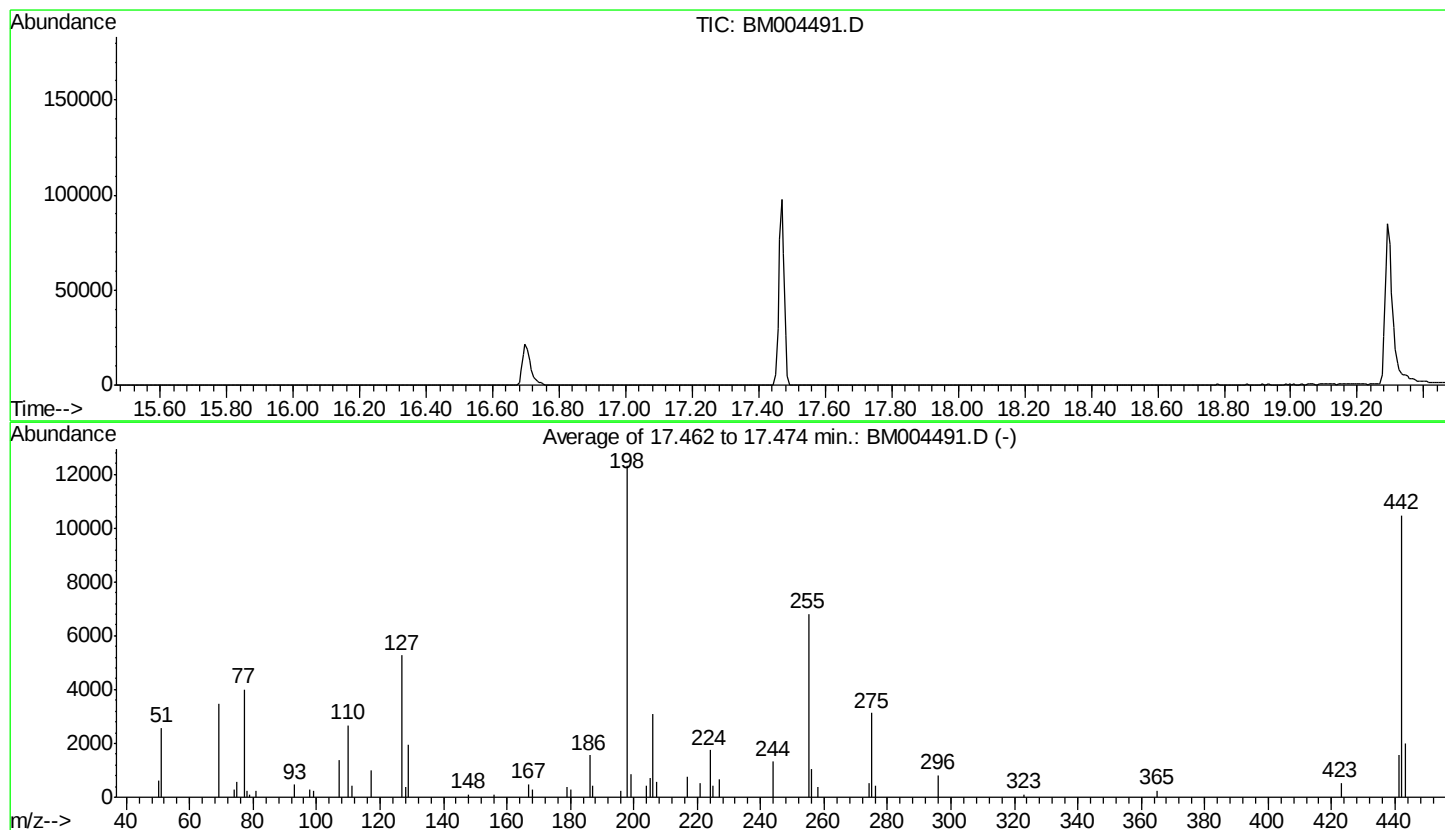

AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.9	2574	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.1	3459	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.8	5265	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12315	PASS
199	198	5	9	6.8	843	PASS
275	198	10	60	25.4	3122	PASS
365	198	1	100	2.1	253	PASS
441	442	0.01	24	15.2	1593	PASS
442	198	50	100	85.0	10468	PASS
443	442	15	24	19.0	1984	PASS