


Data Path : Z:\HPCHEM1\BNA M\Data\BM030116\
 Data File : BM004501.D
 Acq On : 01 Mar 2016 21:05
 Operator : SJ/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM030116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 02 16:18:56 2016

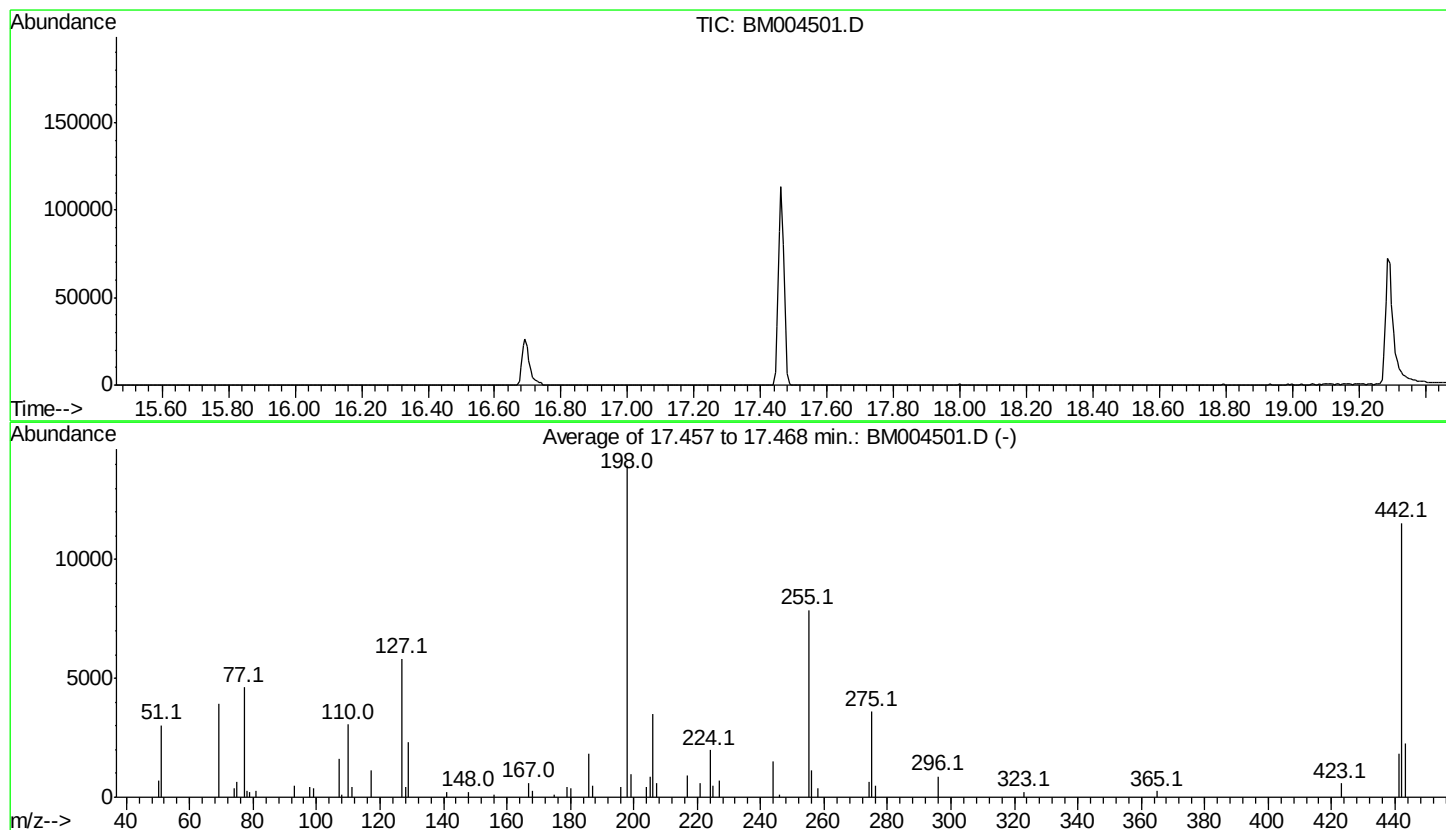

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.8	3043	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.0	3906	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	5828	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	13945	PASS
199	198	5	9	7.0	971	PASS
275	198	10	60	25.8	3597	PASS
365	198	1	100	1.9	258	PASS
441	442	0.01	24	15.7	1815	PASS
442	198	50	100	82.7	11534	PASS
443	442	15	24	19.4	2237	PASS