


Data Path : Z:\HPCHEM1\BNA M\DATA\BM030116\  
 Data File : BM004511.D  
 Acq On : 02 Mar 2016 09:34  
 Operator : SJ/UM  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-SIM-BM030116.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Mar 02 16:18:56 2016

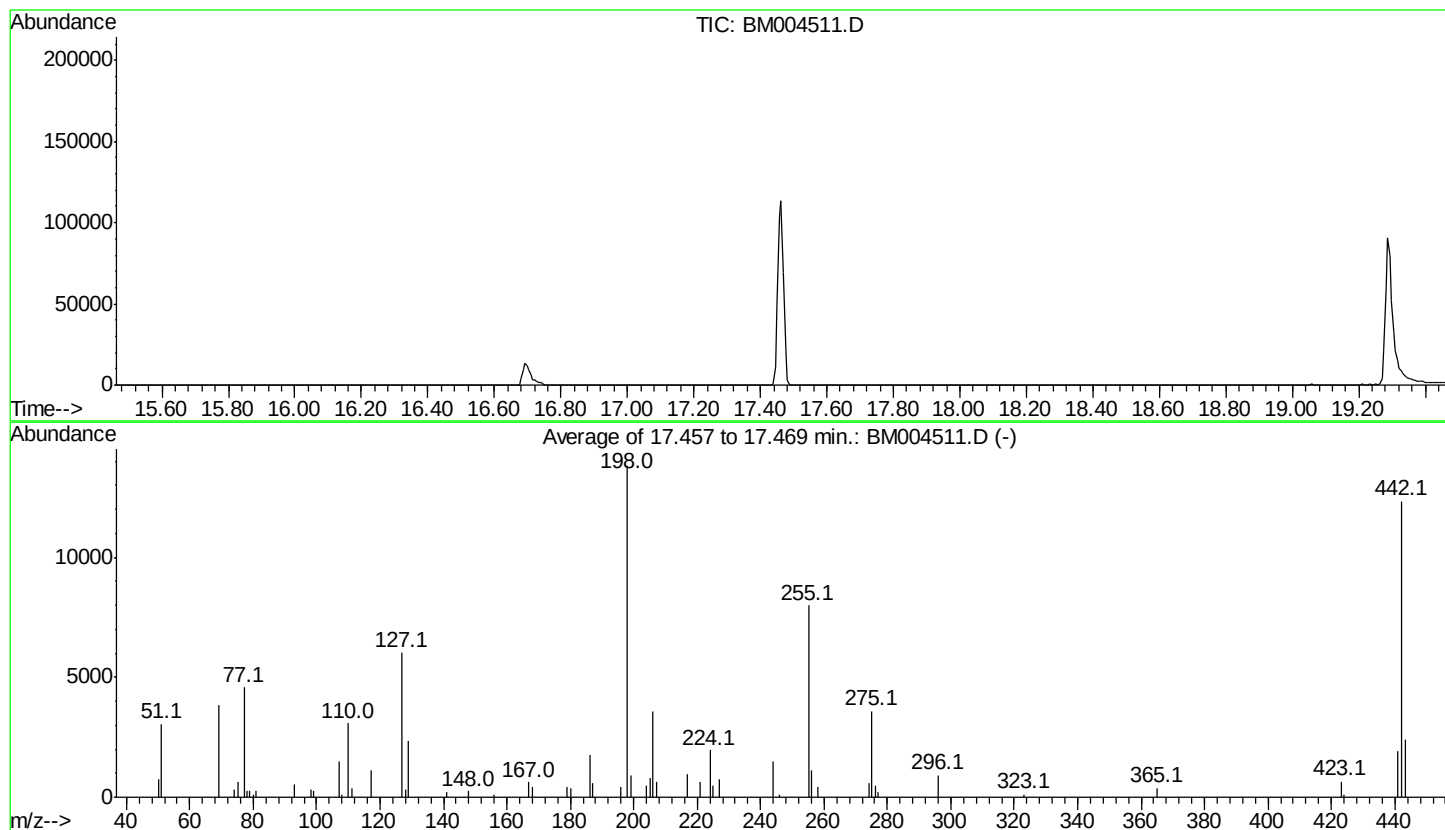

AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2505

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 22.1      | 3050    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 28.0      | 3868    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 43.6      | 6027    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 13824   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 916     | PASS             |
| 275         | 198          | 10           | 60           | 26.0      | 3593    | PASS             |
| 365         | 198          | 1            | 100          | 2.8       | 389     | PASS             |
| 441         | 442          | 0.01         | 24           | 15.7      | 1942    | PASS             |
| 442         | 198          | 50           | 100          | 89.3      | 12351   | PASS             |
| 443         | 442          | 15           | 24           | 19.4      | 2400    | PASS             |