

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
 Data File : BM009048.D
 Acq On : 01 Mar 2017 13:25
 Operator : SJ/MA
 Sample : I1988-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DABR9

Quant Time: Mar 02 03:23:16 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 03:22:17 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	148941	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	598535	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	357915	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	888315	20.00	ng/ul	0.00
75) Chrysene-d12	21.45	240	1269512	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1267400	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	15216	4.10	ng/uL	0.00
5) Phenol-d5	7.05	99	304371	22.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	227097	23.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.42	132	206706	22.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.59	113	218797	22.07	ng/ul	0.00
19) Nitrobenzene-d5	9.06	128	100998	23.58	ng/ul	0.00
22) 2-Nitrophenol-d4	9.78	143	106060	22.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.31	165	215201	22.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.84	131	235148	22.99	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	662132	27.48	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	817861	27.63	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	93987	22.33	ng/ul	0.00
57) Fluorene-d10	15.53	176	648421	28.82	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.64	200	94357	17.65	ng/ul	0.00
70) Anthracene-d10	17.38	188	1066847	25.36	ng/ul	0.00
76) Pyrene-d10	19.67	212	1340044	24.21	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.64	264	1500161	26.07	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.99	163	521234	21.62	ng/ul#	99
45) 2,6-Dinitrotoluene	13.99	165	5582	1.21	ng/ul#	25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
Data File : BM009048.D
Acq On : 01 Mar 2017 13:25
Operator : SJ/MA
Sample : I1988-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABR9

Quant Time: Mar 02 03:23:16 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 03:22:17 2017
Response via : Initial Calibration

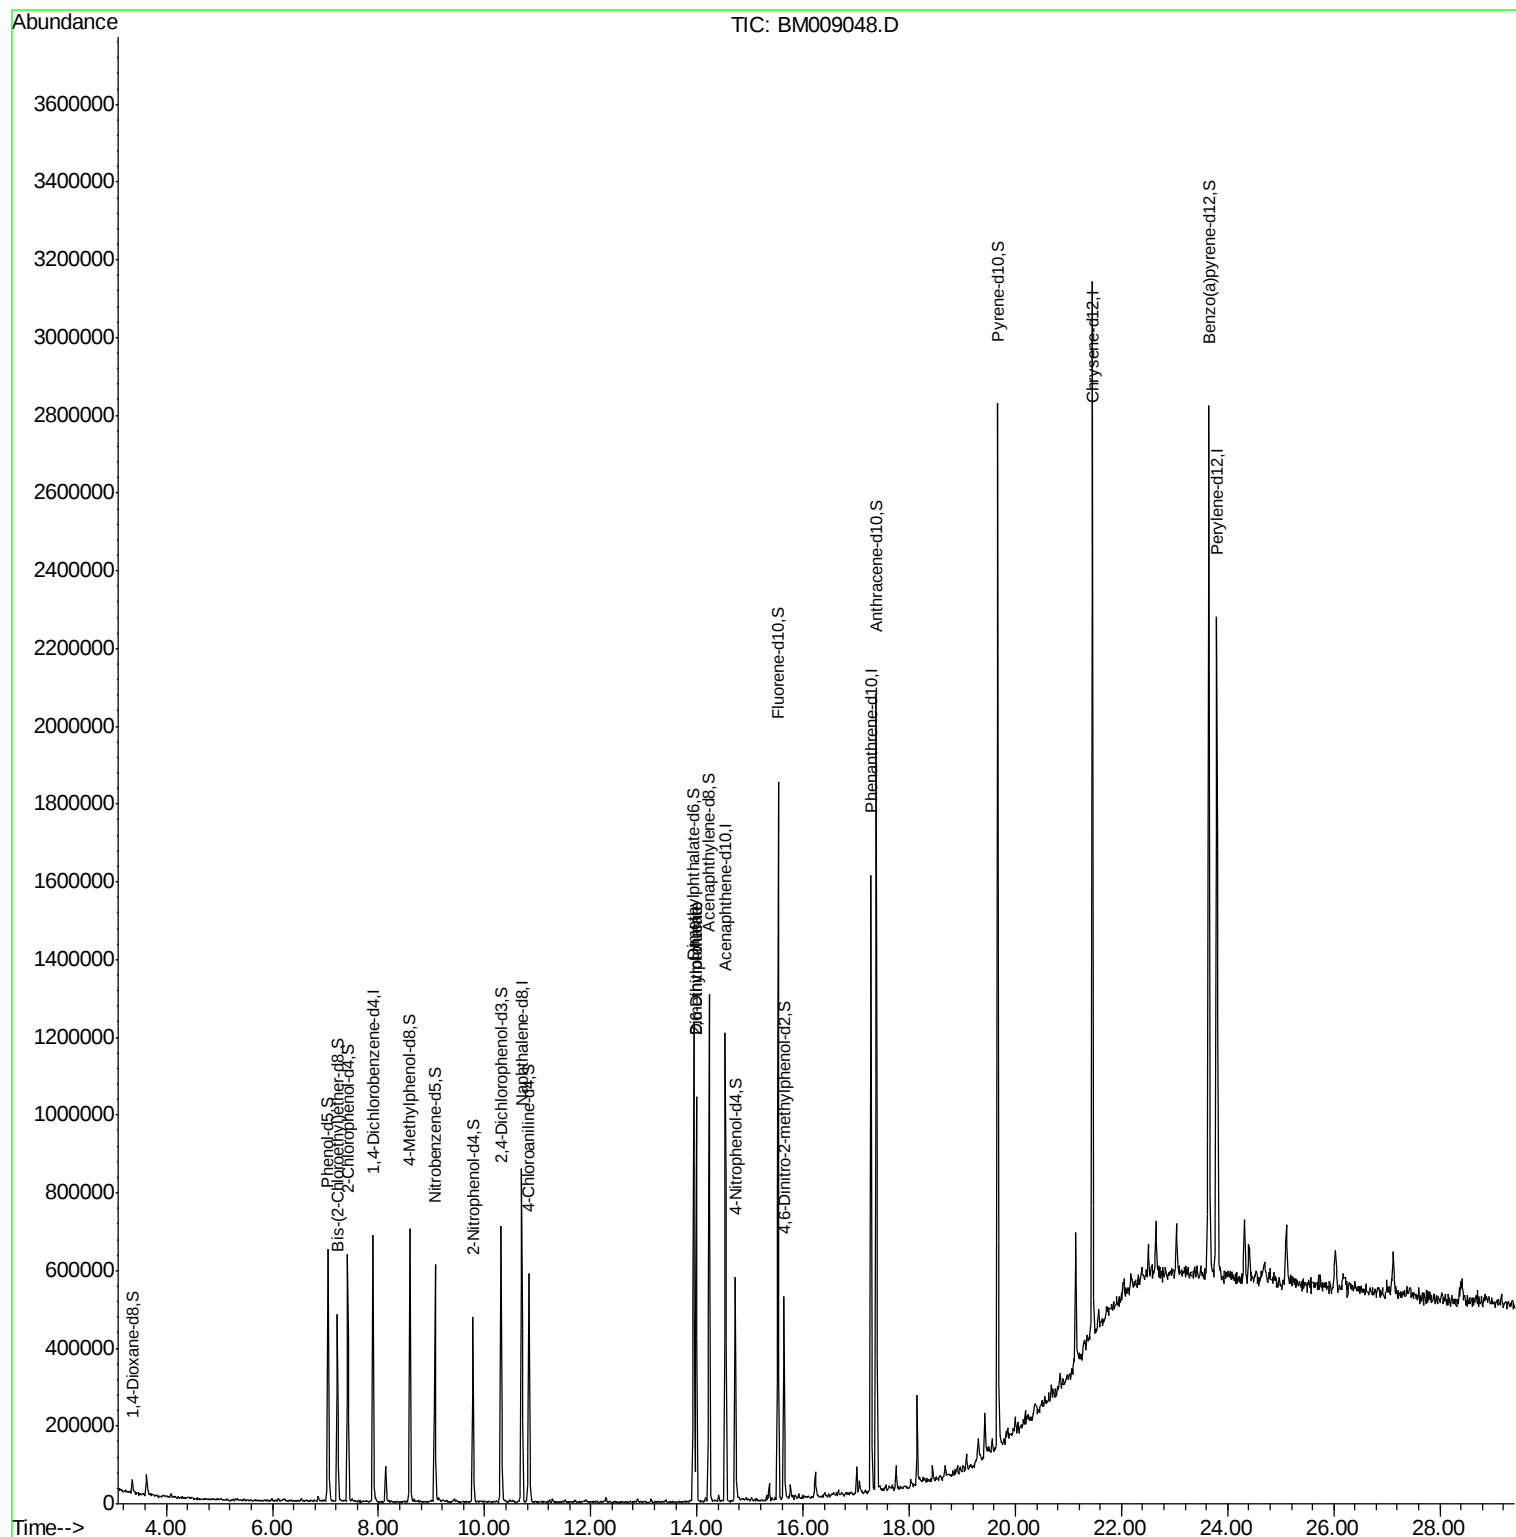

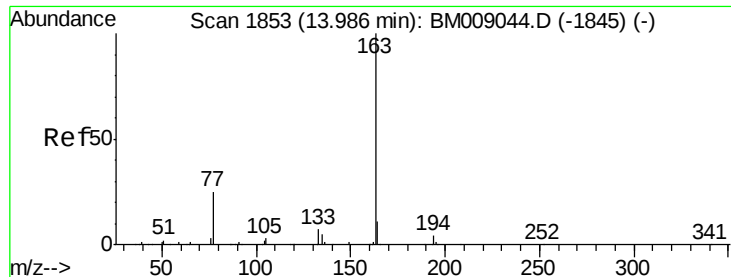

#44

Dimethylphthalate

Concen: 21.62 ng/ul

RT: 13.99 min Scan# 1853

Delta R.T. 0.00 min

Lab File: BM009048.D

Acq: 01 Mar 2017 13:25





Instrument :

BNA_M

ClientSampleId :

DABR9

Tgt Ion:	163	Resp:	521234
Ion	Ratio	Lower	Upper
163	100		
194	4.9	3.0	4.6#
164	10.8	8.6	12.8

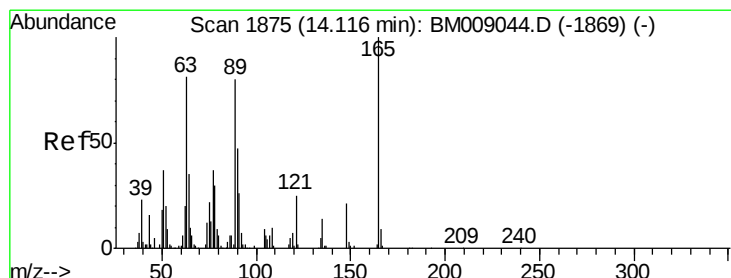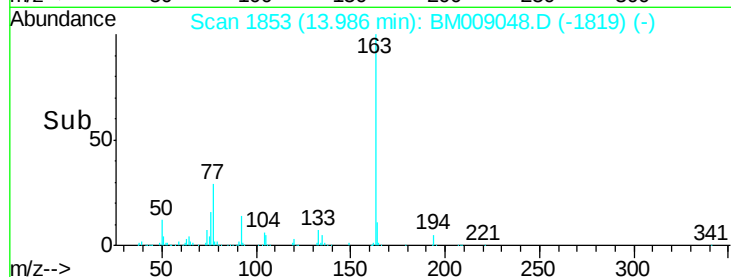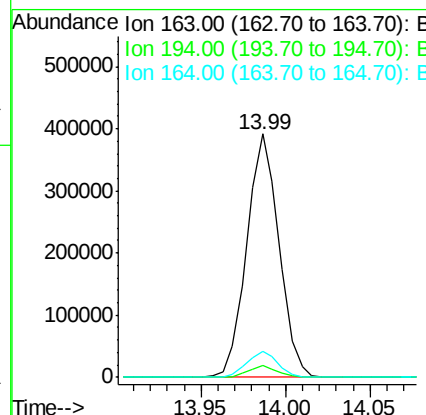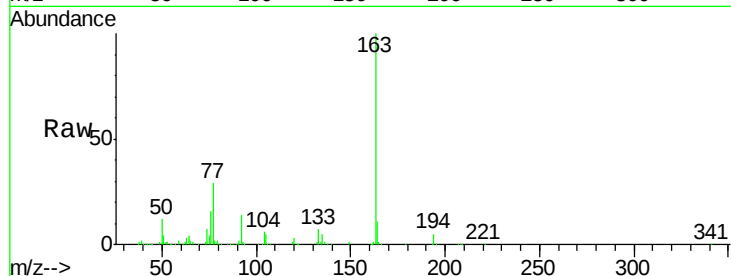

#45

2,6-Dinitrotoluene

Concen: 1.21 ng/ul

RT: 13.99 min Scan# 1853

Delta R.T. -0.13 min

Lab File: BM009048.D

Acq: 01 Mar 2017 13:25

Tgt Ion:	165	Resp:	5582
Ion	Ratio	Lower	Upper
165	100		
89	16.5	89.4	134.0#
121	19.9	21.6	32.4#

