

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
 Data File : BM009049.D
 Acq On : 01 Mar 2017 14:02
 Operator : SJ/MA
 Sample : I1988-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DABS0

Quant Time: Mar 02 03:23:24 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 03:22:17 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	161171	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	633351	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	391371	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	949050	20.00	ng/ul	0.00
75) Chrysene-d12	21.45	240	1249245	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1206489	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	17906	4.46	ng/uL	0.00
5) Phenol-d5	7.05	99	358026	24.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	275691	26.35	ng/ul	0.00
9) 2-Chlorophenol-d4	7.42	132	246647	25.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.59	113	254764	23.75	ng/ul	0.00
19) Nitrobenzene-d5	9.06	128	118559	26.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.78	143	122602	25.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.31	165	252355	24.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.83	131	309044	28.55	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	821712	31.19	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	994180	30.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	114756	24.94	ng/ul	0.00
57) Fluorene-d10	15.53	176	776036	31.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.64	200	114322	20.02	ng/ul	0.00
70) Anthracene-d10	17.38	188	1268842	28.24	ng/ul	0.00
76) Pyrene-d10	19.67	212	1530440	28.10	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.64	264	1581079	28.86	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.99	163	549405	20.84	ng/ul	98
45) 2,6-Dinitrotoluene	13.99	165	7069	1.41	ng/ul#	25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
Data File : BM009049.D
Acq On : 01 Mar 2017 14:02
Operator : SJ/MA
Sample : I1988-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABS0

Quant Time: Mar 02 03:23:24 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 03:22:17 2017
Response via : Initial Calibration

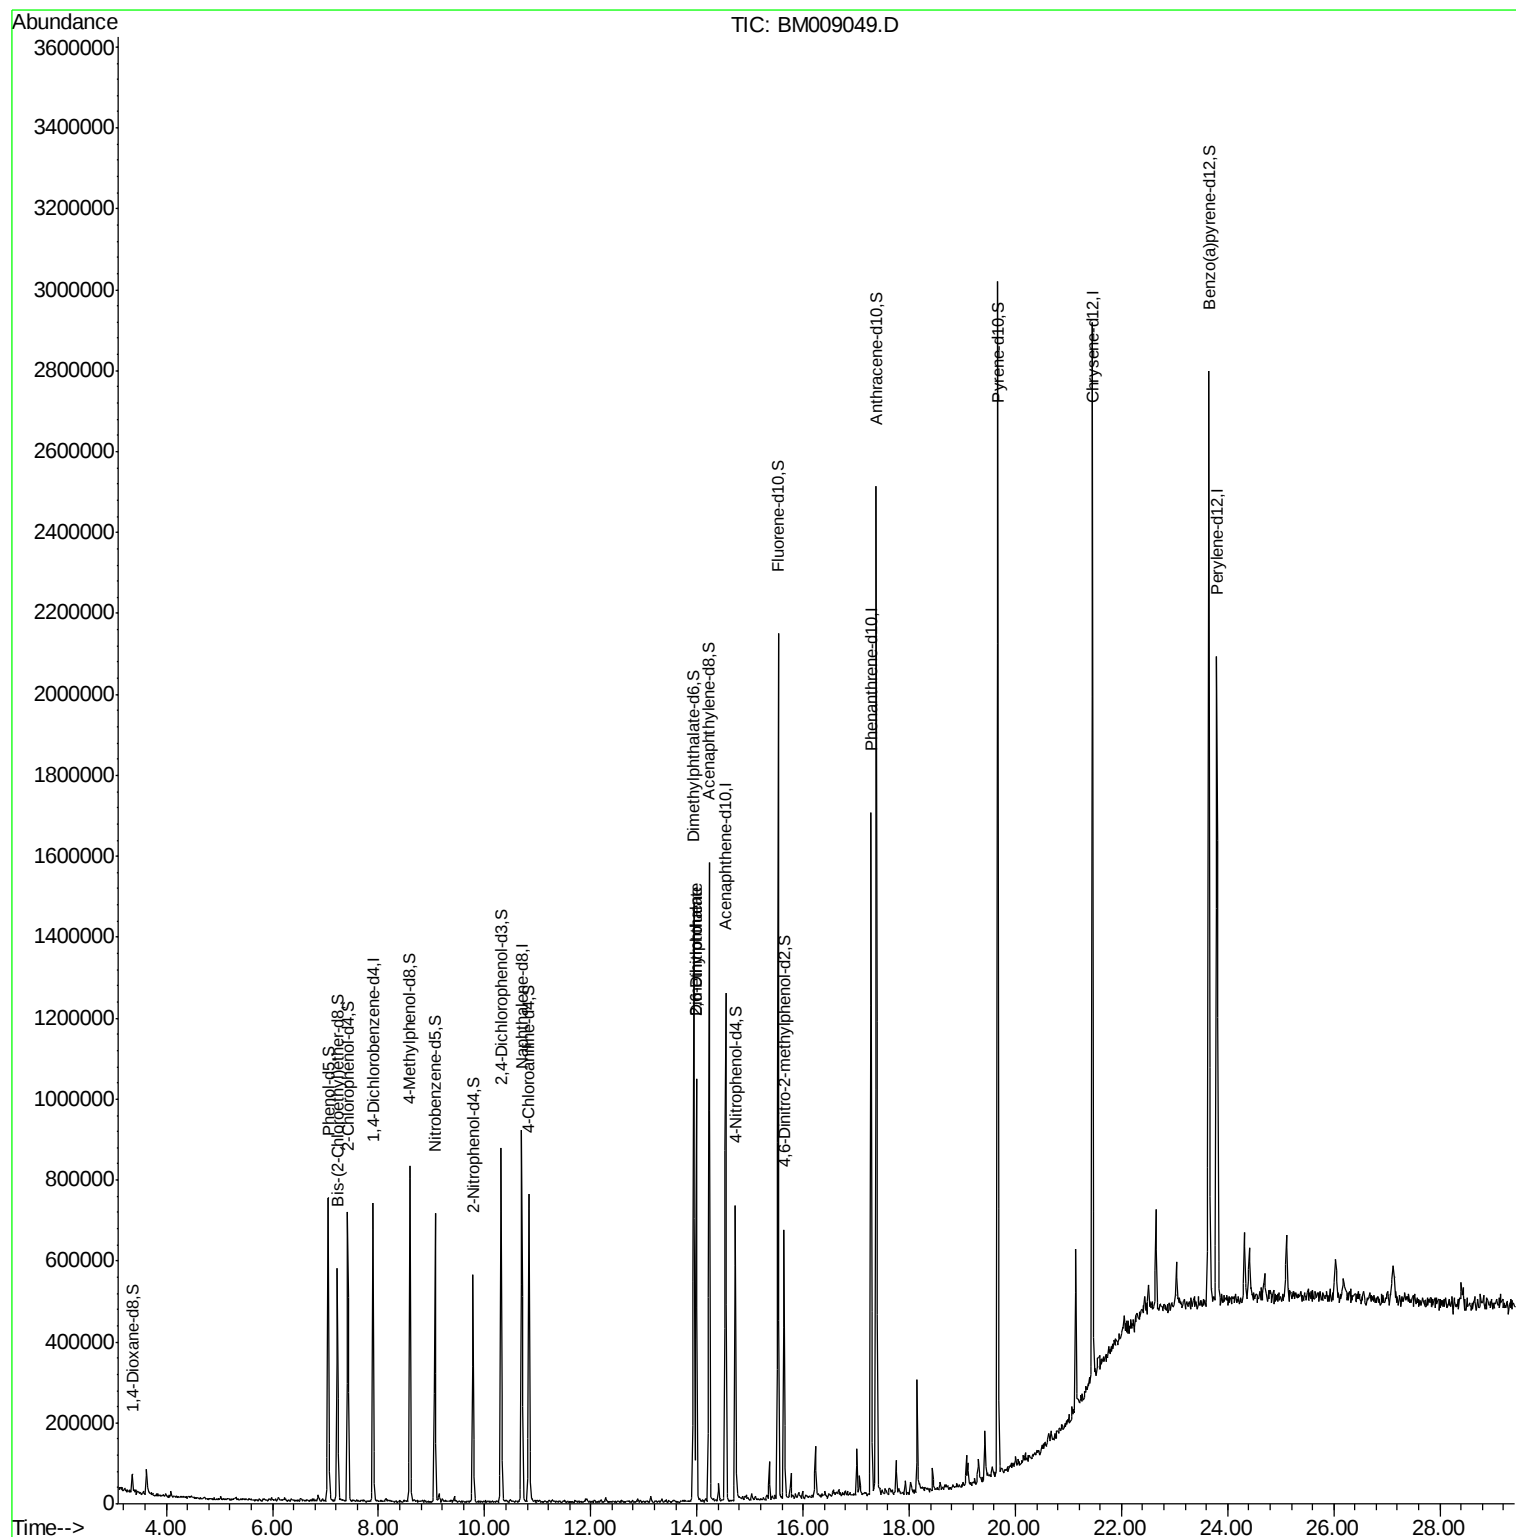

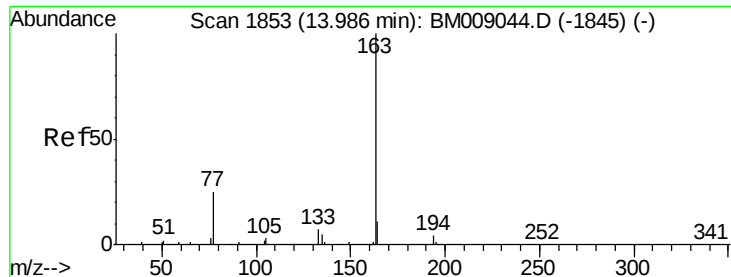

#44

Dimethylphthalate

Concen: 20.84 ng/ul

RT: 13.99 min Scan# 1853

Delta R.T. -0.00 min

Lab File: BM009049.D

Acq: 01 Mar 2017 14:02





Instrument :

BNA_M

ClientSampleId :

DABS0

Tgt Ion:	163	Resp:	549405
Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.0	4.6
164	9.7	8.6	12.8

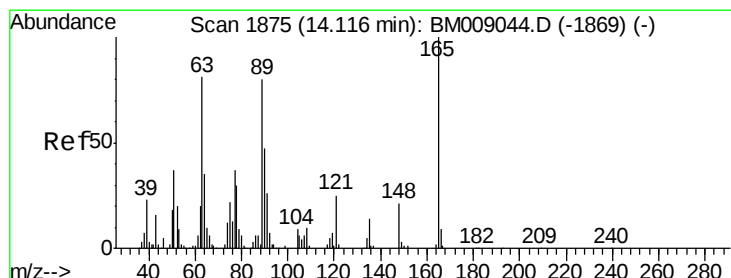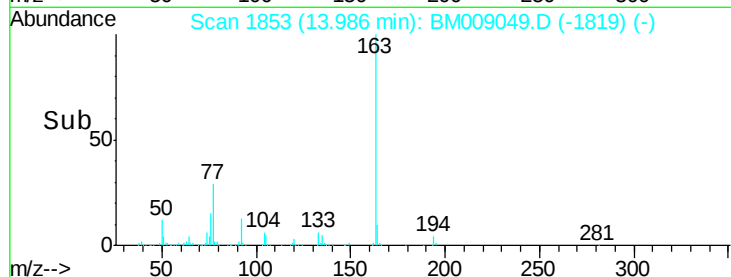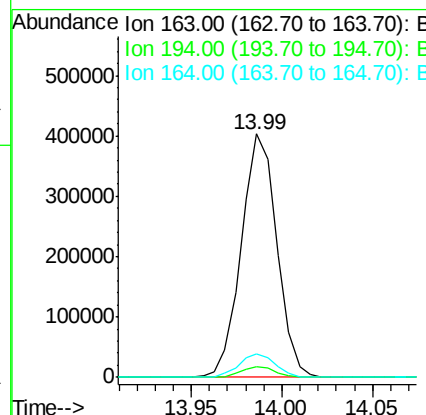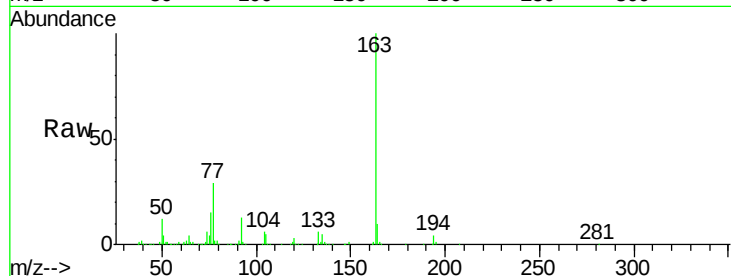

#45

2,6-Dinitrotoluene

Concen: 1.41 ng/ul

RT: 13.99 min Scan# 1853

Delta R.T. -0.13 min

Lab File: BM009049.D

Acq: 01 Mar 2017 14:02

Tgt Ion:	165	Resp:	7069
Ion	Ratio	Lower	Upper
165	100		
89	15.6	89.4	134.0#
121	19.5	21.6	32.4#

