

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
 Data File : BM009050.D
 Acq On : 01 Mar 2017 14:39
 Operator : SJ/MA
 Sample : I1988-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DABS3

Quant Time: Mar 02 03:23:32 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 03:22:17 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	164152	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	622637	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.54	164	365766	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	870566	20.00	ng/ul	0.00
75) Chrysene-d12	21.45	240	1092148	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1034025	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.36	96	18474	4.52	ng/uL	0.00
5) Phenol-d5	7.05	99	324781	21.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	243967	22.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.42	132	227094	22.91	ng/ul	0.00
13) 4-Methylphenol-d8	8.59	113	230342	21.08	ng/ul	0.00
19) Nitrobenzene-d5	9.06	128	105326	23.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.78	143	115053	23.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.31	165	224144	22.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.83	131	275338	25.88	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	704361	28.60	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	854859	28.26	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	94239	21.91	ng/ul	0.00
57) Fluorene-d10	15.53	176	658212	28.63	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.65	200	90328	17.24	ng/ul	0.00
70) Anthracene-d10	17.38	188	1047282	25.41	ng/ul	0.00
76) Pyrene-d10	19.67	212	1249184	26.24	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.65	264	1236901	26.35	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.99	163	485544	19.70	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
Data File : BM009050.D
Acq On : 01 Mar 2017 14:39
Operator : SJ/MA
Sample : I1988-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABS3

Quant Time: Mar 02 03:23:32 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 03:22:17 2017
Response via : Initial Calibration

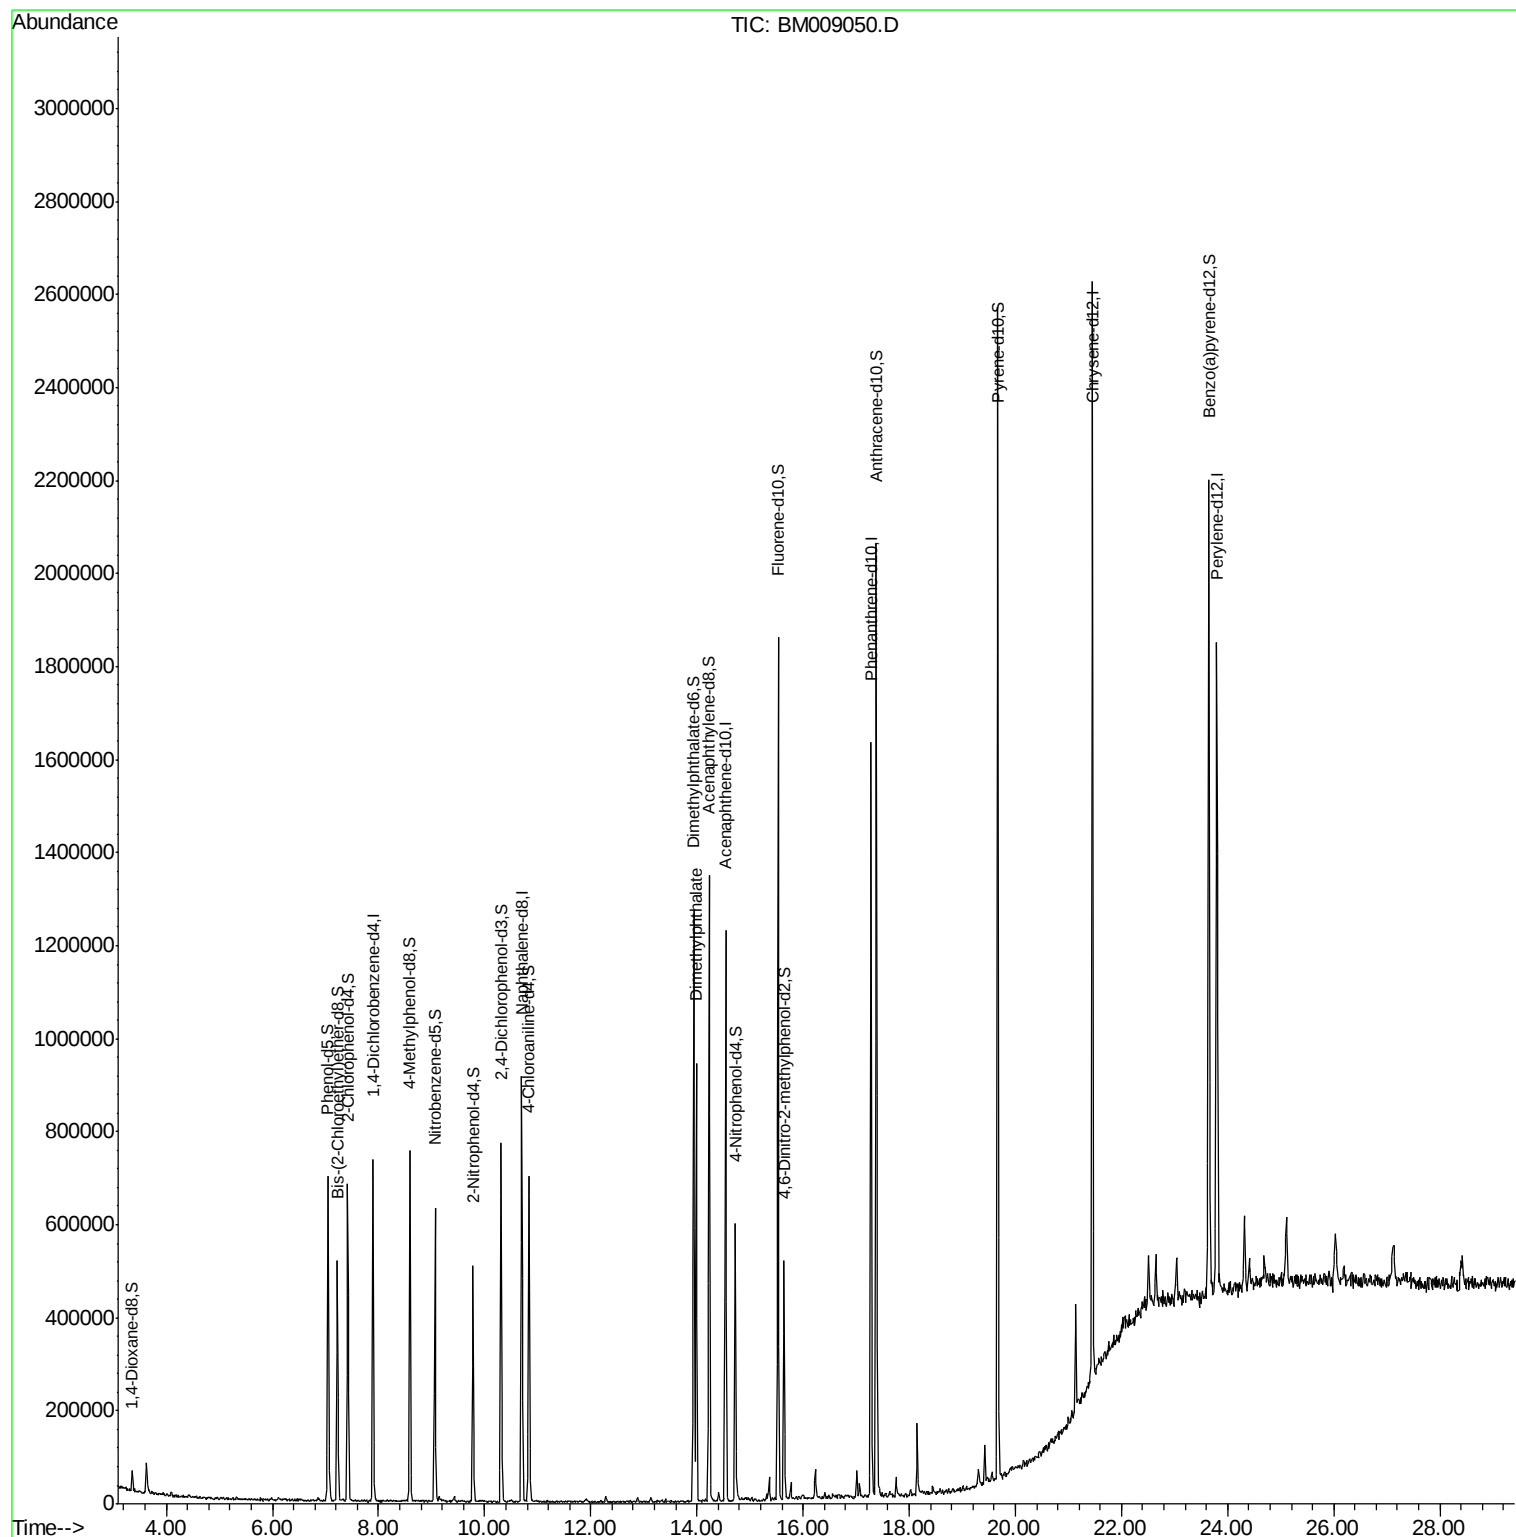

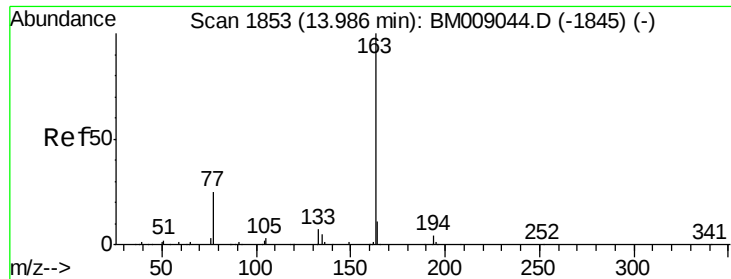

#44
 Dimethylphthalate
 Concen: 19.70 ng/ul
 RT: 13.99 min Scan# 1853
 Delta R.T. 0.00 min
 Lab File: BM009050.D
 Acq: 01 Mar 2017 14:39

Instrument :
 BNA_M
 ClientSampleId :
 DABS3

Tgt Ion:	163	Resp:	485544
Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.0	4.6
164	10.3	8.6	12.8

