

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
 Data File : BM009058.D
 Acq On : 01 Mar 2017 19:34
 Operator : SJ/MA
 Sample : I1988-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DABS8

Quant Time: Mar 02 03:55:54 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 03:54:18 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.90	152	178891	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	693673	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.53	164	418399	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.28	188	975270	20.00	ng/ul	0.00
75) Chrysene-d12	21.45	240	1224423	20.00	ng/ul	0.00
83) Perylene-d12	23.80	264	1179631	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.36	96	19749	4.43	ng/uL	0.00
5) Phenol-d5	7.05	99	369325	22.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.23	67	285809	24.61	ng/ul	0.00
9) 2-Chlorophenol-d4	7.42	132	260625	24.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.59	113	252745	21.23	ng/ul	0.00
19) Nitrobenzene-d5	9.06	128	117418	23.66	ng/ul	0.00
22) 2-Nitrophenol-d4	9.78	143	126094	23.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.31	165	257477	22.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.83	131	253441	21.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.94	166	797068	28.30	ng/ul	0.00
46) Acenaphthylene-d8	14.23	160	1001170	28.94	ng/ul	0.00
51) 4-Nitrophenol-d4	14.72	143	108306	22.02	ng/ul	0.00
57) Fluorene-d10	15.53	176	767252	29.17	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.64	200	103331	17.61	ng/ul	0.00
70) Anthracene-d10	17.38	188	1245075	26.96	ng/ul	0.00
76) Pyrene-d10	19.67	212	1492864	27.97	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.65	264	1476796	27.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.99	163	413274	14.66	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM030117\
Data File : BM009058.D
Acq On : 01 Mar 2017 19:34
Operator : SJ/MA
Sample : I1988-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABS8

Quant Time: Mar 02 03:55:54 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 03:54:18 2017
Response via : Initial Calibration

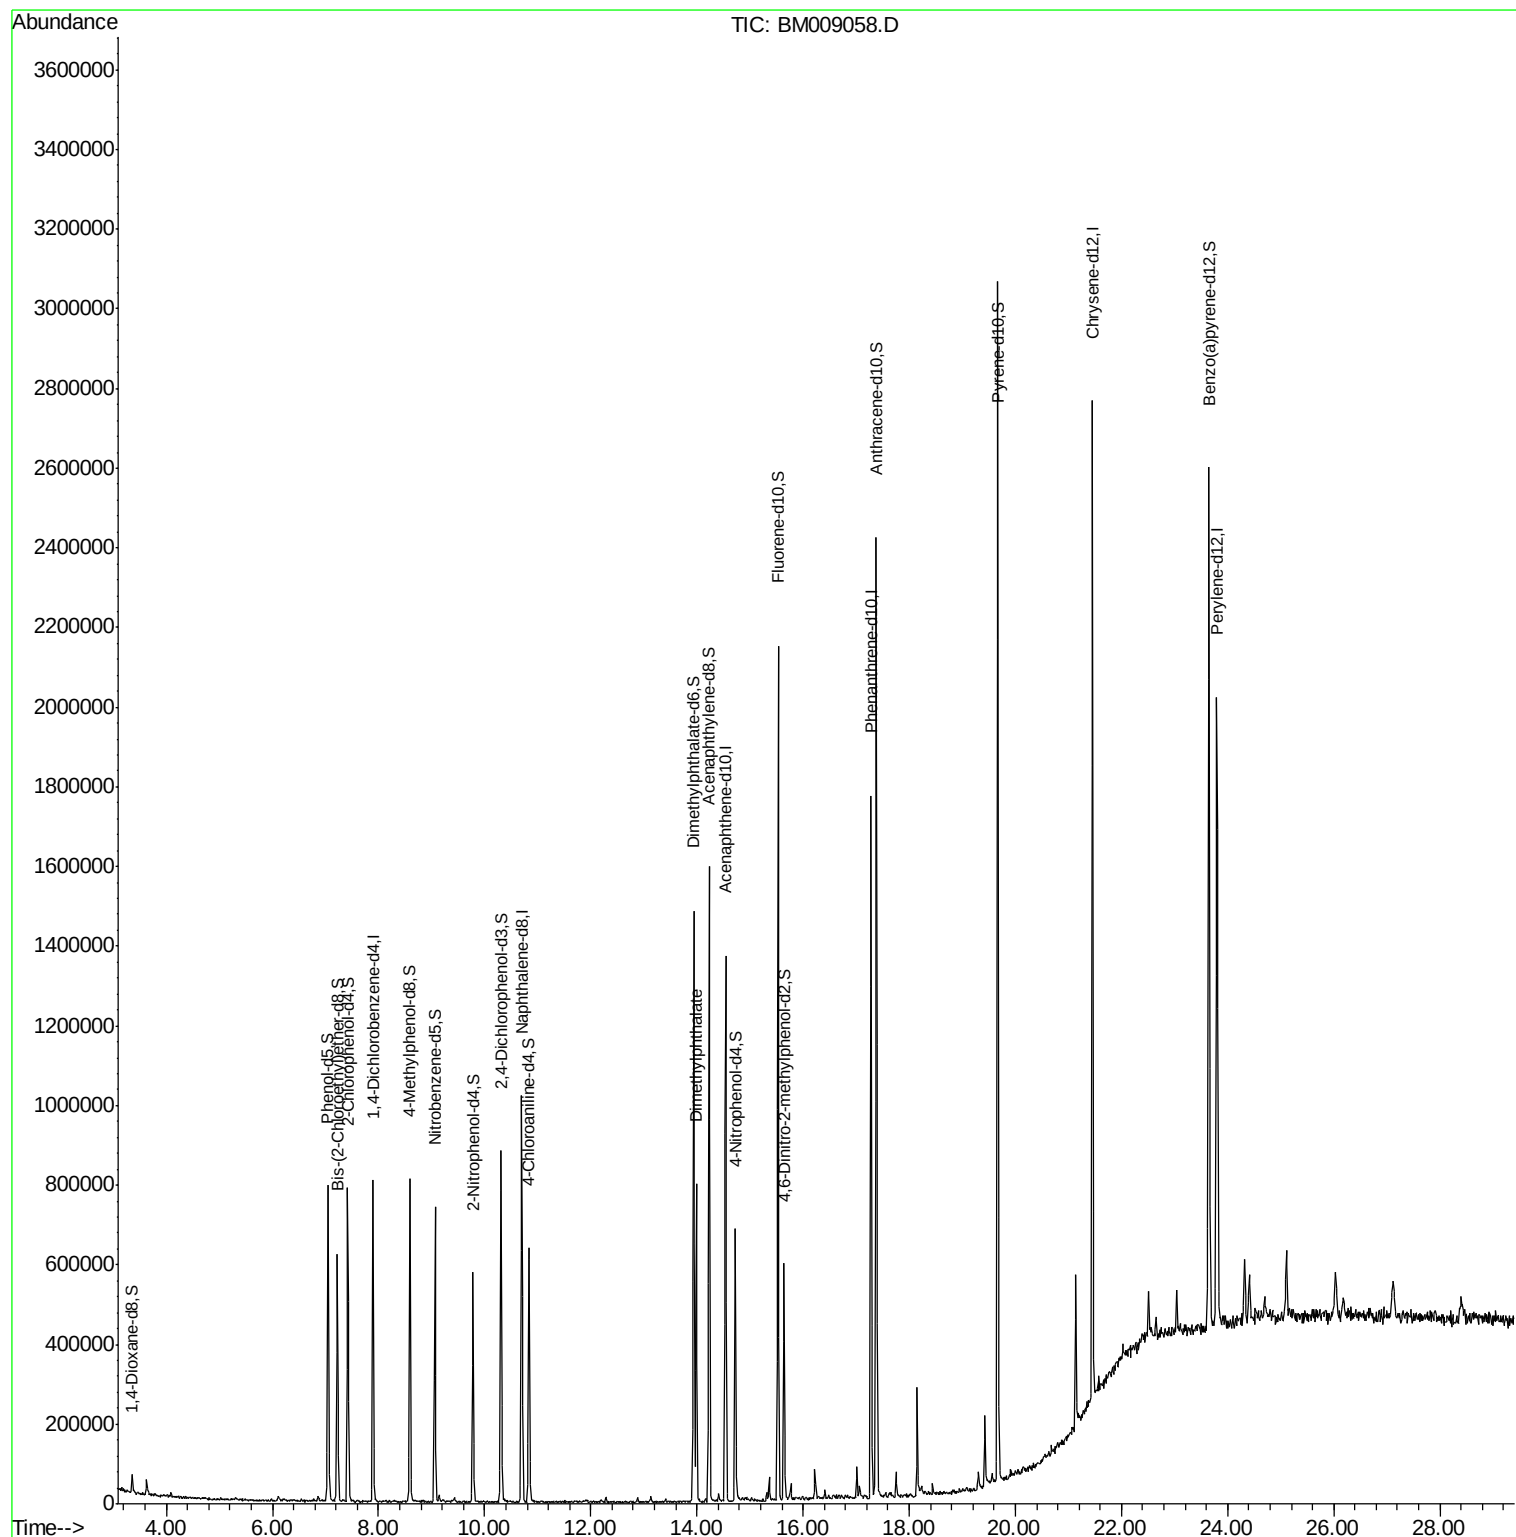

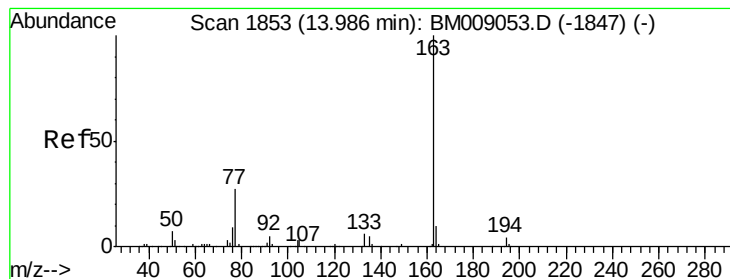

#44

Dimethylphthalate

Concen: 14.66 ng/ul

RT: 13.99 min Scan# 1853

Delta R.T. 0.00 min

Lab File: BM009058.D

Acq: 01 Mar 2017 19:34

Instrument :

BNA_M

ClientSampleId :

DABS8


Tgt Ion:163 Resp: 413274

Ion Ratio Lower Upper

163 100

194 4.9 3.0 4.6#

164 11.6 8.6 12.8

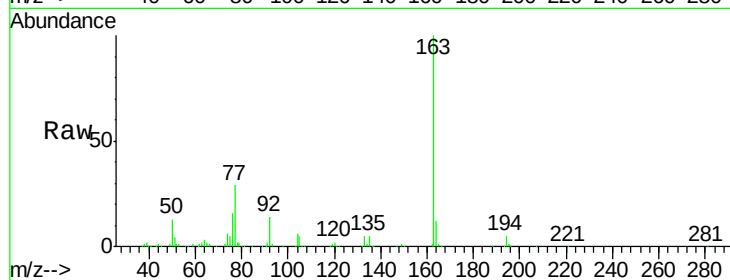

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

